




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023717.D
 Acq On : 14 Jul 2022 22:09
 Operator : SY/VA
 Sample : N3700-06
 Misc : 6.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C13

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:46:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

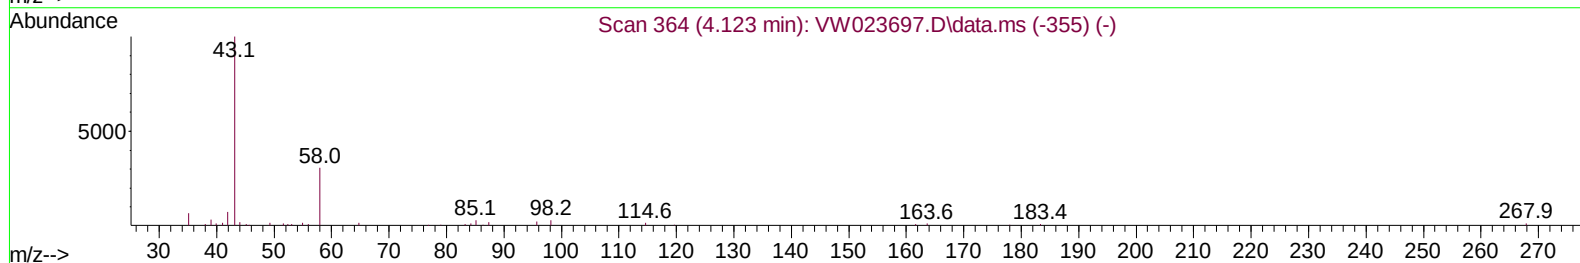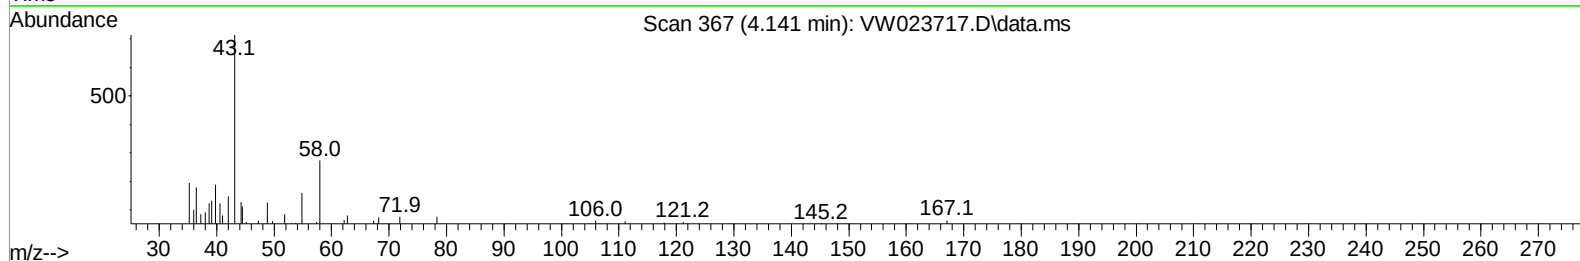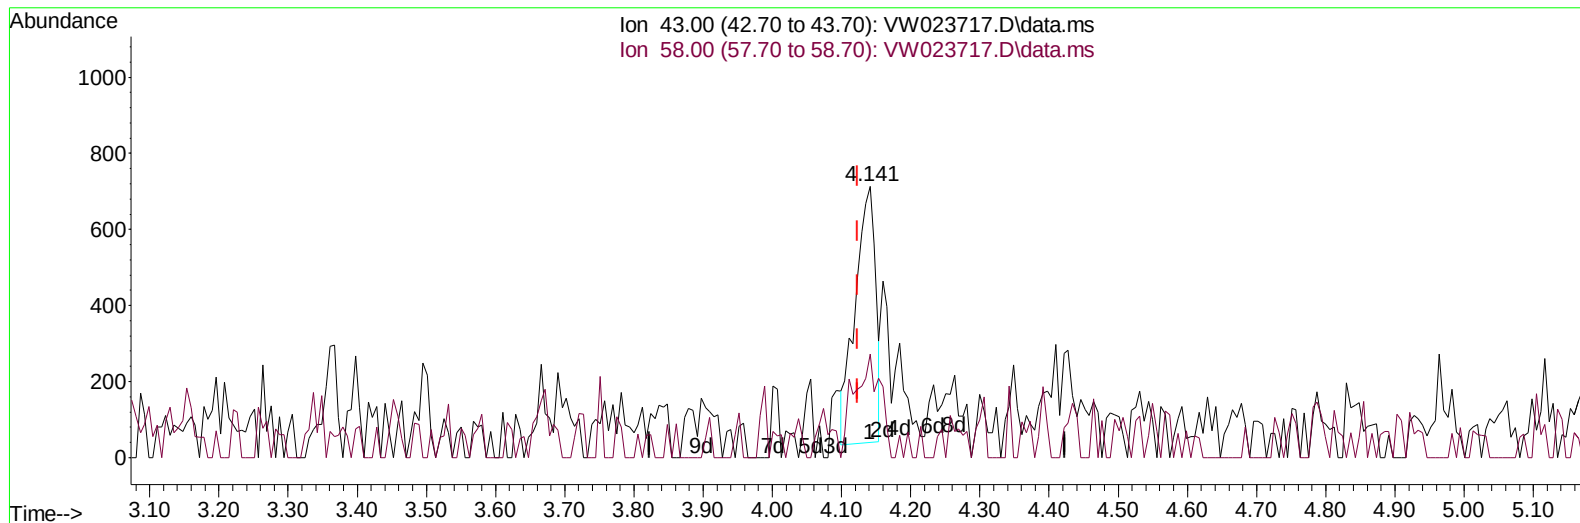

TIC: VW023717.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 21.64 ug/L

response 1390

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	17.19
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023717.D
 Acq On : 14 Jul 2022 22:09
 Operator : SY/VA
 Sample : N3700-06
 Misc : 6.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C13

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:46:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

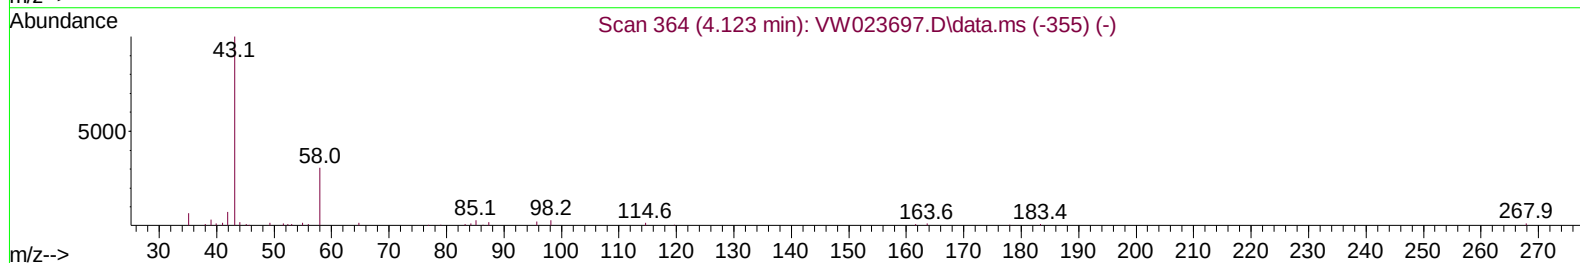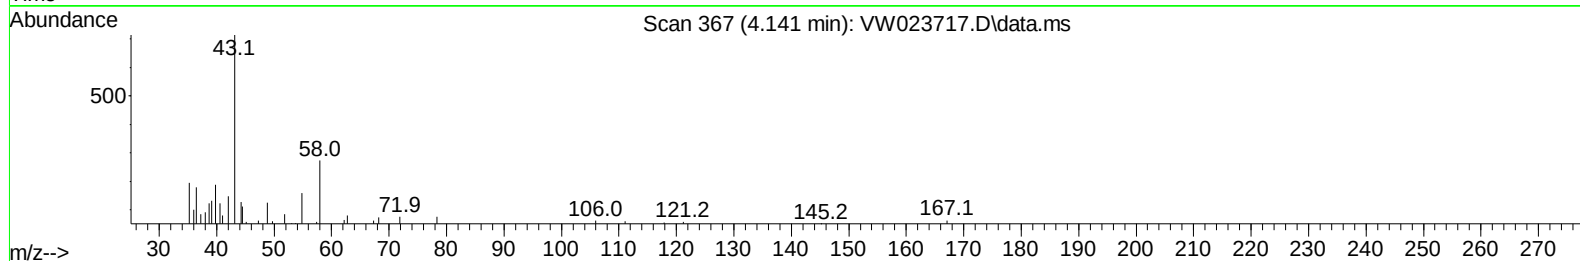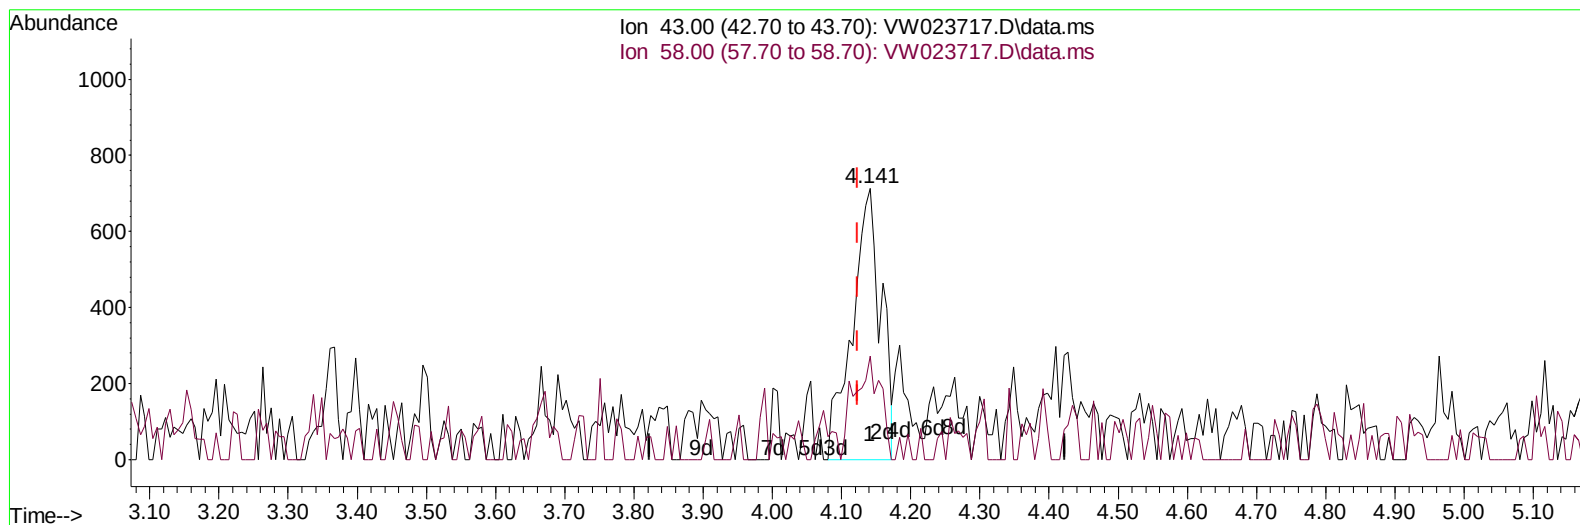

TIC: VW023717.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 32.15 ug/L m

response 2065

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	11.57
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023717.D
 Acq On : 14 Jul 2022 22:09
 Operator : SY/VA
 Sample : N3700-06
 Misc : 6.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C13

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:46:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		22932	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117		20910	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		7390	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		17414	29.732	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	118.920%	
7) Chloroethane-d5	2.879	69		16466	42.141	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	168.560%#	
11) 1,1-Dichloroethene-d2	4.013	63		11105	23.284	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	93.120%	
21) 2-Butanone-d5	7.080	46		5097	56.104	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.200%	
24) Chloroform-d	7.647	84		17881	26.782	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	107.120%	
26) 1,2-Dichloroethane-d4	8.305	65		10039	24.585	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.320%	
32) Benzene-d6	8.281	84		28797	26.493	ug/L	0.01
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.960%	
36) 1,2-Dichloropropane-d6	9.268	67		9626	29.400	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	117.600%	
41) Toluene-d8	10.323	98		21905	19.868	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.480%	
43) trans-1,3-Dichloroprop...	10.573	79		2549	16.609	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.440%	
47) 2-Hexanone-d5	10.927	63		2507	36.413	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.820%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		8376	23.149	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.600%	
66) 1,2-Dichlorobenzene-d4	13.847	152		6065	22.990	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.960%	
Target Compounds							
13) Acetone	4.141	43		2065m	32.150	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023717.D
Acq On : 14 Jul 2022 22:09
Operator : SY/VA
Sample : N3700-06
Misc : 6.42g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C13

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 03:46:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 03:40:01 2022
Response via : Initial Calibration

