




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023718.D
 Acq On : 14 Jul 2022 22:34
 Operator : SY/VA
 Sample : N3700-07
 Misc : 5.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C14

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:46:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

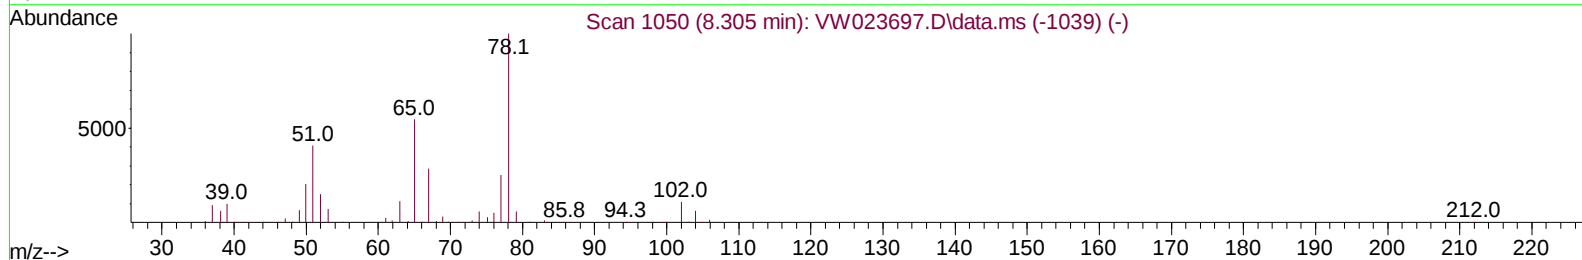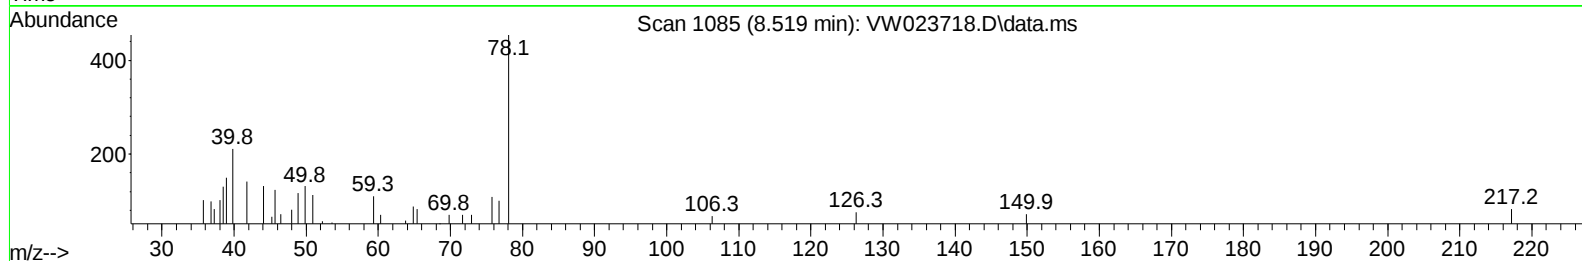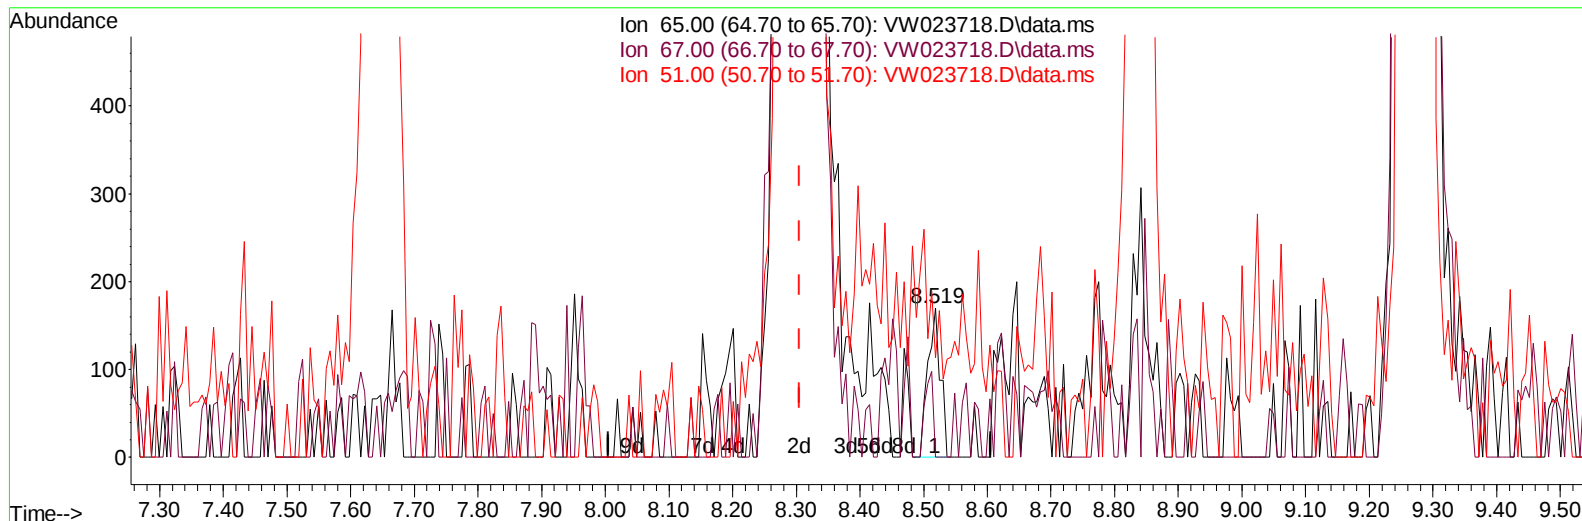

TIC: VW023718.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.519min (+ 0.213) 0.07 ug/L

response 236

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	37.29
51.00	92.20	94.07
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023718.D
 Acq On : 14 Jul 2022 22:34
 Operator : SY/VA
 Sample : N3700-07
 Misc : 5.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C14

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:46:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

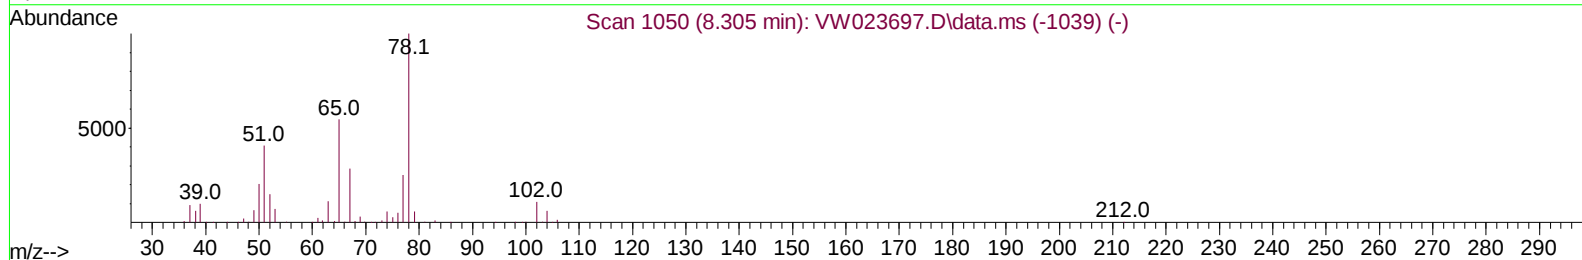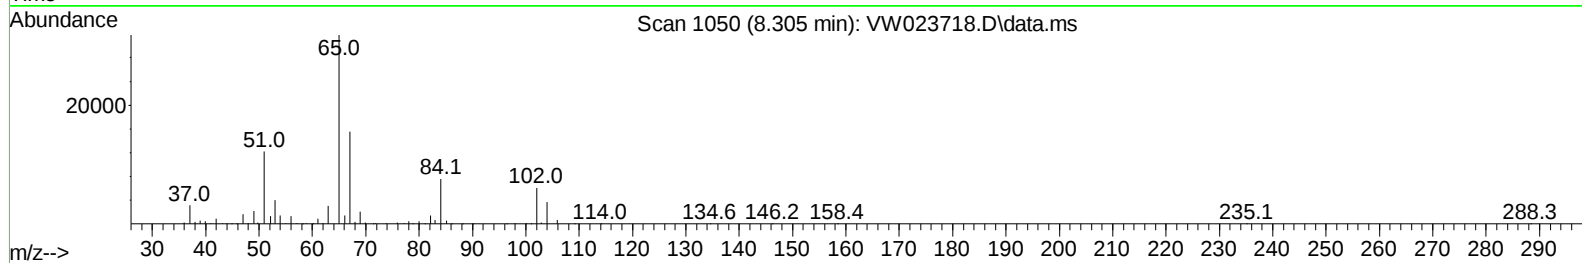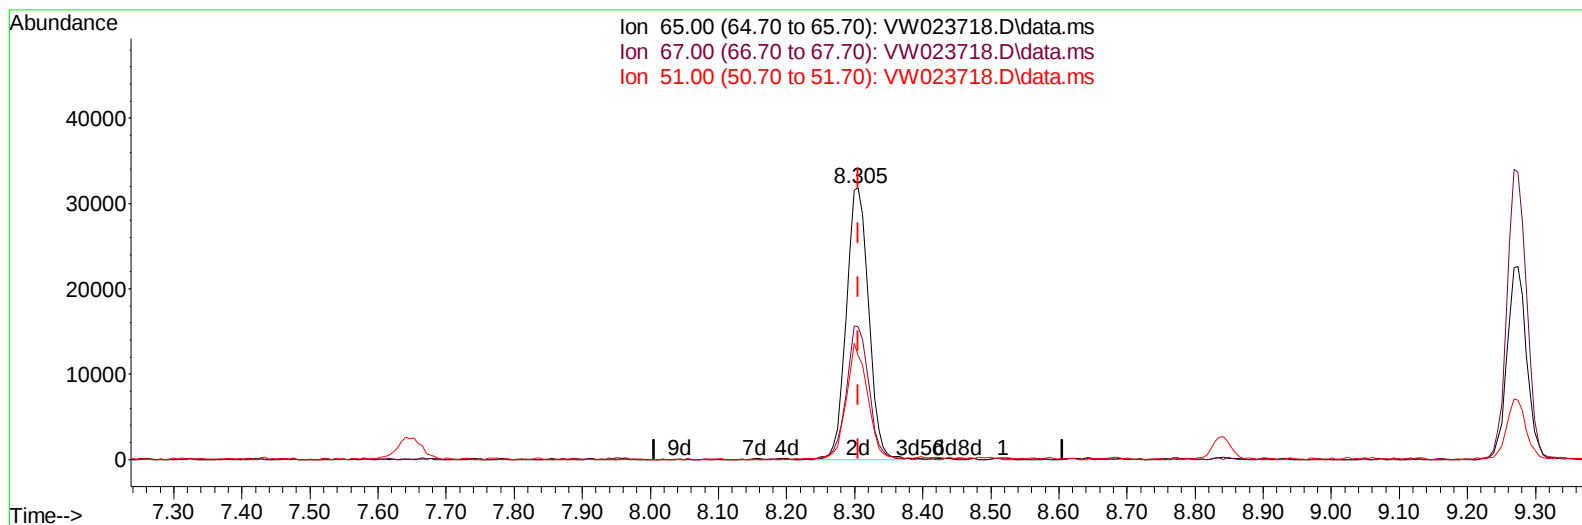

TIC: VW023718.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 21.89 ug/L m

response 72163

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.12#
51.00	92.20	0.31#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023718.D
 Acq On : 14 Jul 2022 22:34
 Operator : SY/VA
 Sample : N3700-07
 Misc : 5.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C14

Manual IntegrationsAPPROVED

Quant Time: Jul 15 03:46:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	185138	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	174827	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	71708	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	94940	20.078	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	80.320%	
7) Chloroethane-d5	2.879	69	73049	23.157	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	92.640%	
11) 1,1-Dichloroethene-d2	4.013	63	47848	12.427	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	49.720%	
21) 2-Butanone-d5	7.080	46	33680	45.920	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.840%	
24) Chloroform-d	7.647	84	118722	22.025	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.120%	
26) 1,2-Dichloroethane-d4	8.305	65	72163m	21.889	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	87.560%	
32) Benzene-d6	8.275	84	209550	23.058	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	92.240%	
36) 1,2-Dichloropropane-d6	9.268	67	68466	25.010	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	100.040%	
41) Toluene-d8	10.323	98	192467	20.879	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	83.520%	
43) trans-1,3-Dichloroprop...	10.579	79	21894	17.062	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	68.240%	
47) 2-Hexanone-d5	10.921	63	26342	45.761	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.520%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	63801	21.089	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	84.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	59392	23.202	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.800%	
Target Compounds						
					Qvalue	
13) Acetone	4.123	43	8657	16.694	ug/L	94
14) Carbon disulfide	4.385	76	14832	2.569	ug/L #	95
42) Toluene	10.384	91	10868	0.959	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023718.D
Acq On : 14 Jul 2022 22:34
Operator : SY/VA
Sample : N3700-07
Misc : 5.21g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C14

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 03:46:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 03:40:01 2022
Response via : Initial Calibration

