




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023725.D
 Acq On : 15 Jul 2022 04:26
 Operator : SY/VA
 Sample : N3700-11
 Misc : 4.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C18

Manual IntegrationsAPPROVED

Quant Time: Jul 15 06:30:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

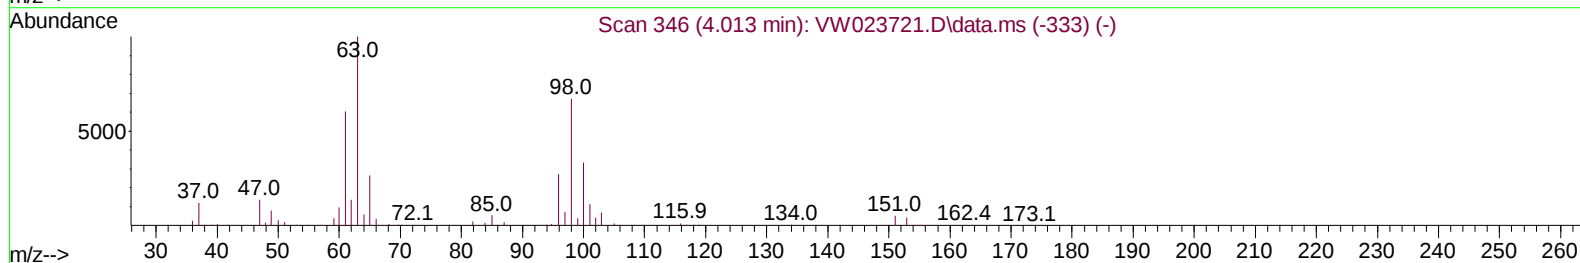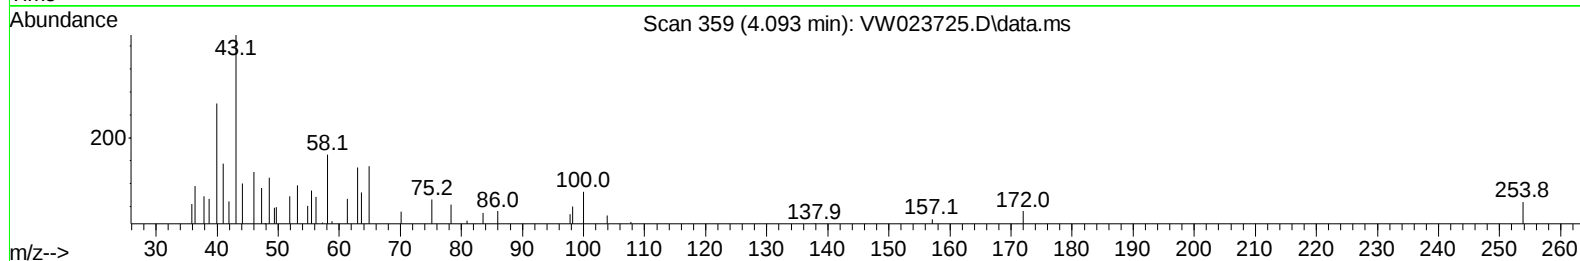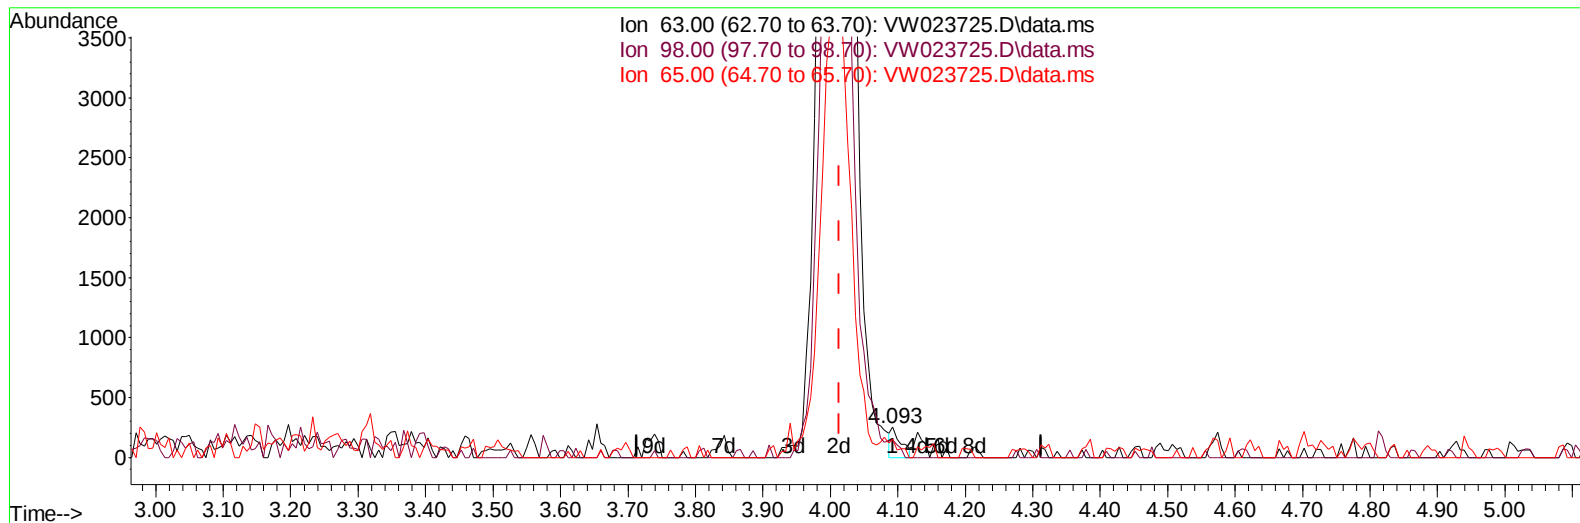

TIC: VW023725.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.093min (+ 0.079) 0.08 ug/L

response 256

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.20	67.19
65.00	24.10	19.92
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023725.D
Acq On : 15 Jul 2022 04:26
Operator : SY/VA
Sample : N3700-11
Misc : 4.88g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C18

Manual IntegrationsAPPROVED

Quant Time: Jul 15 06:30:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 06:03:21 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

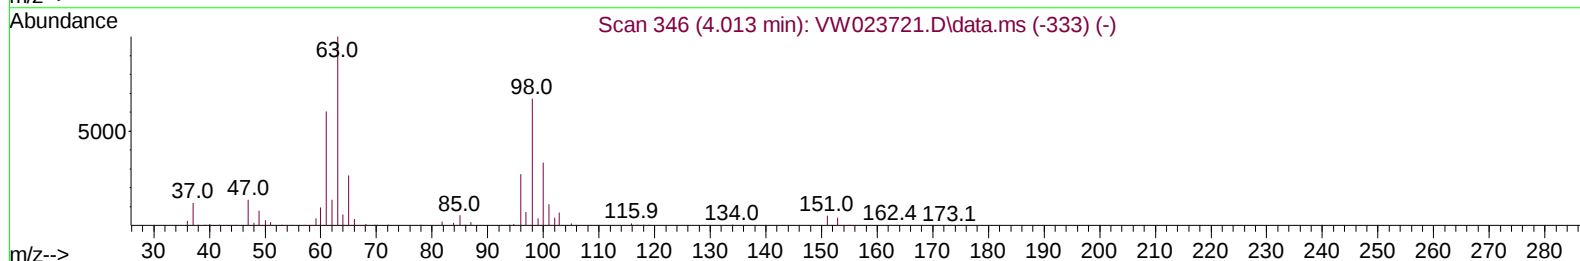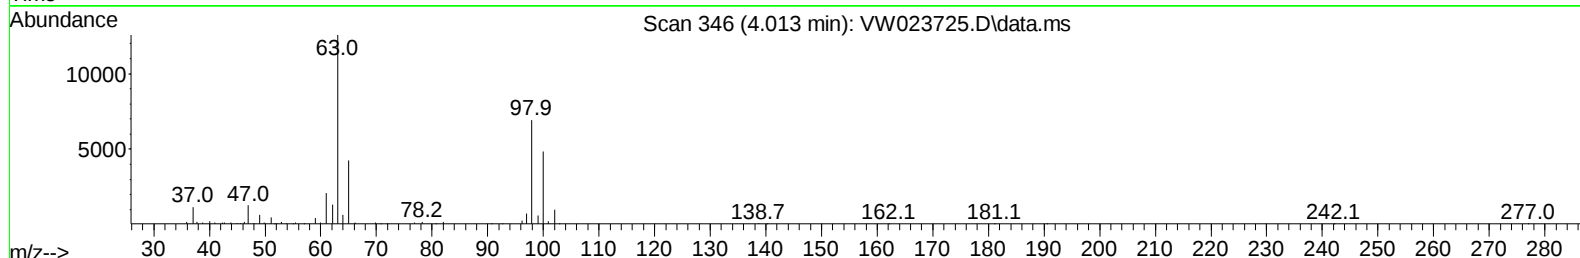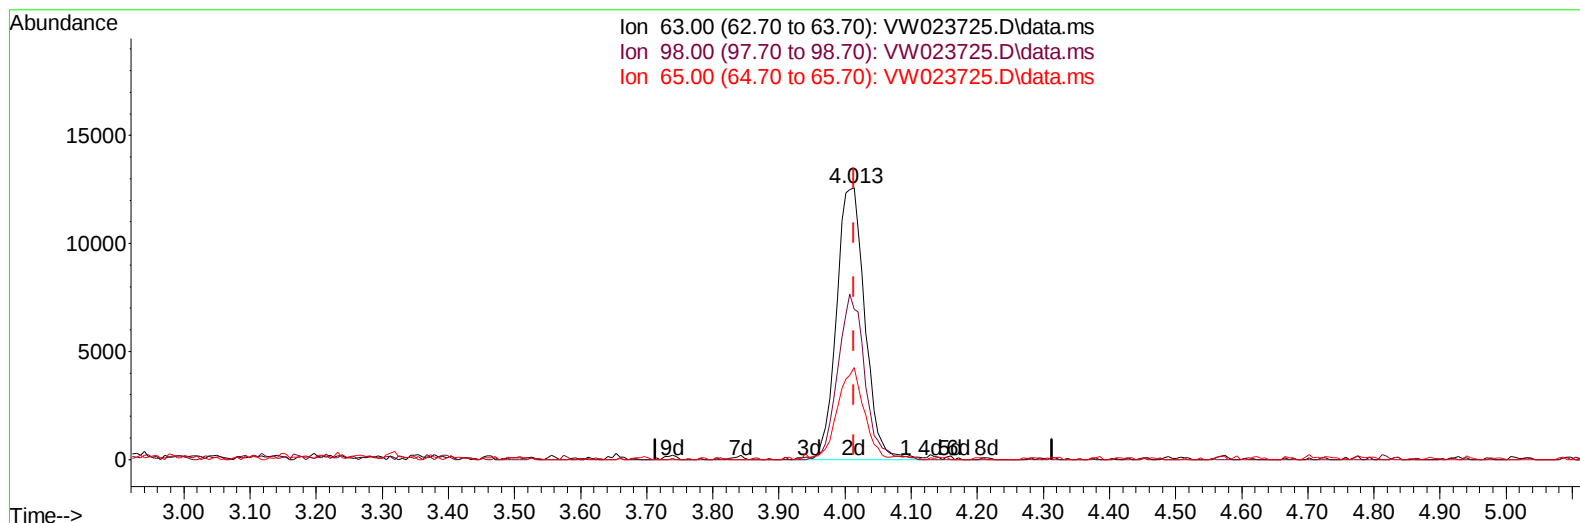

TIC: VW023725.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.000) 12.15 ug/L m

response 37546

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.20	0.46#
65.00	24.10	0.14#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023725.D
Acq On : 15 Jul 2022 04:26
Operator : SY/VA
Sample : N3700-11
Misc : 4.88g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C18

Manual IntegrationsAPPROVED

Quant Time: Jul 15 06:30:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 06:03:21 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

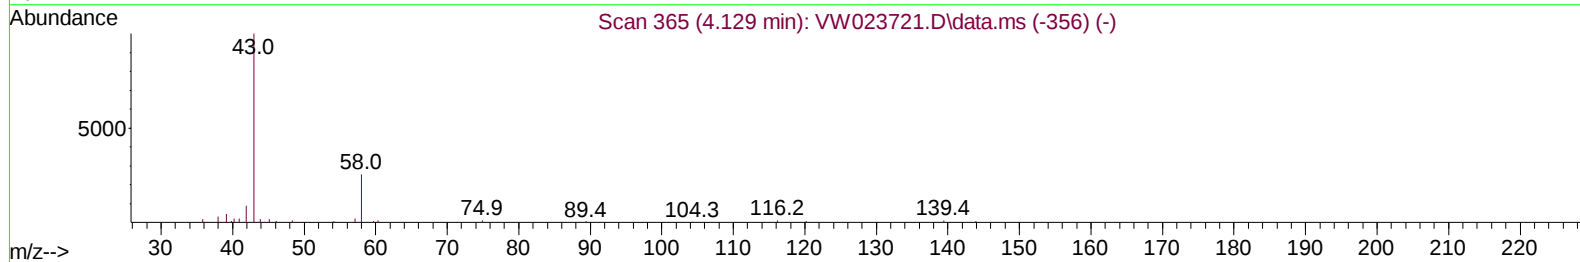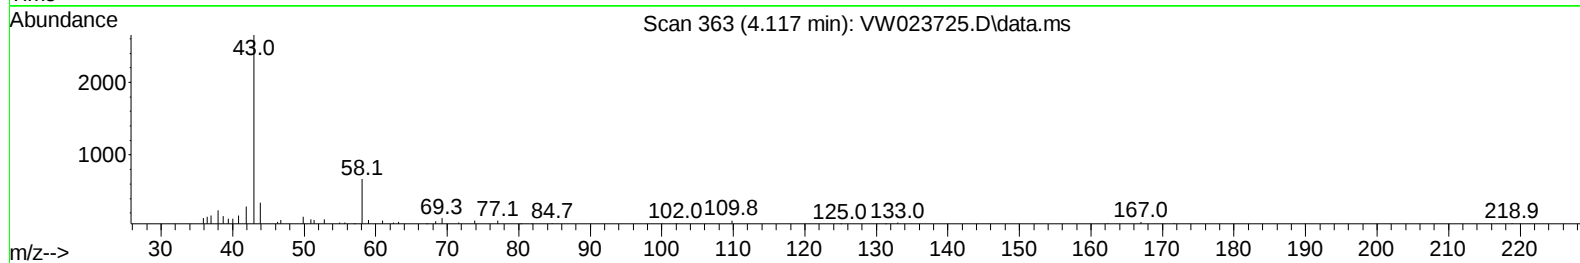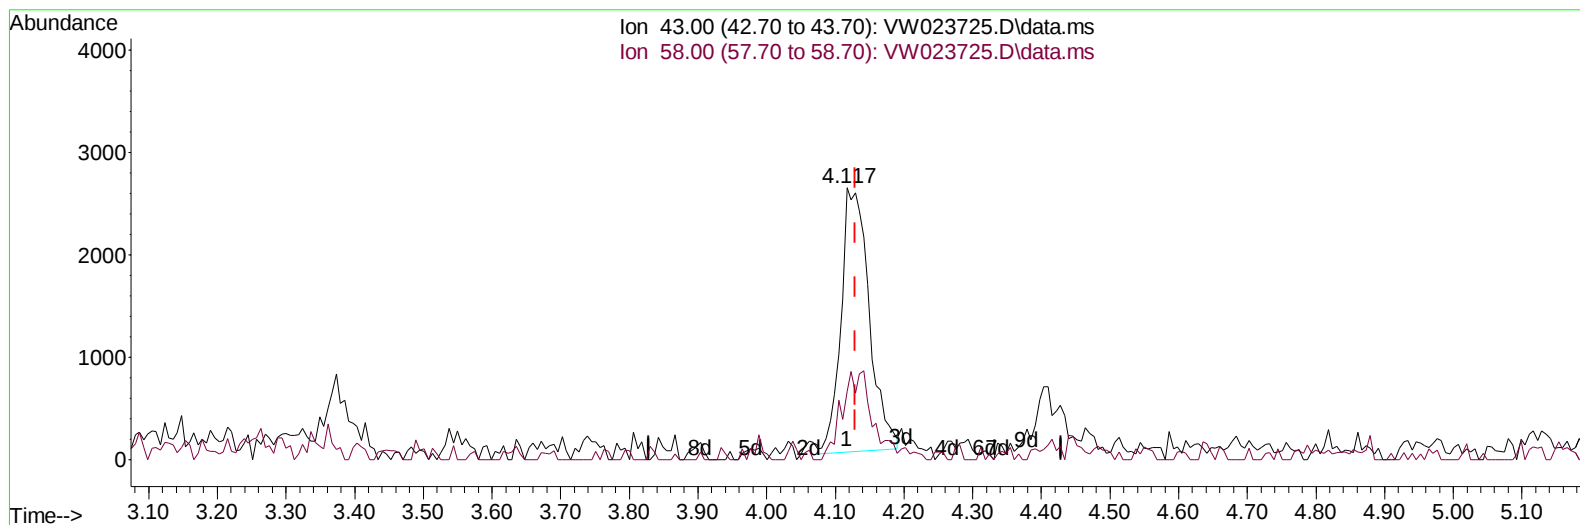

TIC: VW023725.D\data.ms

(13) Acetone (T)

4.117min (-0.012) 17.66 ug/L

response 7349

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	10.36
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023725.D
 Acq On : 15 Jul 2022 04:26
 Operator : SY/VA
 Sample : N3700-11
 Misc : 4.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C18

Manual IntegrationsAPPROVED

Quant Time: Jul 15 06:30:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

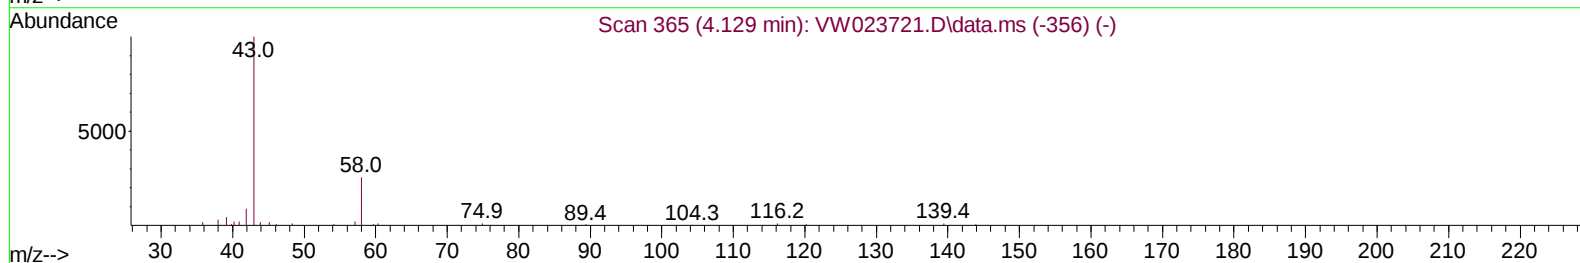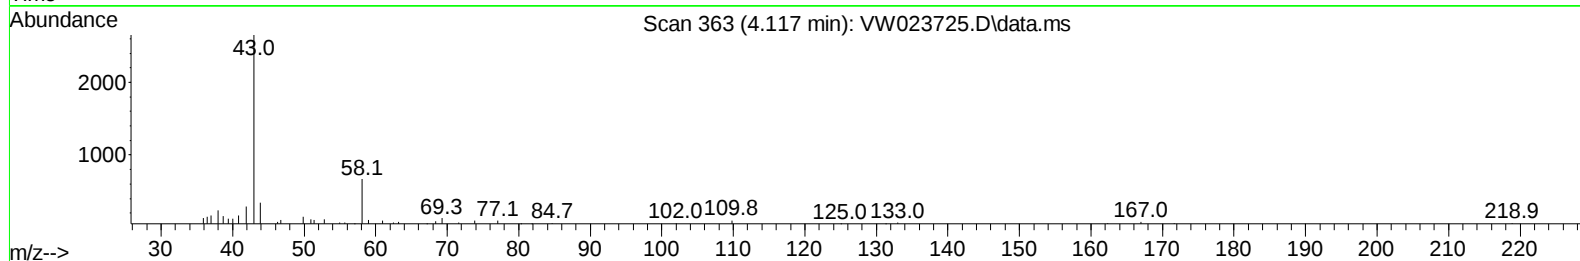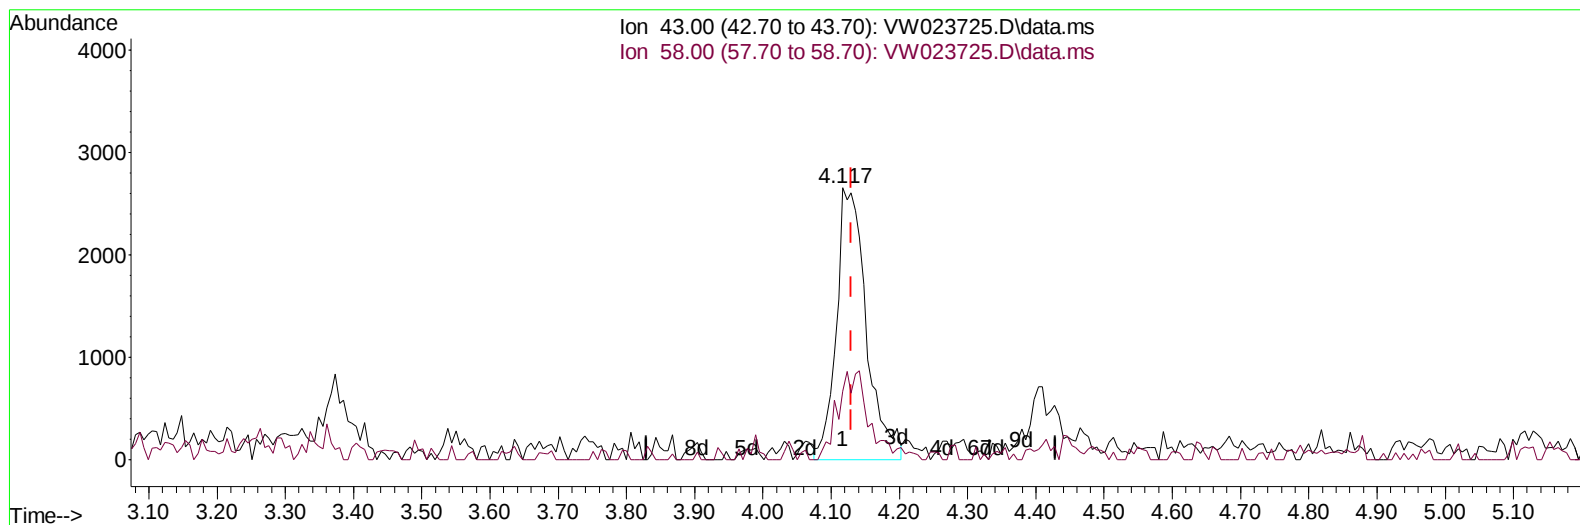

TIC: VW023725.D\data.ms

(13) Acetone (T)

4.117min (-0.012) 19.36 ug/L m

response 8059

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	9.44
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023725.D
 Acq On : 15 Jul 2022 04:26
 Operator : SY/VA
 Sample : N3700-11
 Misc : 4.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C18

Manual IntegrationsAPPROVED

Quant Time: Jul 15 06:30:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		148610	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		133112	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		46067	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		64256	16.929	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	67.720%		
7) Chloroethane-d5	2.879	69		42591	16.820	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	67.280%		
11) 1,1-Dichloroethene-d2	4.013	63		37546m	12.148	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	48.600%		
21) 2-Butanone-d5	7.080	46		23965	40.706	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	81.420%		
24) Chloroform-d	7.647	84		90562	20.931	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	83.720%		
26) 1,2-Dichloroethane-d4	8.299	65		54413	20.562	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	82.240%		
32) Benzene-d6	8.275	84		163625	23.647	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	94.600%		
36) 1,2-Dichloropropane-d6	9.275	67		52057	24.976	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	99.920%		
41) Toluene-d8	10.323	98		140887	20.073	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	80.280%		
43) trans-1,3-Dichloroprop...	10.573	79		15782	16.154	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	64.600%		
47) 2-Hexanone-d5	10.921	63		16862	38.472	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	76.940%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84		44124	19.156	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	76.640%		
66) 1,2-Dichlorobenzene-d4	13.853	152		37621	22.877	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	91.520%		
Target Compounds							
13) Acetone	4.117	43		8059m	19.361	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023725.D
Acq On : 15 Jul 2022 04:26
Operator : SY/VA
Sample : N3700-11
Misc : 4.88g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C18

Manual IntegrationsAPPROVED

Quant Time: Jul 15 06:30:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 06:03:21 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

