




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023733.D
 Acq On : 15 Jul 2022 07:40
 Operator : SY/VA
 Sample : N3700-19
 Misc : 5.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B61

Manual IntegrationsAPPROVED

Quant Time: Jul 15 08:04:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

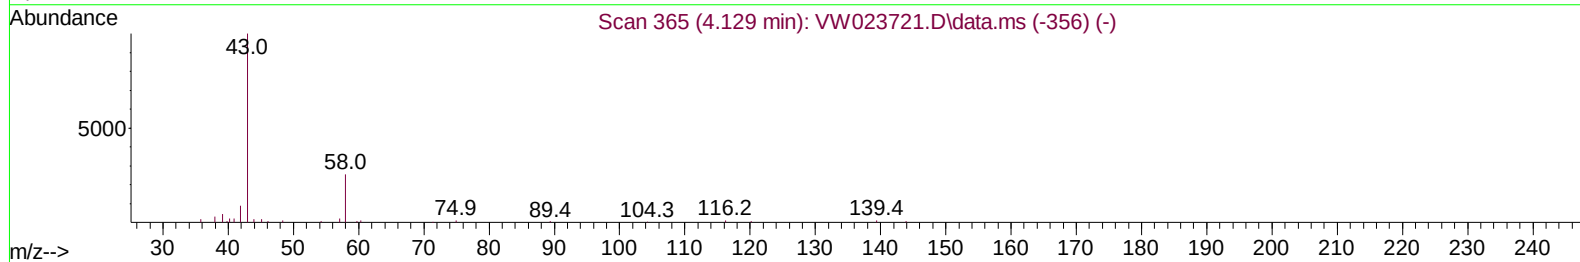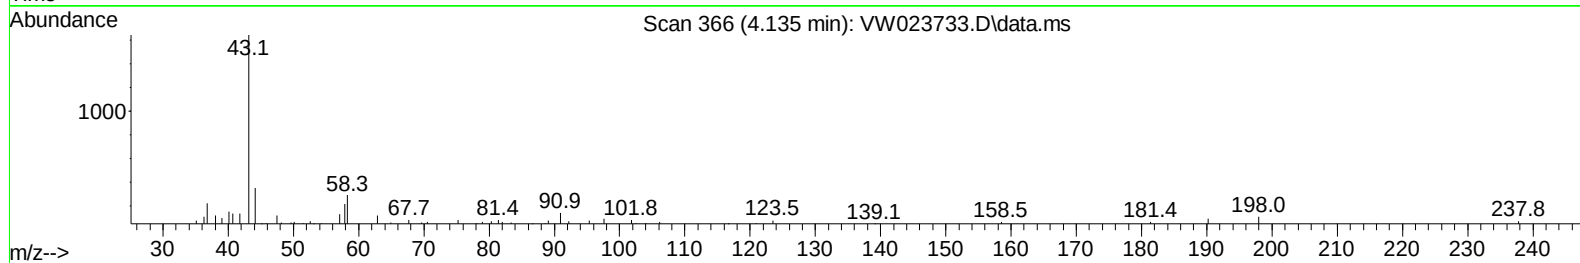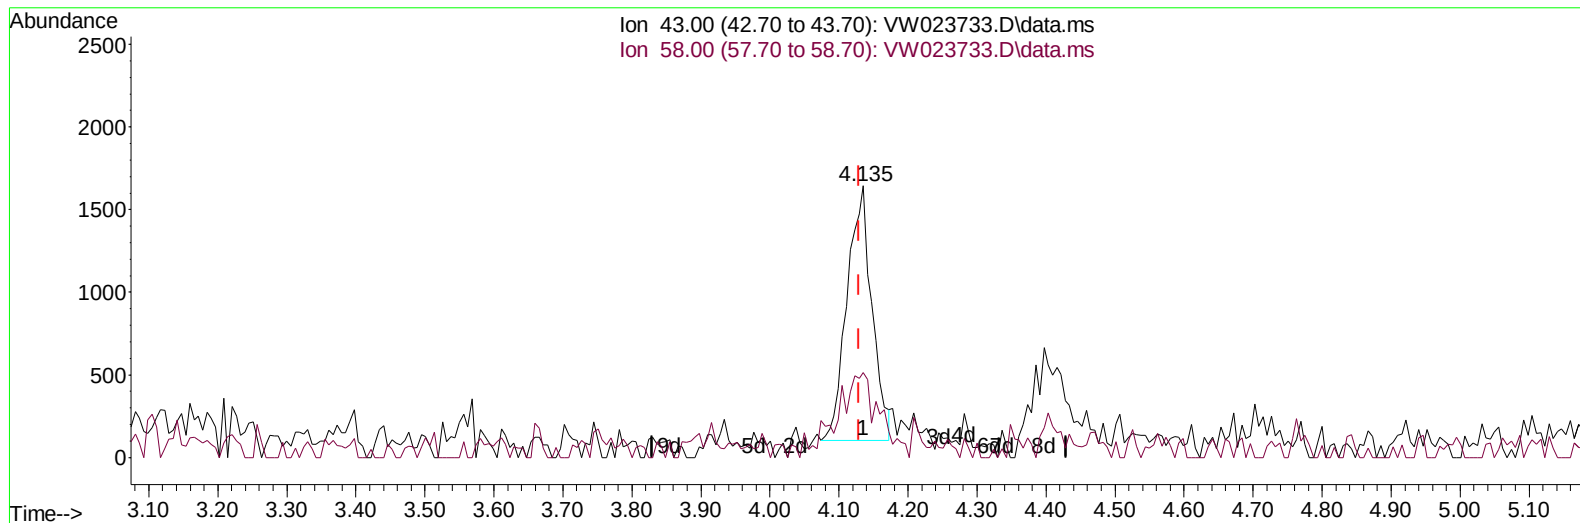

TIC: VW023733.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 6.52 ug/L

response 3837

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	24.42
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023733.D
 Acq On : 15 Jul 2022 07:40
 Operator : SY/VA
 Sample : N3700-19
 Misc : 5.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B61

Manual IntegrationsAPPROVED

Quant Time: Jul 15 08:04:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

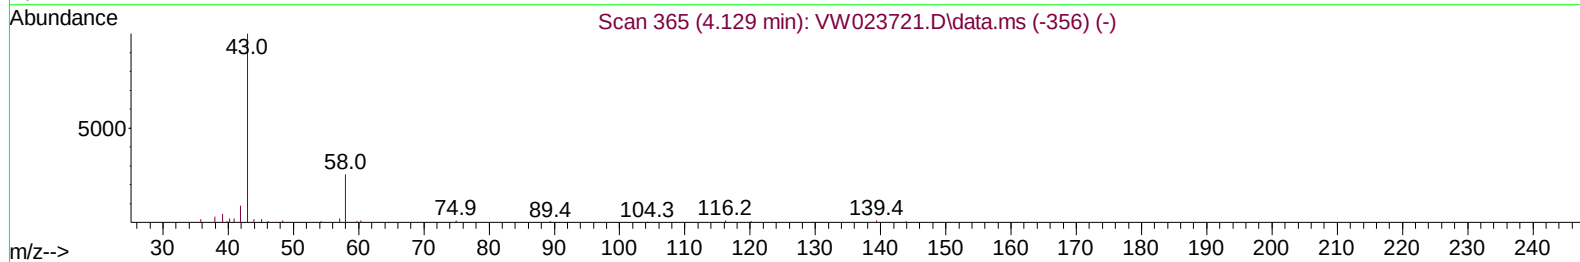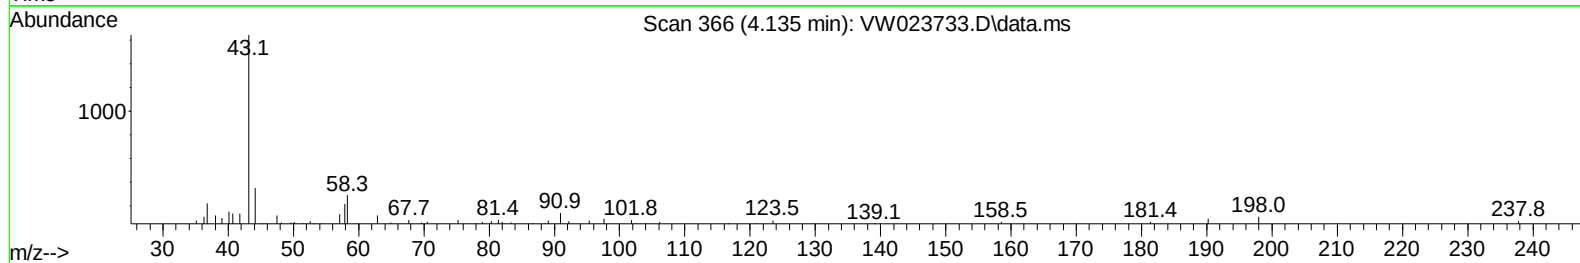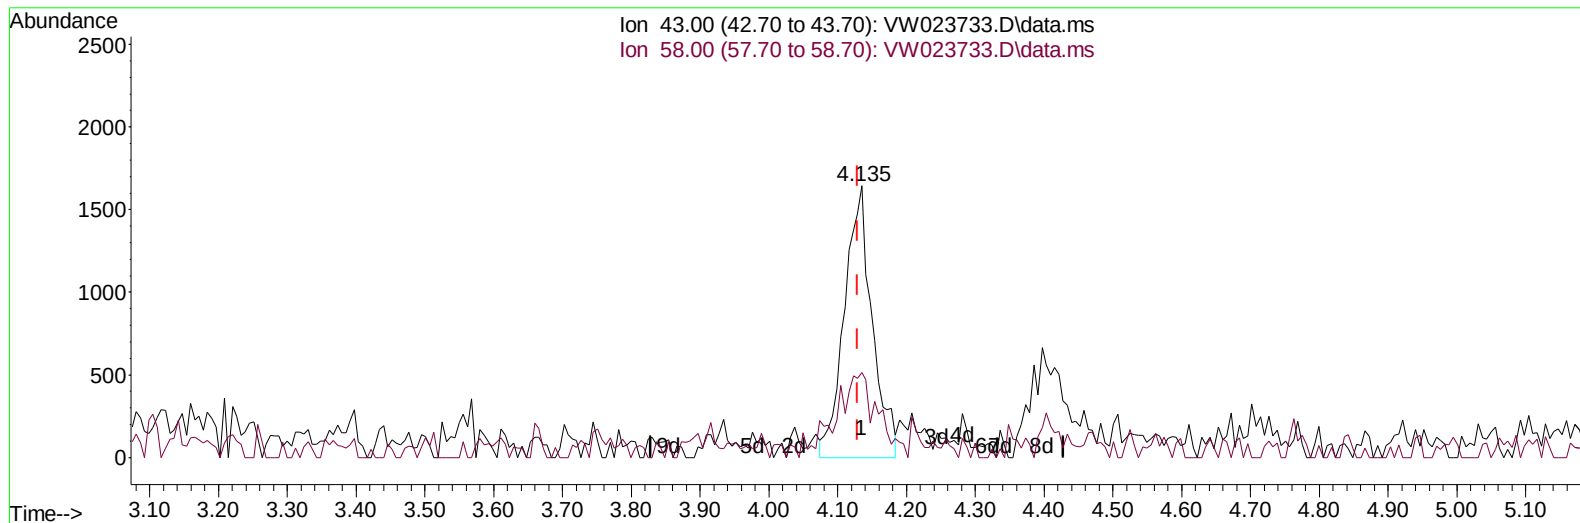

TIC: VW023733.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 7.83 ug/L m

response 4609

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	20.33
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023733.D
 Acq On : 15 Jul 2022 07:40
 Operator : SY/VA
 Sample : N3700-19
 Misc : 5.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B61

Manual IntegrationsAPPROVED

Quant Time: Jul 15 08:04:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	210170	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	189083	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	81606	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	75102	13.991	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	55.960%	
7) Chloroethane-d5	2.879	69	59261	16.549	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	66.200%	
11) 1,1-Dichloroethene-d2	4.007	63	44404	10.159	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	40.640%#	
21) 2-Butanone-d5	7.080	46	26822	32.214	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	64.420%	
24) Chloroform-d	7.647	84	109145	17.837	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	71.360%	
26) 1,2-Dichloroethane-d4	8.305	65	63252	16.901	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	67.600%#	
32) Benzene-d6	8.275	84	192900	19.625	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	78.520%	
36) 1,2-Dichloropropane-d6	9.274	67	63433	21.425	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	85.680%	
41) Toluene-d8	10.323	98	174694	17.522	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	70.080%	
43) trans-1,3-Dichloroprop...	10.579	79	18143	13.073	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	52.280%	
47) 2-Hexanone-d5	10.927	63	20007	32.136	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	64.280%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	53868	16.464	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	65.840%	
66) 1,2-Dichlorobenzene-d4	13.853	152	53829	18.478	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	73.920%#	
Target Compounds						
13) Acetone	4.135	43	4609m	7.829	ug/L	
14) Carbon disulfide	4.379	76	10289	1.570	ug/L	97
53) m,p-Xylene	11.835	106	4934	0.908	ug/L	88
63) 1,2,4-Trimethylbenzene	13.249	105	6097	0.679	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023733.D
Acq On : 15 Jul 2022 07:40
Operator : SY/VA
Sample : N3700-19
Misc : 5.82g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B61

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 08:04:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 06:03:21 2022
Response via : Initial Calibration

