




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023736.D
 Acq On : 15 Jul 2022 08:54
 Operator : SY/VA
 Sample : N3701-03
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B64

Manual IntegrationsAPPROVED

Quant Time: Jul 15 09:16:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

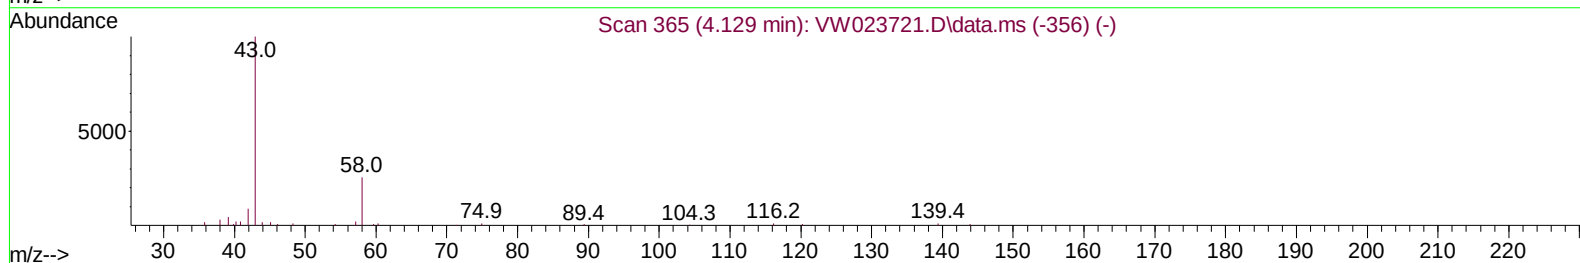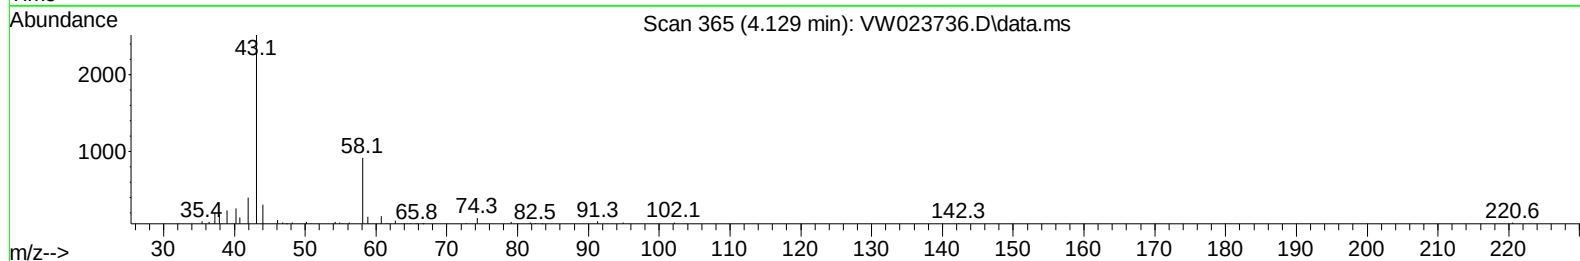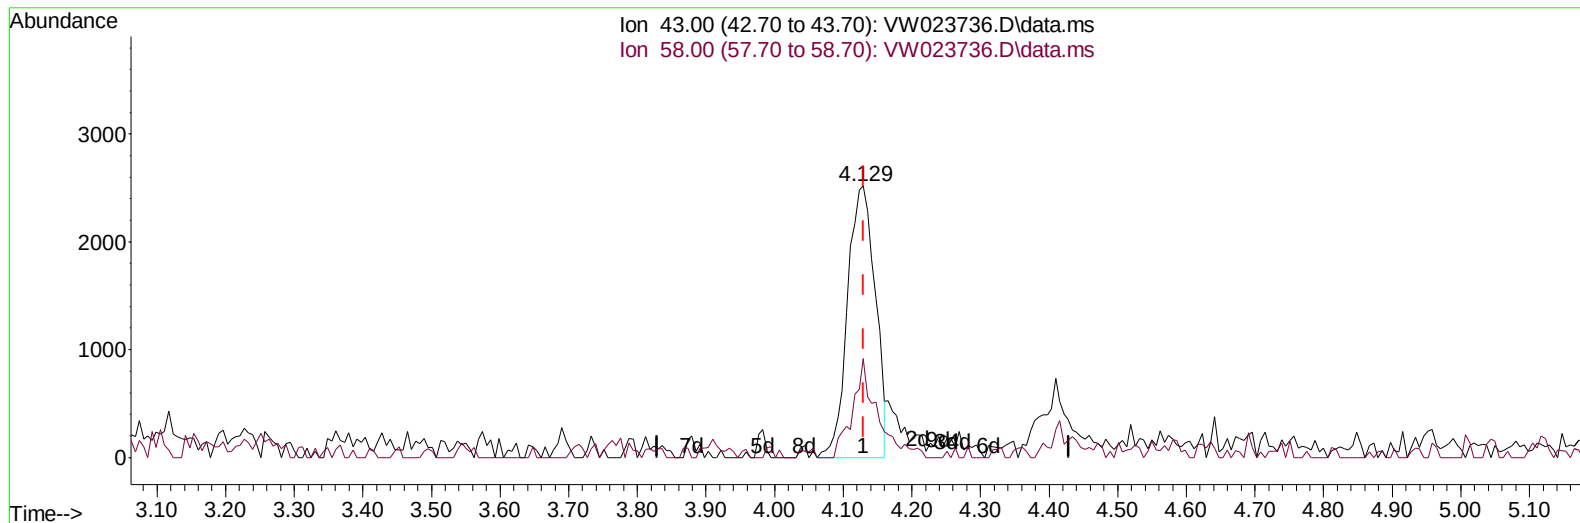

TIC: VW023736.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 28.99 ug/L

response 7023

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	9.91
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023736.D
 Acq On : 15 Jul 2022 08:54
 Operator : SY/VA
 Sample : N3701-03
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B64

Manual IntegrationsAPPROVED

Quant Time: Jul 15 09:16:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

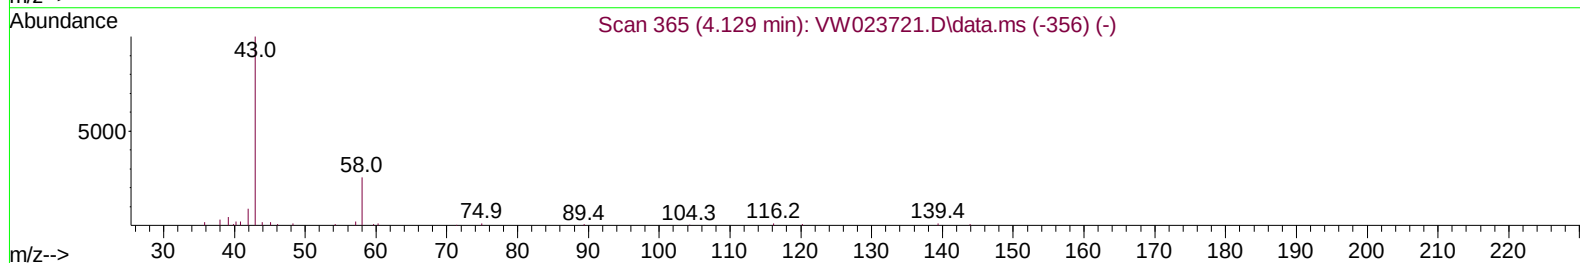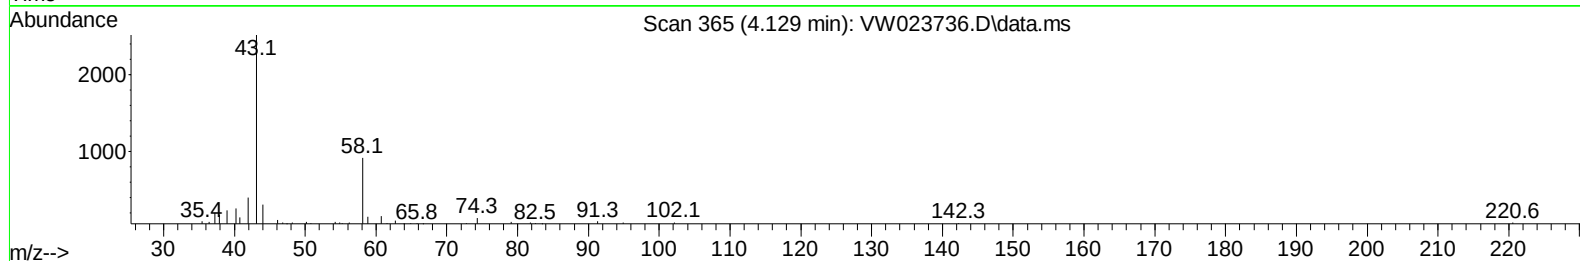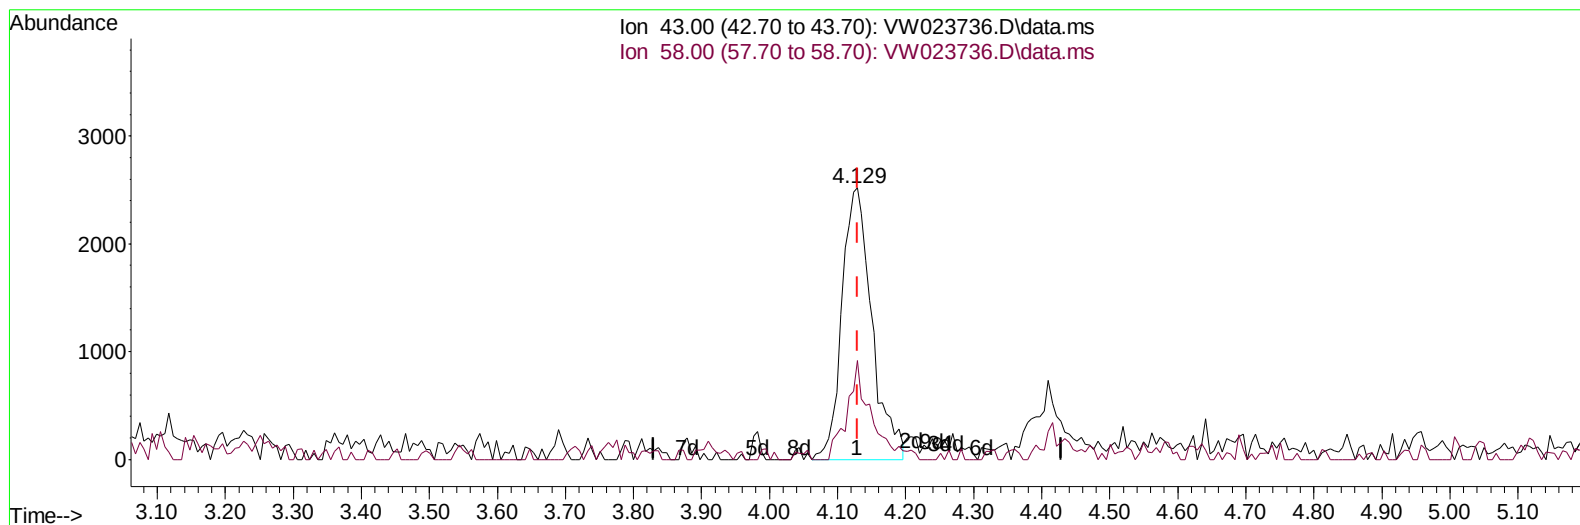

TIC: VW023736.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 32.00 ug/L m

response 7752

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	8.98
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023736.D
 Acq On : 15 Jul 2022 08:54
 Operator : SY/VA
 Sample : N3701-03
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B64

Manual IntegrationsAPPROVED

Quant Time: Jul 15 09:16:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		86495	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		77415	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		29105	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		45770	20.718	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	82.880%	
7) Chloroethane-d5	2.879	69		37302	25.311	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	101.240%	
11) 1,1-Dichloroethene-d2	4.007	63		30475	16.941	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	67.760%	
21) 2-Butanone-d5	7.074	46		16170	47.189	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	94.380%	
24) Chloroform-d	7.647	84		55233	21.933	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	87.720%	
26) 1,2-Dichloroethane-d4	8.305	65		35413	22.993	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	91.960%	
32) Benzene-d6	8.275	84		102953	25.583	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	102.320%	
36) 1,2-Dichloropropane-d6	9.275	67		33590	27.710	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	110.840%	
41) Toluene-d8	10.323	98		85164	20.864	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	83.440%	
43) trans-1,3-Dichloroprop...	10.579	79		8473	14.912	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	59.640%	
47) 2-Hexanone-d5	10.927	63		10835	42.507	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	85.020%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		29531	22.044	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	88.160%	
66) 1,2-Dichlorobenzene-d4	13.853	152		23440	22.560	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	90.240%	
Target Compounds							
13) Acetone	4.129	43		7752m	31.998	ug/L	
14) Carbon disulfide	4.367	76		8140	3.018	ug/L #	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023736.D
Acq On : 15 Jul 2022 08:54
Operator : SY/VA
Sample : N3701-03
Misc : 5.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5B64

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 09:16:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 06:03:21 2022
Response via : Initial Calibration

