

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023706.D
 Acq On : 14 Jul 2022 17:38
 Operator : SY/VA
 Sample : N3698-02
 Misc : 5.79g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5B67

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 03:44:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 03:40:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	191433	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	166850	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	69278	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	76497	15.646	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.600%
7) Chloroethane-d5	2.879	69	58702	17.997	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.000%
11) 1,1-Dichloroethene-d2	4.013	63	38503	9.671	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	38.680%#
21) 2-Butanone-d5	7.074	46	34806	45.895	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.780%
24) Chloroform-d	7.647	84	91084	16.342	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	65.360%
26) 1,2-Dichloroethane-d4	8.305	65	57850m	16.971	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	67.880%#
32) Benzene-d6	8.269	84	167858	19.353	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.400%
36) 1,2-Dichloropropane-d6	9.275	67	52873	20.238	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	80.960%
41) Toluene-d8	10.323	98	147121	16.723	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	66.880%
43) trans-1,3-Dichloroprop...	10.579	79	20391	16.651	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.600%
47) 2-Hexanone-d5	10.927	63	24679	44.922	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.840%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	55041	19.064	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	45067	18.223	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	72.880%#
Target Compounds						
5) Vinyl chloride	2.349	62	87445	15.985	ug/L	97
13) Acetone	4.129	43	9925	18.510	ug/L	97
17) trans-1,2-Dichloroethene	5.422	96	3702	1.504	ug/L	79
20) cis-1,2-Dichloroethene	7.165	96	89516	32.818	ug/L #	94
29) Cyclohexane	7.952	56	12884	4.222	ug/L	94
33) Benzene	8.317	78	26407	2.785	ug/L	100
35) Methylcyclohexane	9.335	83	23634	6.199	ug/L #	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023706.D
Acq On : 14 Jul 2022 17:38
Operator : SY/VA
Sample : N3698-02
Misc : 5.79g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F5B67

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022


Quant Time: Jul 15 03:44:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 03:40:01 2022
Response via : Initial Calibration

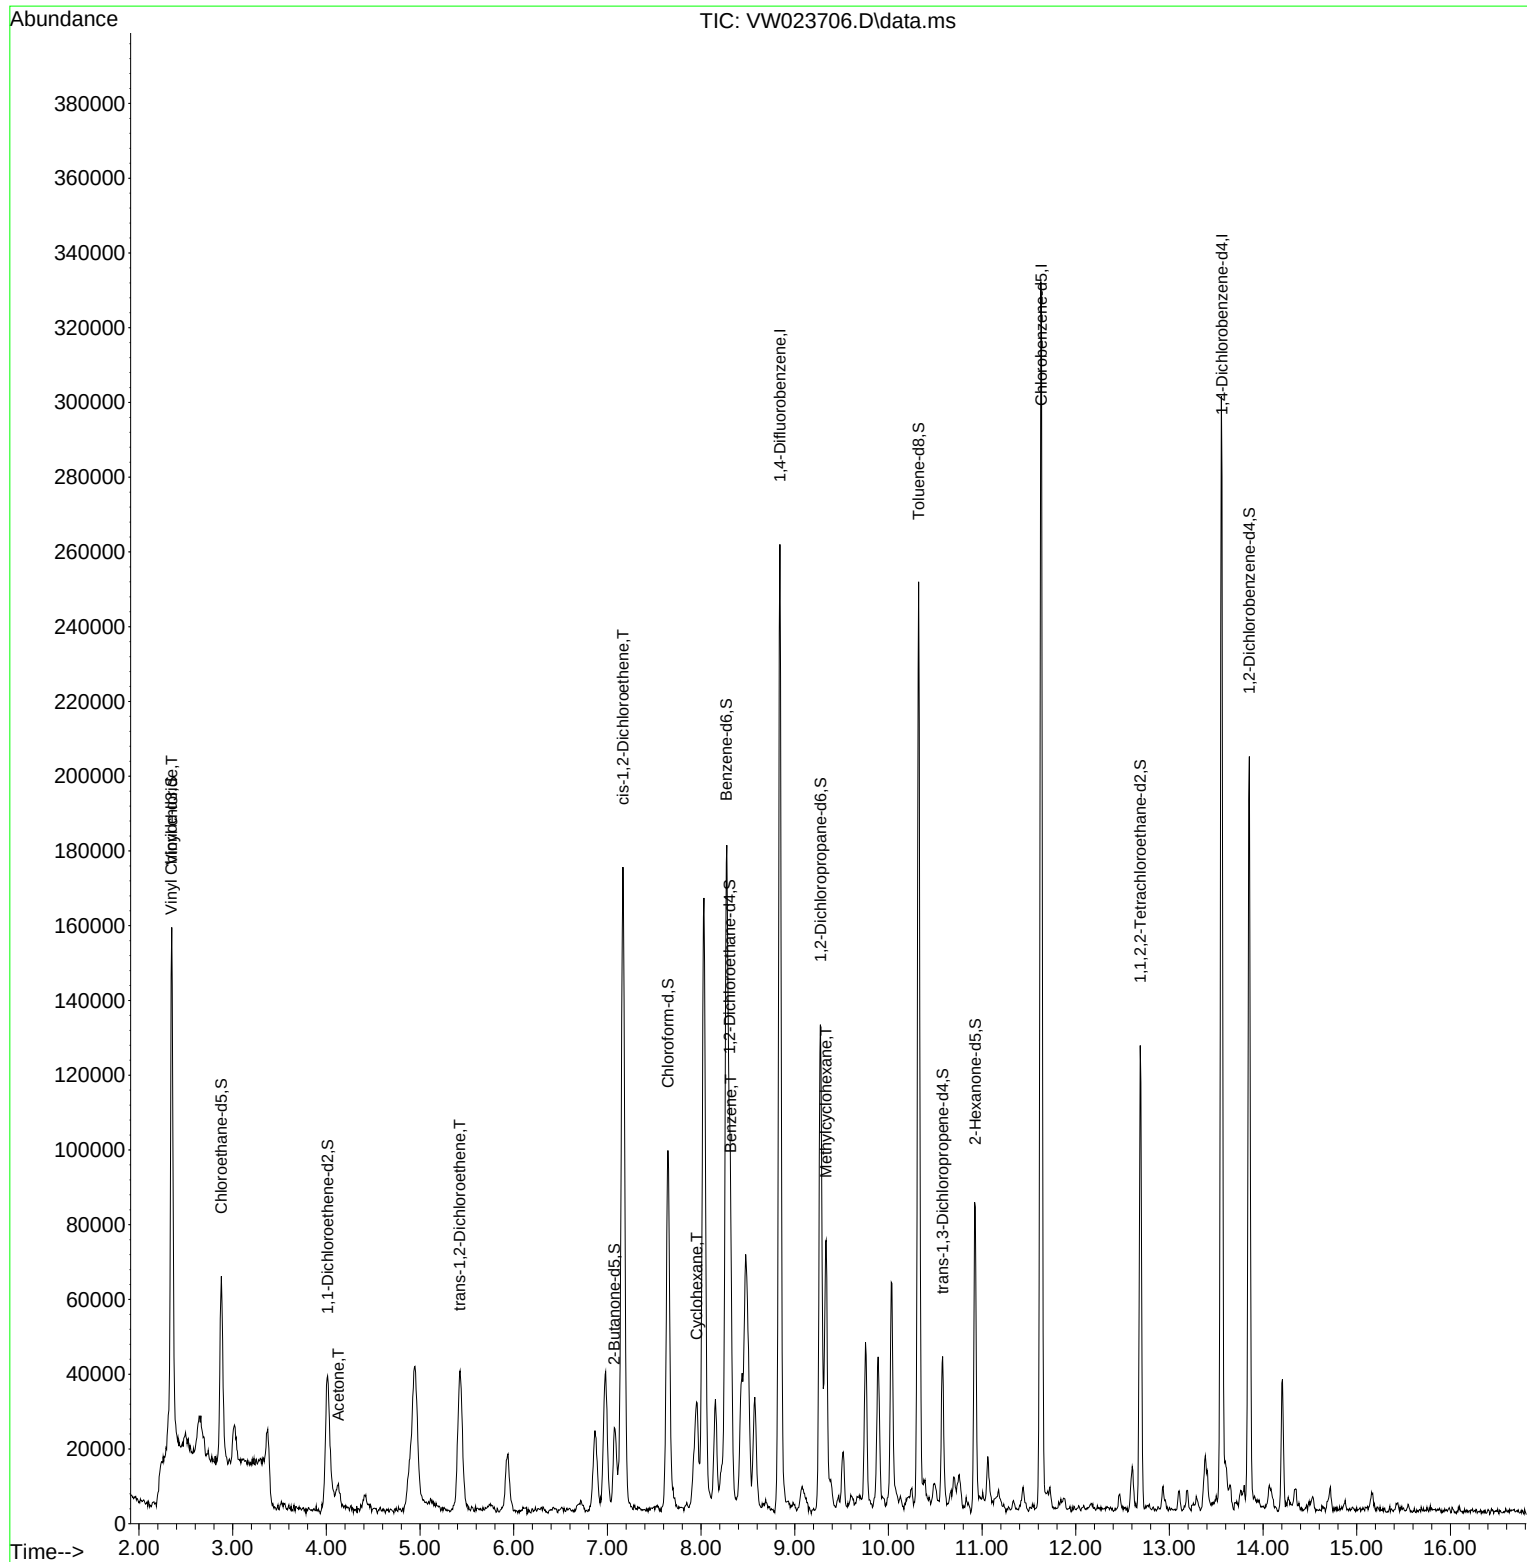

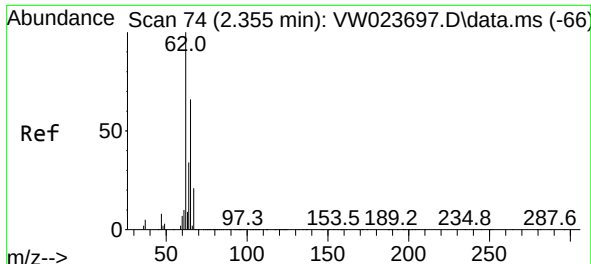

#5
 Vinyl chloride
 Concen: 15.985 ug/L
 RT: 2.349 min Scan# 71
 Delta R.T. -0.006 min
 Lab File: VW023706.D
 Acq: 14 Jul 2022 17:38




Instrument :
 MSVOA_W
 ClientSampleId :
 F5B67

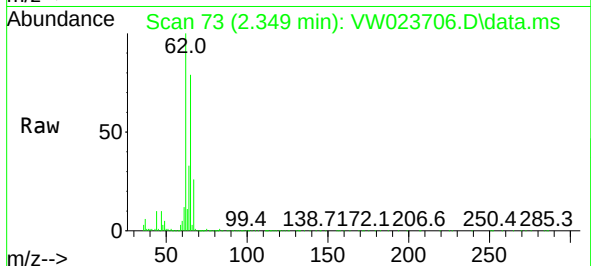

Tgt Ion: 62 Resp: 8744
 Ion Ratio Lower Upper
 62 100
 64 32.8 24.0 44.6




Manual Integrations
 APPROVED


Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

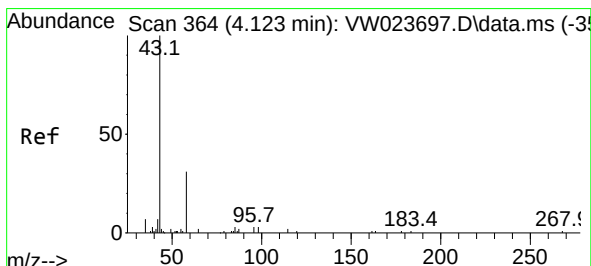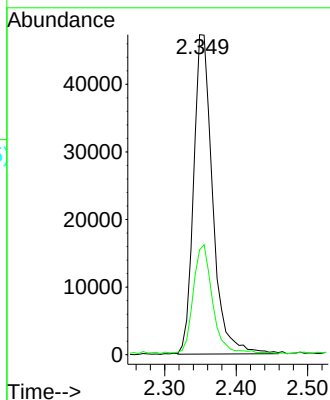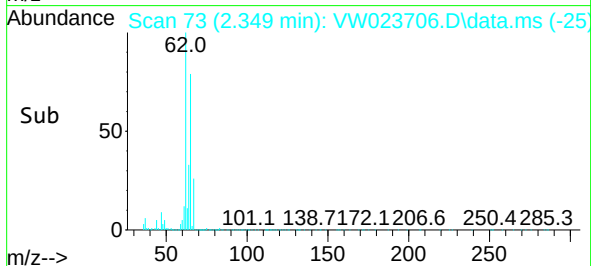

#13
 Acetone
 Concen: 18.510 ug/L
 RT: 4.129 min Scan# 365
 Delta R.T. 0.006 min
 Lab File: VW023706.D
 Acq: 14 Jul 2022 17:38


Tgt Ion: 43 Resp: 9925
 Ion Ratio Lower Upper
 43 100
 58 30.4 0.0 64.2

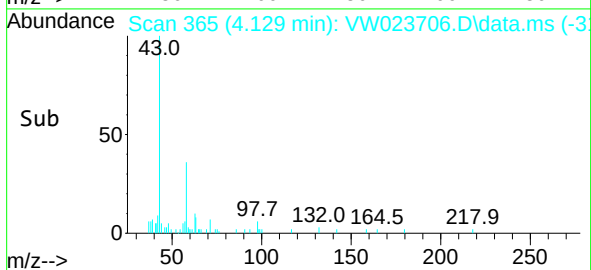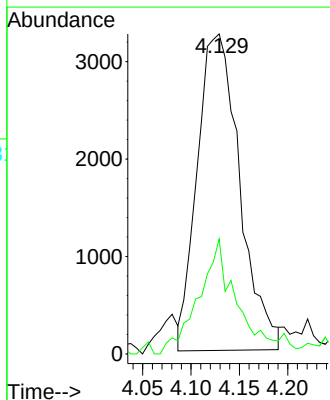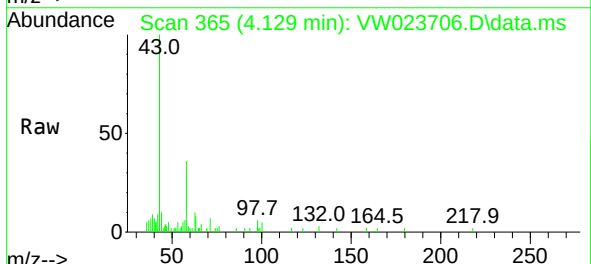

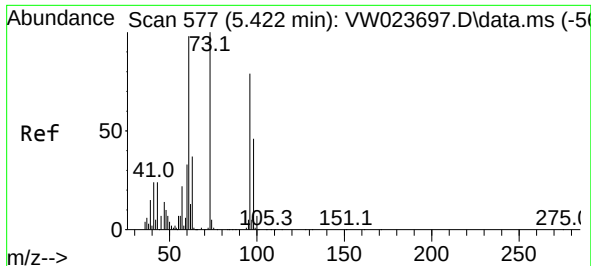

#17
trans-1,2-Dichloroethene
Concen: 1.504 ug/L
RT: 5.422 min Scan# 577
Delta R.T. 0.000 min
Lab File: VW023706.D
Acq: 14 Jul 2022 17:38




Instrument :
MSVOA_W
ClientSampleId :
F5B67

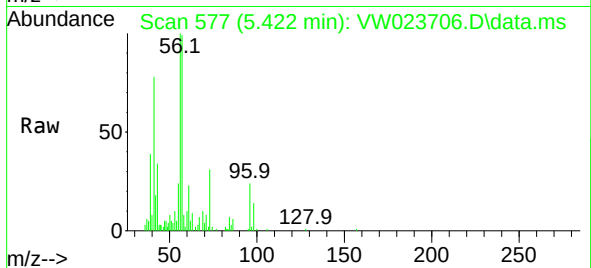

Tgt Ion: 96 Resp: 3702
Ion Ratio Lower Upper
96 100
61 96.3 90.8 168.6
98 58.3 42.8 79.6




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

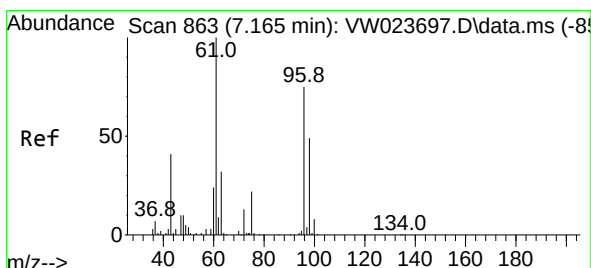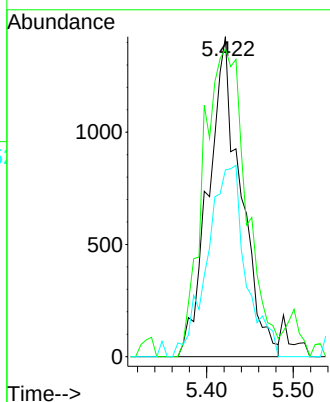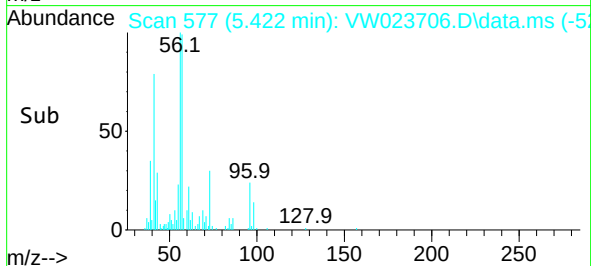

#20
cis-1,2-Dichloroethene
Concen: 32.818 ug/L
RT: 7.165 min Scan# 863
Delta R.T. 0.000 min
Lab File: VW023706.D
Acq: 14 Jul 2022 17:38

Tgt Ion: 96 Resp: 89516
Ion Ratio Lower Upper
96 100
61 122.4 90.6 168.2
68 0.2 0.2 0.4

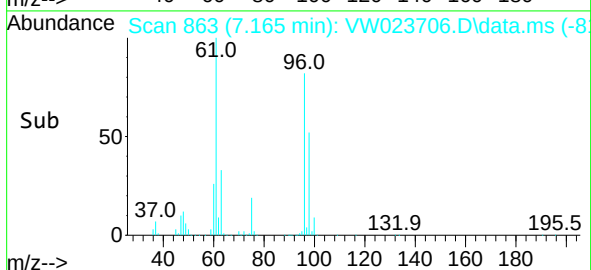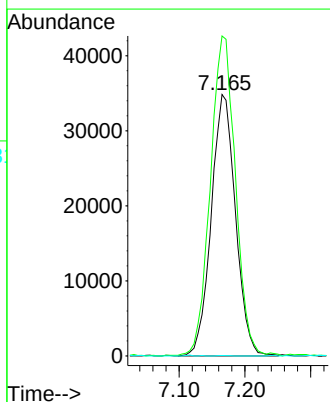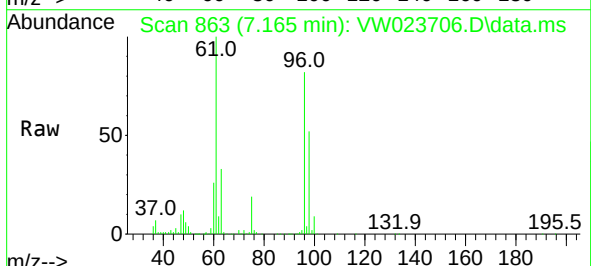

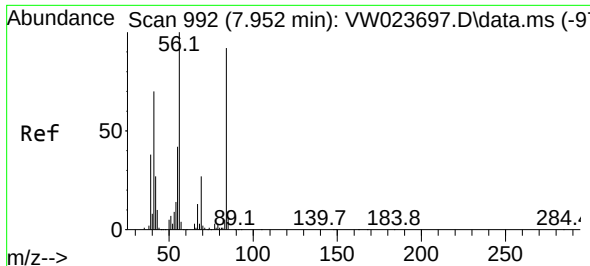

#29

Cyclohexane

Concen: 4.222 ug/L

RT: 7.952 min Scan# 992

Delta R.T. 0.000 min

Lab File: VW023706.D


Acq: 14 Jul 2022 17:38

Instrument :

MSVOA_W

ClientSampleId :

F5B67

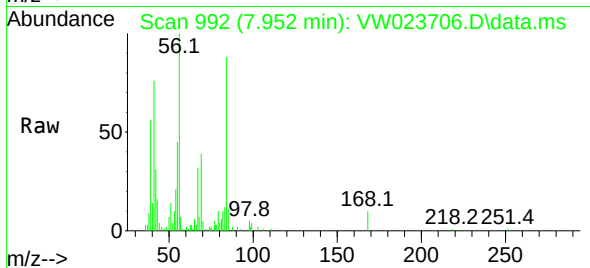




Tgt Ion: 56	Resp: 12884
Ion Ratio	Lower Upper
56	100
69	30.2 25.4 38.0
84	86.4 75.0 112.4

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 07/18/2022

Supervised By :Mahesh Dadoda 07/18/2022

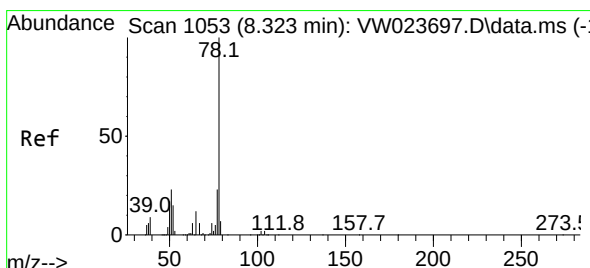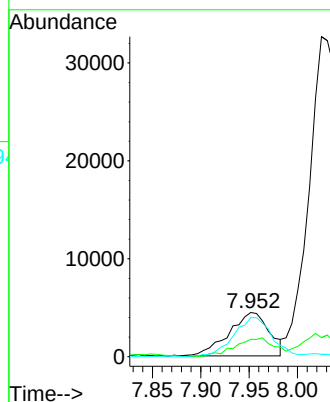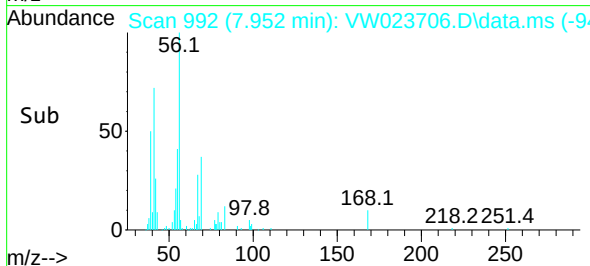

#33

Benzene

Concen: 2.785 ug/L




RT: 8.317 min Scan# 1052


Delta R.T. -0.006 min

Lab File: VW023706.D

Acq: 14 Jul 2022 17:38

Tgt Ion: 78 Resp: 26407

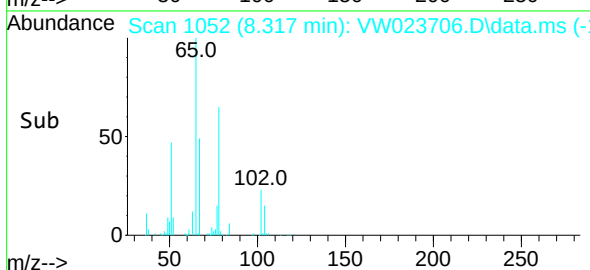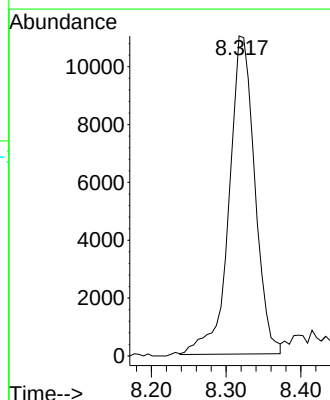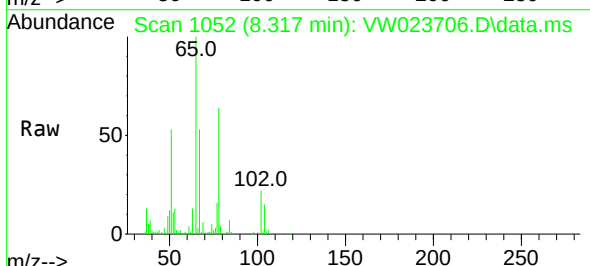

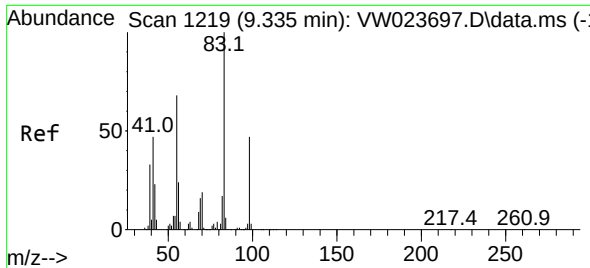

#35

Methylcyclohexane

Concen: 6.199 ug/L

RT: 9.335 min Scan# 11

Delta R.T. 0.000 min

Lab File: VW023706.D

Acq: 14 Jul 2022 17:38

Instrument :

MSVOA_W

ClientSampleId :

F5B67

Tgt Ion: 83 Resp: 23634

Ion Ratio Lower Upper

83 100

55 93.4 60.8 91.2

98 50.1 39.5 59.3

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 07/18/2022

Supervised By :Mahesh Dadoda 07/18/2022

