

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
 Data File : VW023725.D
 Acq On : 15 Jul 2022 04:26
 Operator : SY/VA
 Sample : N3700-11
 Misc : 4.88g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C18

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 06:30:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 15 06:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	148610	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	133112	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	46067	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	64256	16.929	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	67.720%		
7) Chloroethane-d5	2.879	69	42591	16.820	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	67.280%		
11) 1,1-Dichloroethene-d2	4.013	63	37546m	12.148	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	48.600%		
21) 2-Butanone-d5	7.080	46	23965	40.706	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.420%		
24) Chloroform-d	7.647	84	90562	20.931	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	83.720%		
26) 1,2-Dichloroethane-d4	8.299	65	54413	20.562	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	82.240%		
32) Benzene-d6	8.275	84	163625	23.647	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.600%		
36) 1,2-Dichloropropane-d6	9.275	67	52057	24.976	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	99.920%		
41) Toluene-d8	10.323	98	140887	20.073	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.280%		
43) trans-1,3-Dichloroprop...	10.573	79	15782	16.154	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	64.600%		
47) 2-Hexanone-d5	10.921	63	16862	38.472	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	76.940%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	44124	19.156	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	76.640%		
66) 1,2-Dichlorobenzene-d4	13.853	152	37621	22.877	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.520%		
Target Compounds					Qvalue	
13) Acetone	4.117	43	8059m	19.361	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071422\
Data File : VW023725.D
Acq On : 15 Jul 2022 04:26
Operator : SY/VA
Sample : N3700-11
Misc : 4.88g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F5C18

Quant Time: Jul 15 06:30:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 15 06:03:21 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

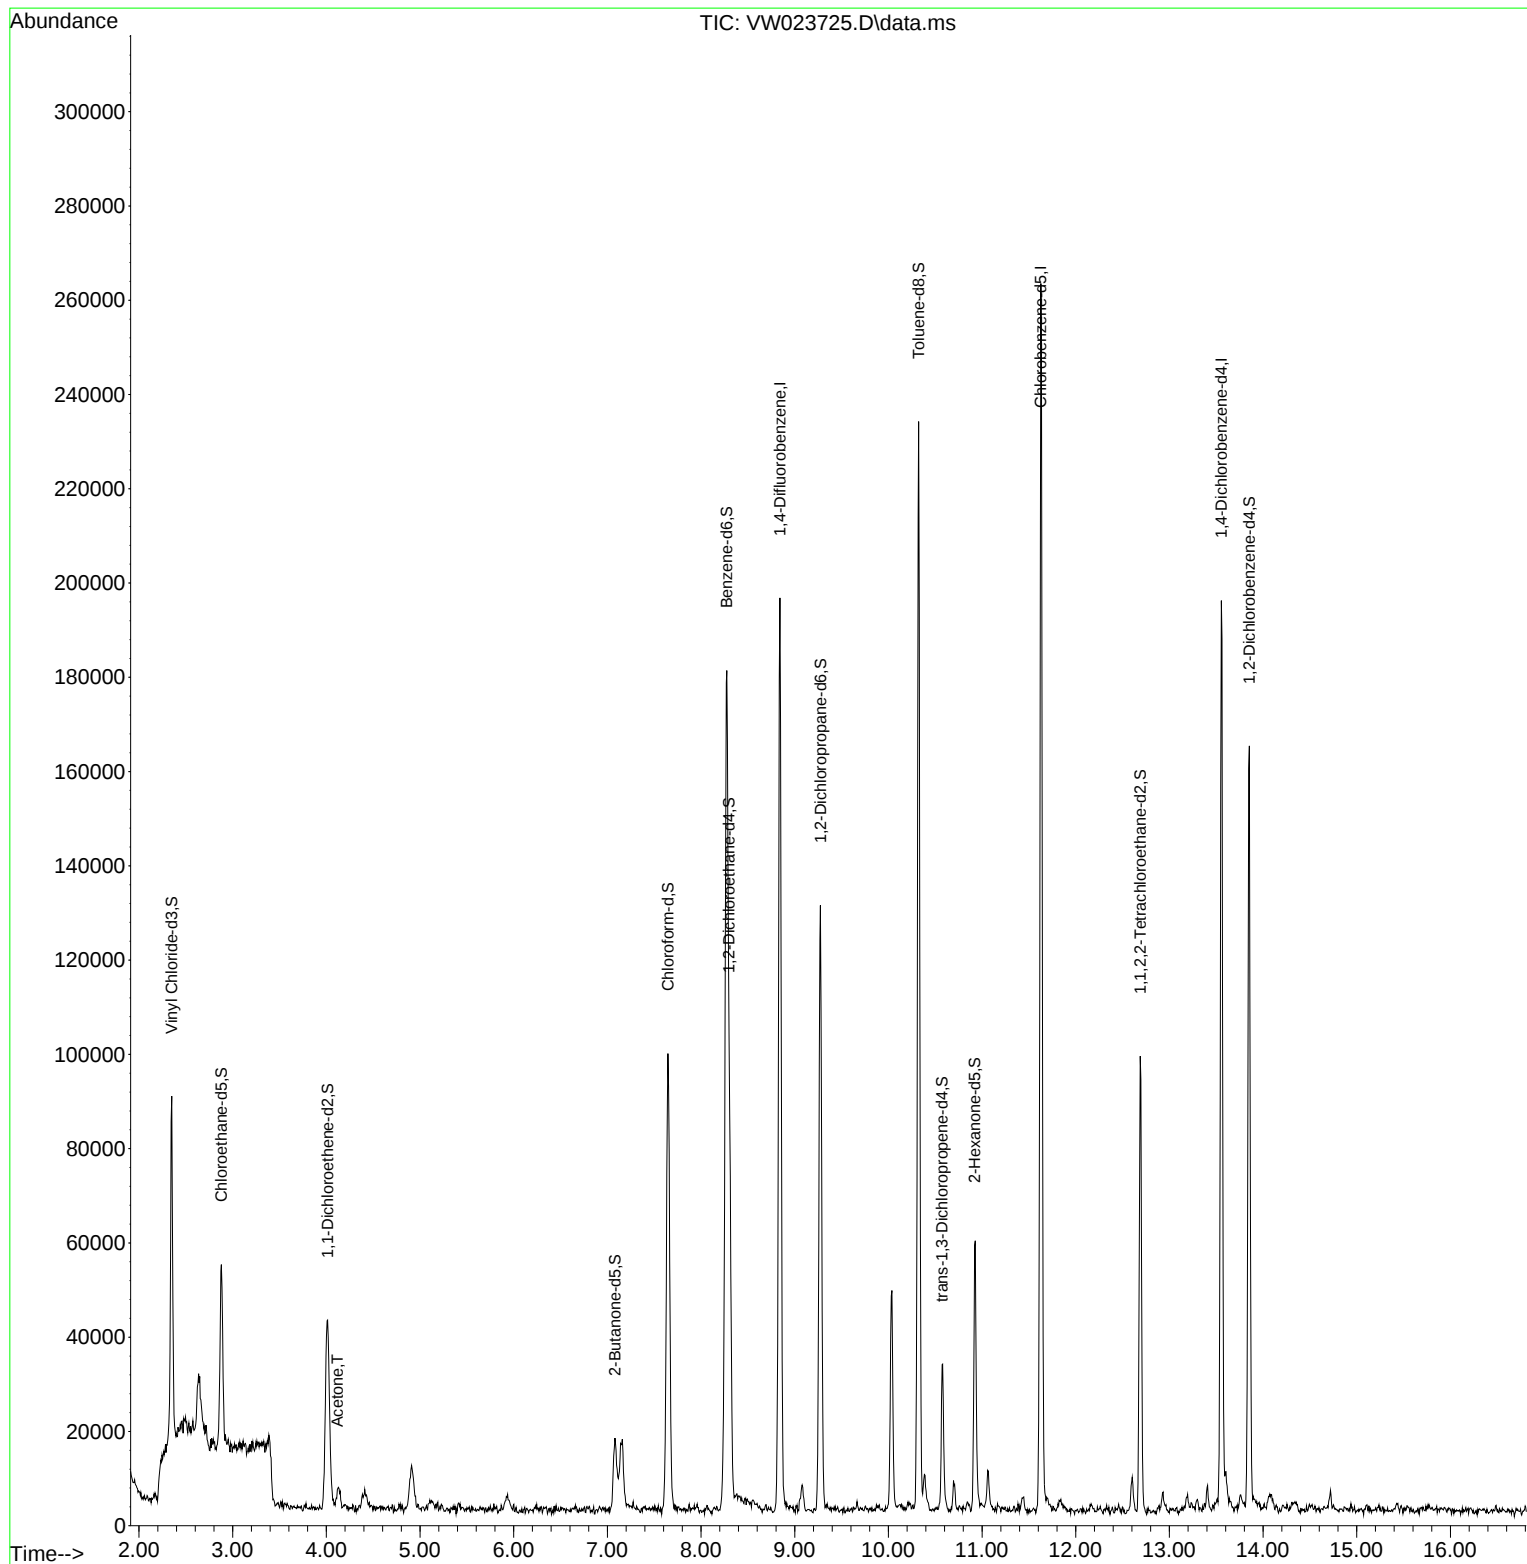

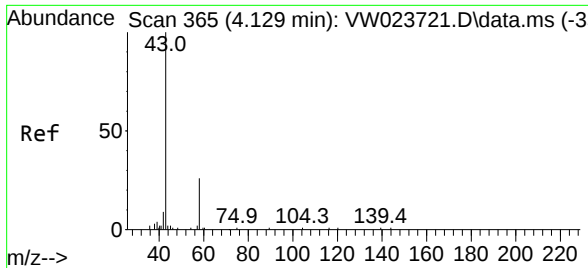

#13
 Acetone
 Concen: 19.361 ug/L m
 RT: 4.117 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: VW023725.D
 Acq: 15 Jul 2022 04:26

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C18

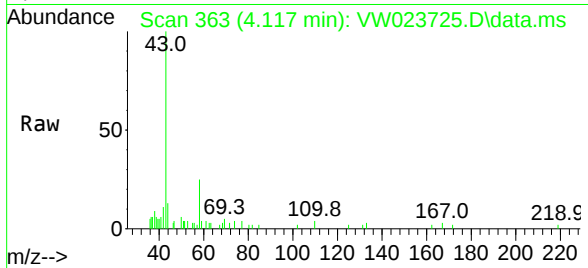

Tgt Ion: 43 Resp: 805
 Ion Ratio Lower Upper
 43 100
 58 9.4 0.0 64.2

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

