

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW071519\
Quantitation Report (QT Reviewed)


Data File : VW011272.D
Acq On : 15 Jul 2019 20:12
Operator : SY/VA
Sample : K3798-12
Misc : 4.46G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A52J1

Manual Integrations
APPROVED

MMDadoda
7/18/2019 7:53:42 AM

Quant Time: Jul 16 07:24:28 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 05:02:41 2019
Response via : Initial Calibration

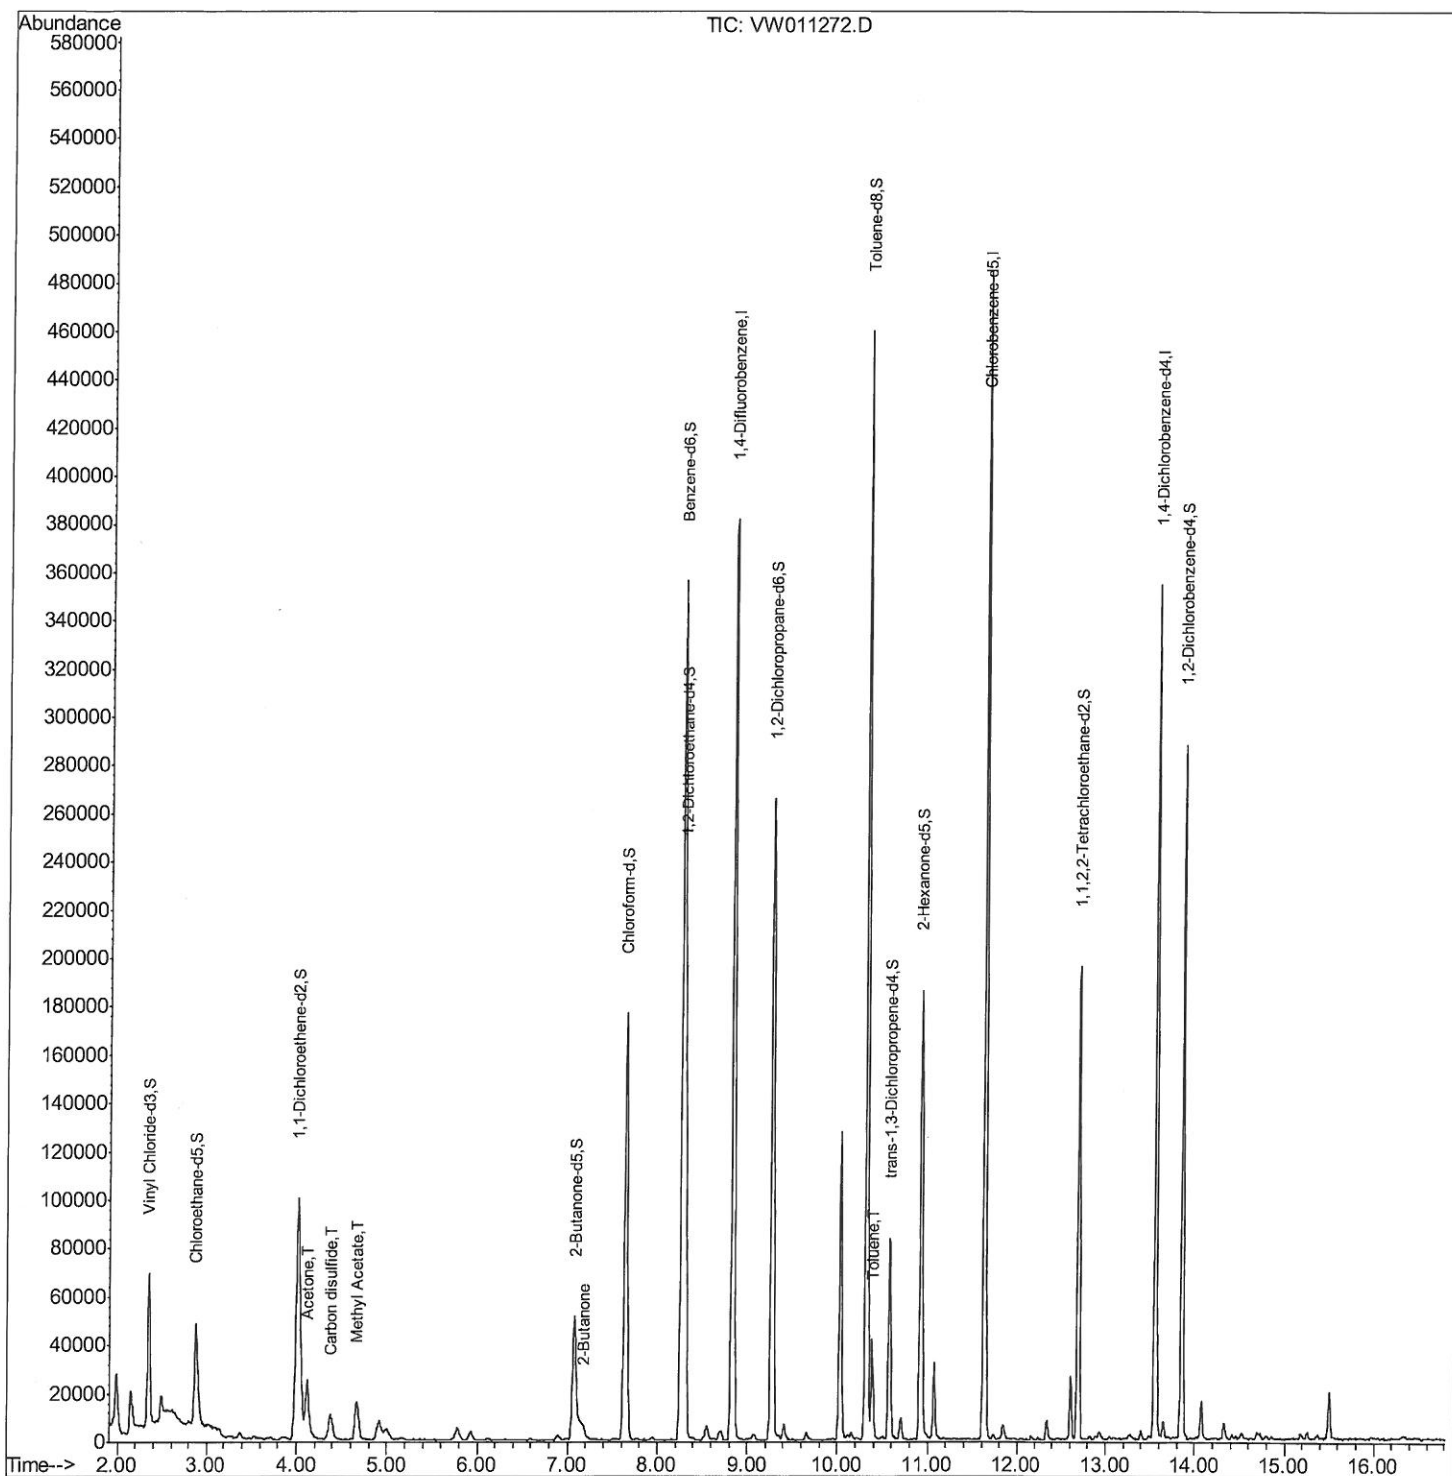

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW071519\
Quantitation Report (Qedit)




Data File : VW011272.D
Acq On : 15 Jul 2019 20:12
Operator : SY/VA
Sample : K3798-12
Misc : 4.46G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A52J1

Manual Integrations
APPROVED

MMDadoda
7/18/2019 7:53:42 AM

Quant Time: Jul 16 05:07:32 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 05:02:41 2019
Response via : Initial Calibration

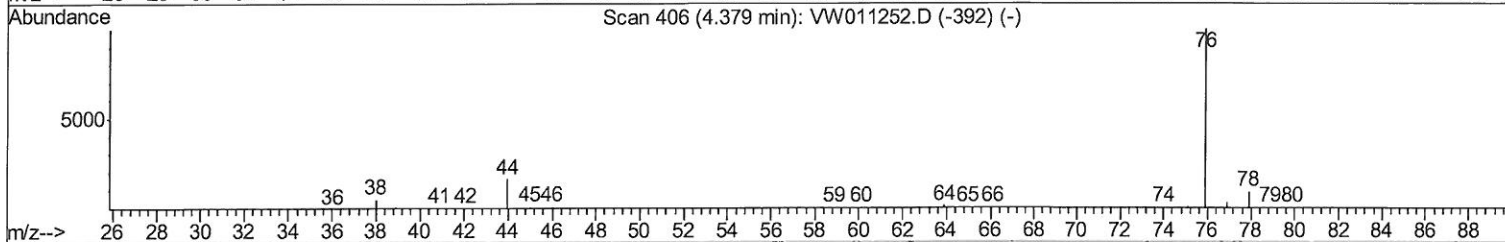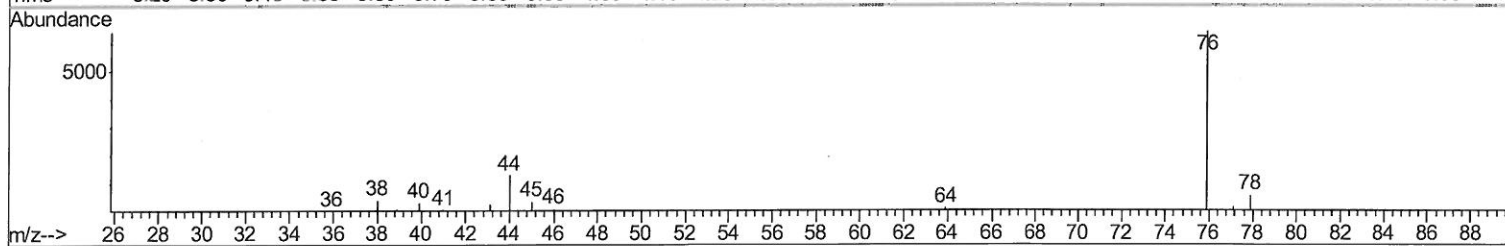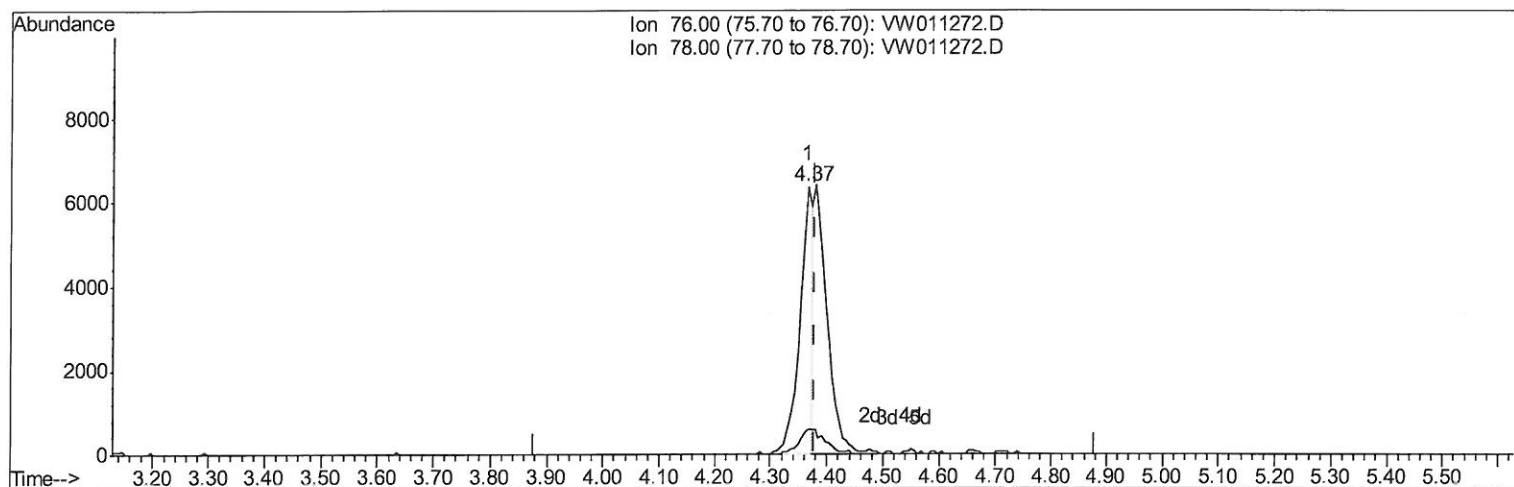

TIC: VW011272.D

(14) Carbon disulfide (T)

4.367min (-0.012) 0.88ug/L

response 9871

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	9.28
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW071519\
Quantitation Report (Qedit)




Data File : VW011272.D
Acq On : 15 Jul 2019 20:12
Operator : SY/VA
Sample : K3798-12
Misc : 4.46G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A52J1

Manual Integrations
APPROVED

MMDadoda
7/18/2019 7:53:42 AM

Quant Time: Jul 16 05:07:32 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 05:02:41 2019
Response via : Initial Calibration

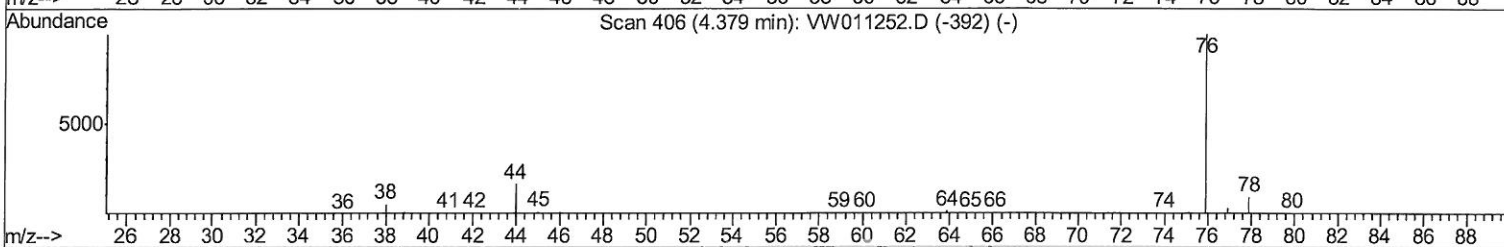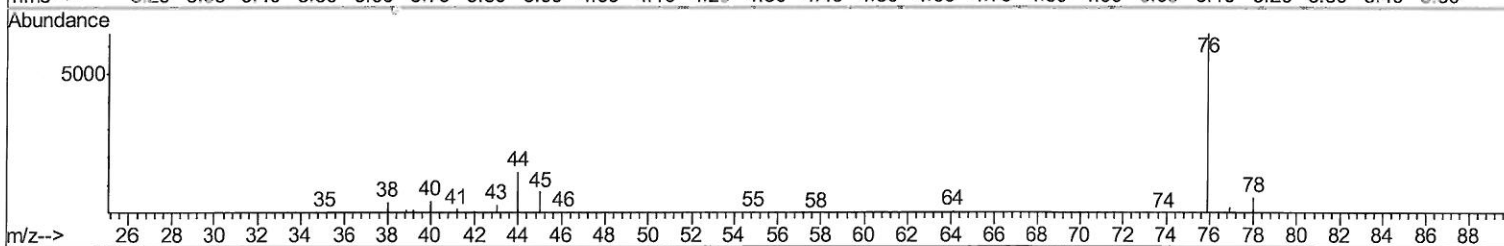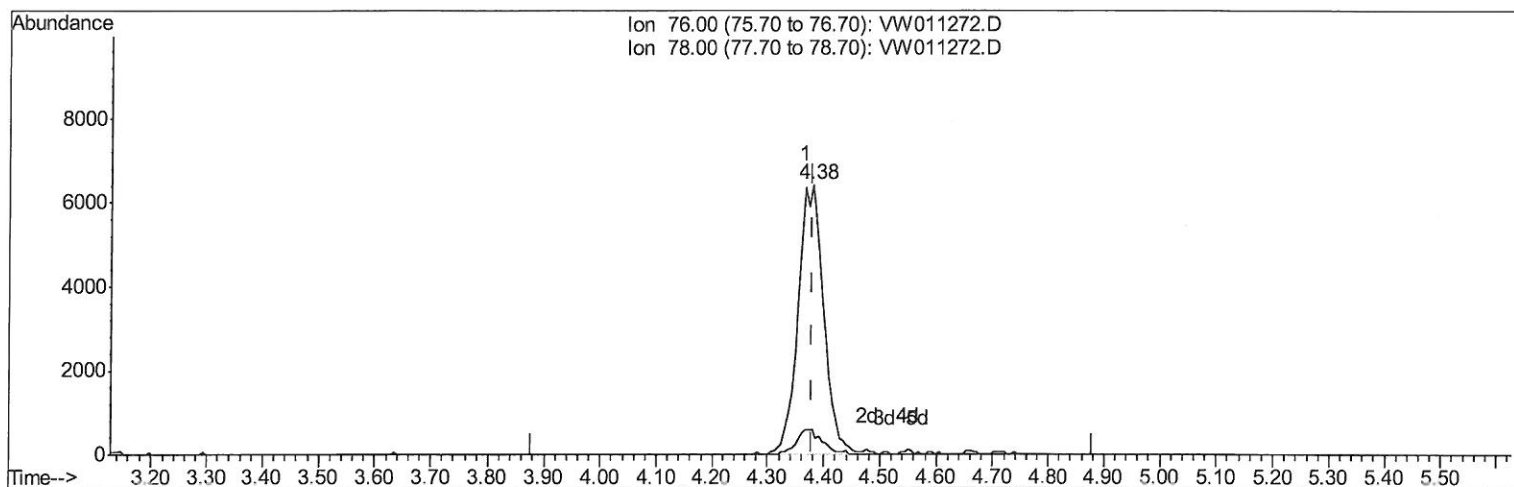

TIC: VW011272.D

(14) Carbon disulfide (T)

4.379min (-0.000) 1.81ug/L m

response 20258

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	8.95
0.00	0.00	0.00
0.00	0.00	0.00

7 MB
7/13/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW071519\
Quantitation Report (Qedit)




Data File : VW011272.D
Acq On : 15 Jul 2019 20:12
Operator : SY/VA
Sample : K3798-12
Misc : 4.46G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A52J1

Manual Integrations
APPROVED

MMDadoda
7/18/2019 7:53:42 AM

Quant Time: Jul 16 05:07:32 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 05:02:41 2019
Response via : Initial Calibration

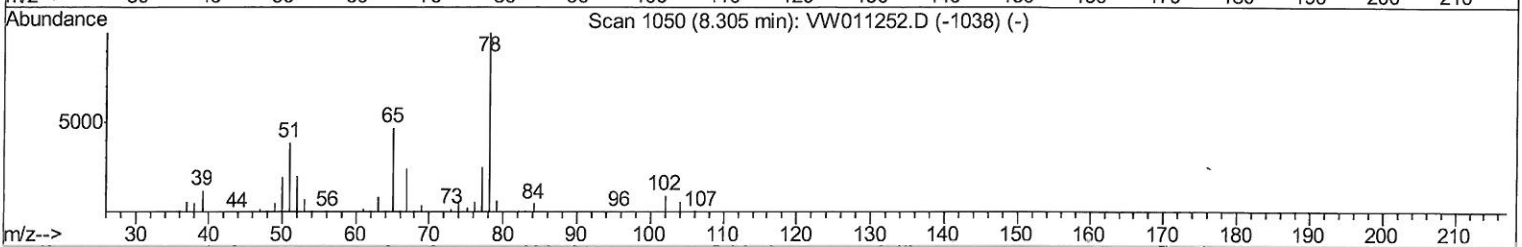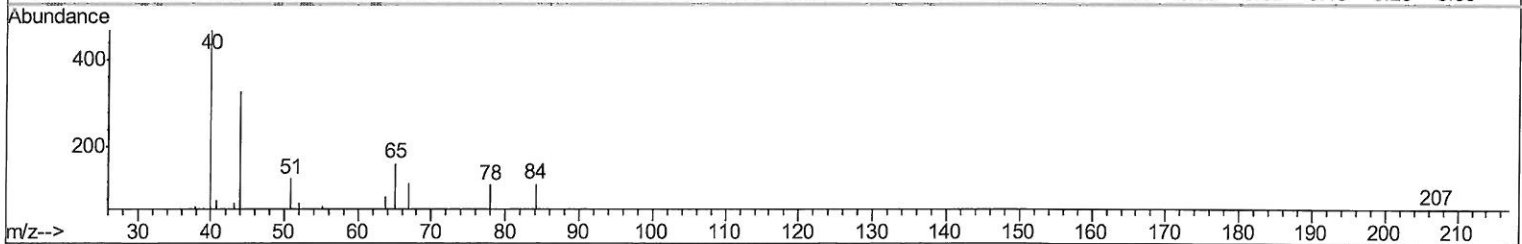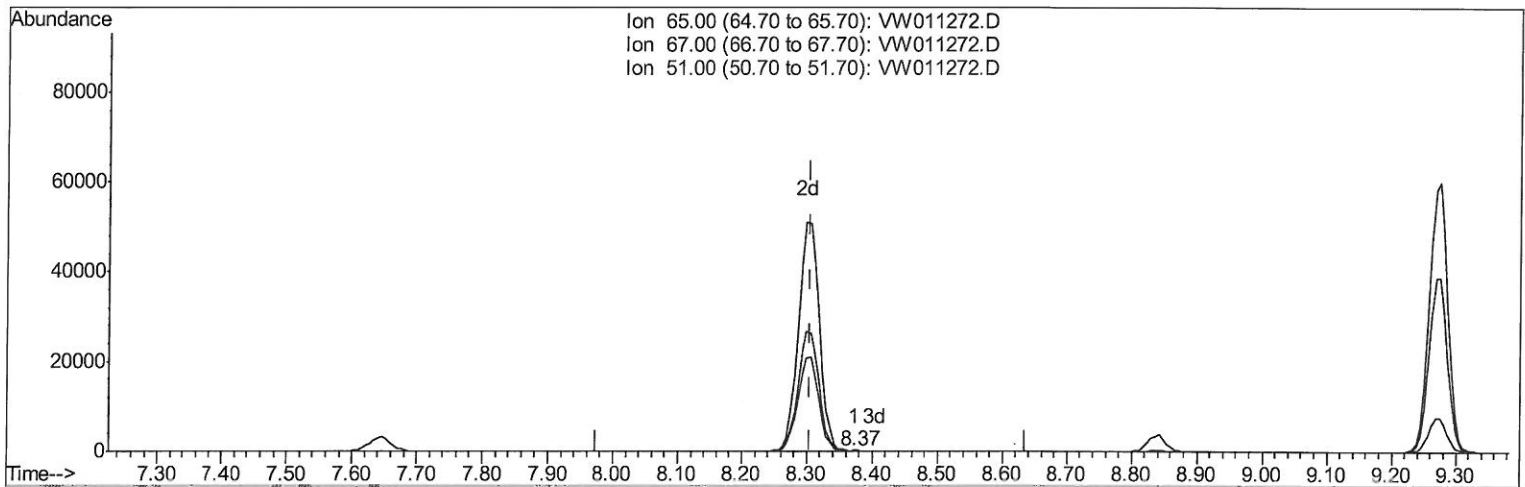

TIC: VW011272.D

(26) 1,2-Dichloroethane-d4 (S)

8.372min (+0.067) 0.03ug/L

response 144

Ion	Exp%	Act%
65.00	100	100
67.00	52.40	68.06
51.00	100.70	90.28
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW071519\
Quantitation Report (Qedit)




Data File : VW011272.D
Acq On : 15 Jul 2019 20:12
Operator : SY/VA
Sample : K3798-12
Misc : 4.46G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A52J1

Manual Integrations
APPROVED

MMDadoda
7/18/2019 7:53:42 AM

Quant Time: Jul 16 05:07:32 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 16 05:02:41 2019
Response via : Initial Calibration

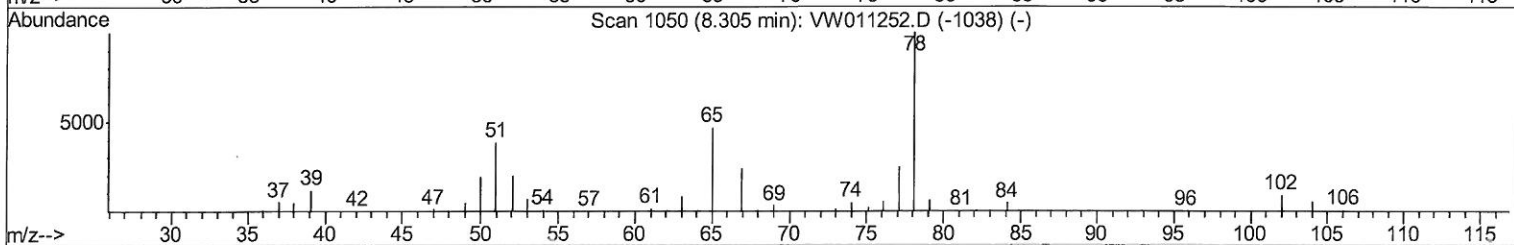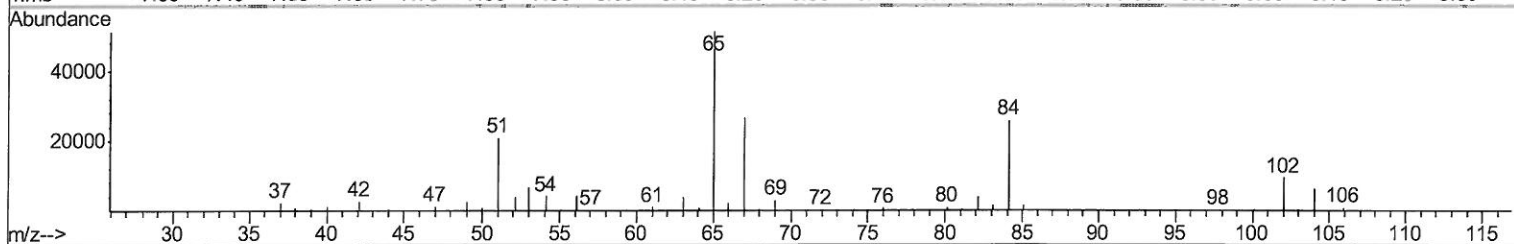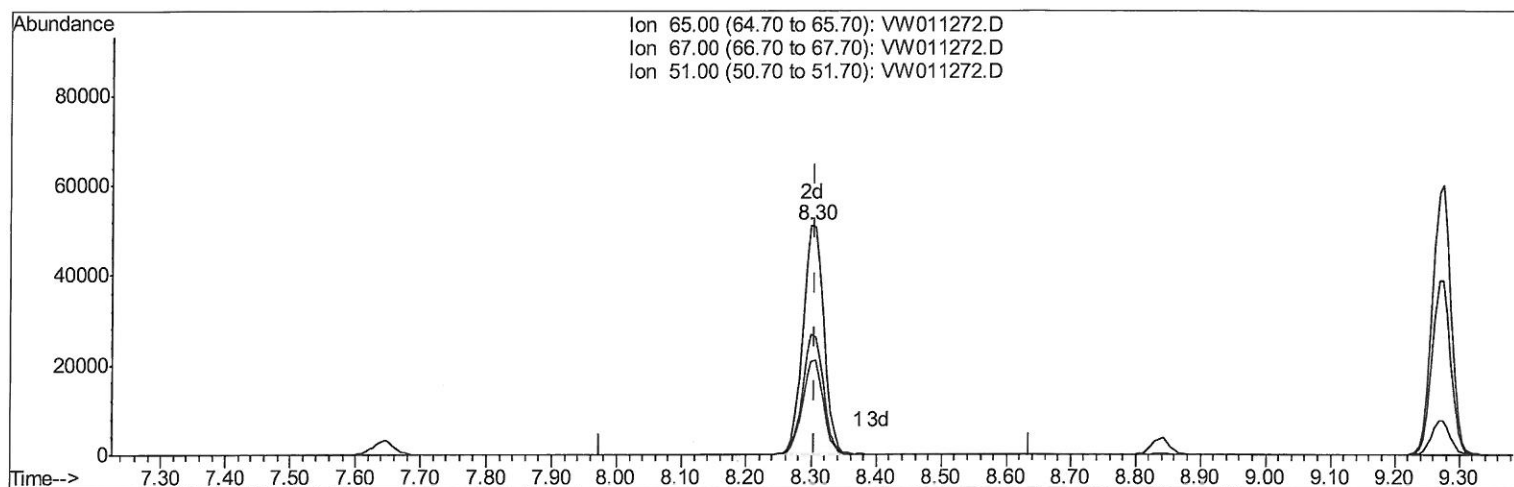

TIC: VW011272.D

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.006) 22.64ug/L m

response 113815

Ion	Exp%	Act%
65.00	100	100
67.00	52.40	0.09#
51.00	100.70	0.11#
0.00	0.00	0.00

7 MD
7/31/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW071519\

Quantitation Report (QT Reviewed)

Data File : VW011272.D

Acq On : 15 Jul 2019 20:12

Operator : SY/VA

Sample : K3798-12

Misc : 4.46G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Instrument :

MSVOA_W

ClientSampleId :

A52J1

Manual Integrations
APPROVEDMMDadoda
7/18/2019 7:53:42 AM

Quant Time: Jul 16 07:24:28 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M

Quant Title : VOC Analysis

QLast Update : Tue Jul 16 05:02:41 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	297842	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	246724	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	88219	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.34	65	68718	15.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.44%
7) Chloroethane-d5	2.88	69	58541	18.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.40%
10) 1,1-Dichloroethene-d2	4.01	63	125297	13.01	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.04%
20) 2-Butanone-d5	7.07	46	92402	51.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.16%
24) Chloroform-d	7.65	84	174737	21.40	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.60%
26) 1,2-Dichloroethane-d4	8.30	65	113815m	22.64	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.56%
29) Benzene-d6	8.27	84	342910	22.56	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.24%
33) 1,2-Dichloropropane-d6	9.27	67	119572	24.16	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.64%
37) Toluene-d8	10.32	98	282285	20.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.36%
38) trans-1,3-Dichloropropene-	10.58	79	43659	20.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.96%
39) 2-Hexanone-d5	10.92	63	61430	54.12	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.24%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	96019	23.45	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.80%
61) 1,2-Dichlorobenzene-d4	13.85	152	70785	20.90	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.60%

Target Compounds

Target Compounds					Qvalue
13) Acetone	4.12	43	41572	23.757	ug/L 98
14) Carbon disulfide	4.38	76	20258m	1.809	ug/L
15) Methyl Acetate	4.67	43	31863	11.190	ug/L 99
21) 2-Butanone	7.17	43	9075	4.017	ug/L 89
44) Toluene	10.38	91	28127	1.762	ug/L 99

(#)=qualifier out of range (m)=manual integration (+)=signals summed