


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071519\
Data File : VW011251.D
Acq On : 15 Jul 2019 09:47
Operator : SY/VA
Sample : BFB26
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB26

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Title : VOC Analysis
Last Update : Wed Jul 17 07:20:32 2019

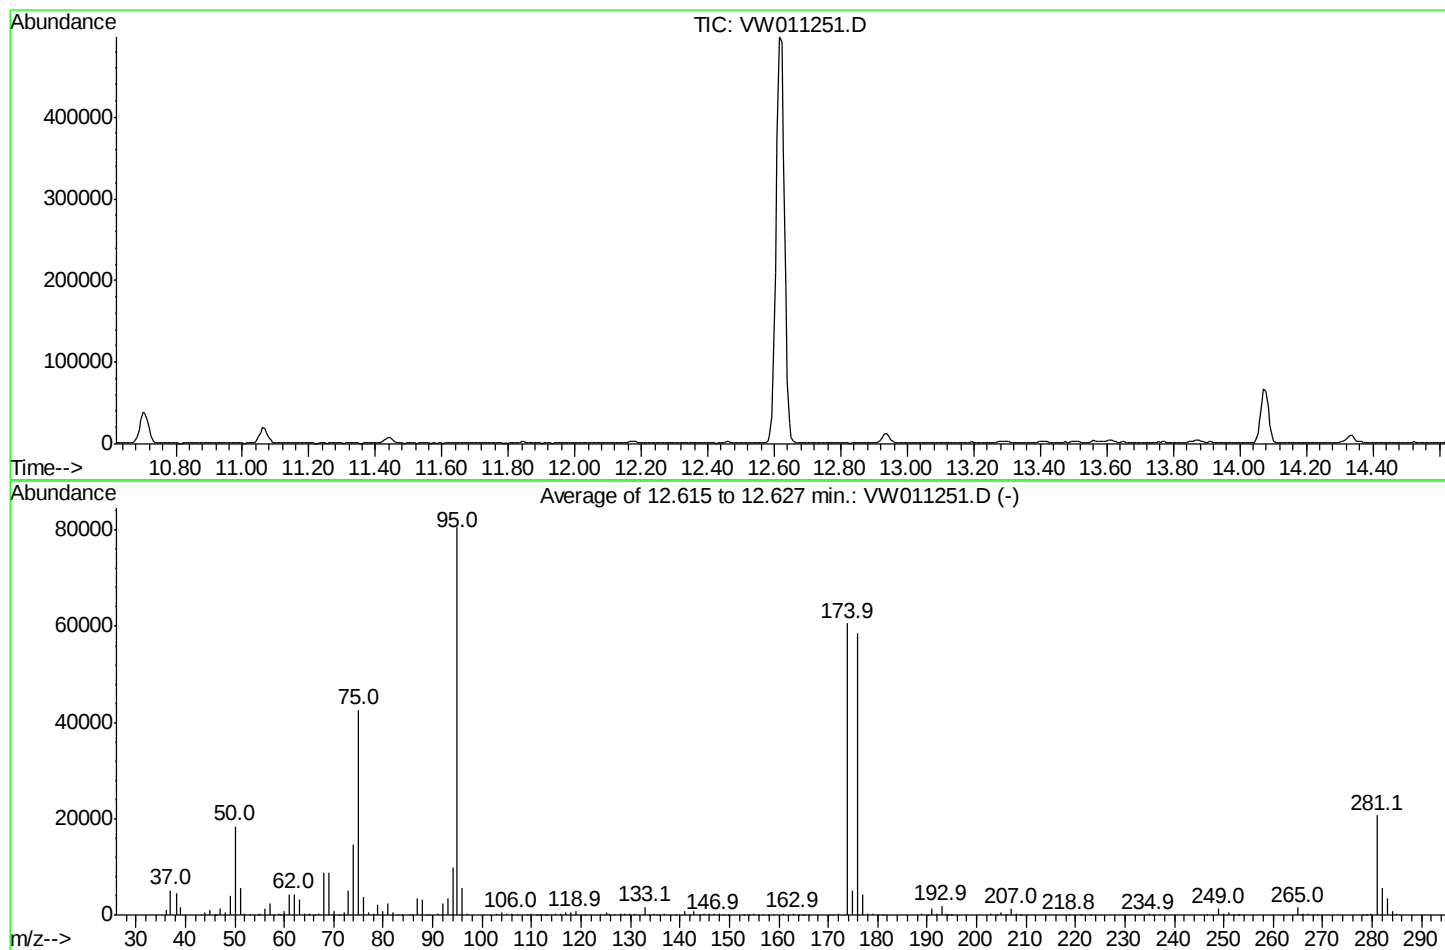

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	18471	PASS
75	95	30	80	52.9	42648	PASS
95	95	100	100	100.0	80562	PASS
96	95	5	9	6.8	5506	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.3	60648	PASS
175	174	5	9	8.4	5085	PASS
176	174	95	101	96.6	58565	PASS
177	176	5	9	7.1	4139	PASS

Scan 1749 (12.566 min): VW011251.D
BFB26

m/z	Abundance
38.90	101.0
39.90	403.0
41.10	107.0
41.90	80.0
43.10	114.0
44.00	317.0
57.10	86.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

m/z	Abundance
36.10	1069.0
37.00	5770.0
38.10	5314.0
39.10	2242.0
40.00	478.0
41.10	74.0
42.10	58.0
43.00	248.0
44.00	914.0
45.00	1358.0
45.90	194.0
47.00	1309.0
48.00	637.0
49.10	4364.0
50.00	21088.0
51.10	6563.0
52.00	398.0
53.00	118.0
55.00	312.0
56.00	1360.0
57.00	2707.0
58.00	155.0
59.00	593.0
60.10	905.0
61.00	4589.0
62.00	4743.0
63.00	3270.0
64.00	412.0
65.00	255.0
66.20	64.0
66.90	332.0
68.00	9778.0
69.00	9493.0
70.00	716.0
71.10	90.0
72.00	585.0
73.00	6345.0
74.00	16179.0
75.00	46424.0
76.00	3933.0
77.00	421.0
78.00	359.0
78.90	2452.0
79.90	637.0
80.90	2472.0
82.00	707.0
83.10	118.0
83.70	176.0
85.30	65.0
85.90	159.0
87.00	3566.0
87.90	3507.0
89.20	57.0
90.80	307.0
92.00	2465.0
93.00	3630.0
94.00	10026.0
95.00	86272.0
96.00	6215.0
97.00	236.0
103.00	466.0
103.80	485.0
104.90	312.0
106.00	401.0
107.00	146.0
109.90	229.0
111.20	201.0
111.60	177.0
112.10	128.0
113.10	124.0
114.90	272.0
116.00	344.0
116.90	562.0
118.00	577.0
118.90	848.0
119.90	94.0
120.90	136.0
124.00	58.0
125.10	650.0
125.80	275.0
126.80	67.0
127.90	269.0
128.90	168.0
129.80	329.0
130.90	194.0
133.00	2965.0
134.90	262.0
135.80	71.0
136.80	160.0
140.90	664.0
142.10	144.0
142.90	620.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

144.20	66.0
144.80	228.0
145.90	153.0
146.90	312.0
147.80	234.0
148.70	147.0
149.70	79.0
152.90	101.0
154.00	86.0
154.90	130.0
156.90	193.0
158.80	122.0
161.00	262.0
163.00	446.0
164.00	65.0
165.10	261.0
166.00	73.0
170.20	68.0
172.00	493.0
174.00	59880.0
175.00	5029.0
175.90	57600.0
177.00	4394.0
178.00	409.0
179.00	557.0
180.00	171.0
181.00	57.0
188.80	204.0
190.10	173.0
191.00	2327.0
192.00	678.0
193.00	3122.0
193.80	565.0
194.90	380.0
202.90	329.0
204.10	68.0
205.00	574.0
206.00	176.0
207.10	1777.0
208.00	388.0
208.90	188.0
218.80	121.0
220.90	98.0
223.00	69.0
234.90	337.0
235.80	91.0
237.00	77.0
246.70	74.0
249.00	1957.0
250.00	364.0
250.90	850.0
252.00	131.0
253.00	88.0
265.00	2187.0
266.10	660.0
267.10	692.0
268.10	98.0
268.80	91.0
278.80	146.0
279.70	523.0
281.10	30208.0
282.00	8414.0
283.00	5297.0
284.00	1037.0
285.00	260.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

m/z	Abundance
36.00	1098.0
37.00	5421.0
38.10	4812.0
39.00	1897.0
39.90	367.0
41.10	100.0
42.90	152.0
44.00	831.0
45.10	1102.0
46.20	122.0
47.10	1413.0
48.00	661.0
49.00	4456.0
50.00	20368.0
51.00	6212.0
52.00	264.0
55.10	297.0
56.00	1449.0
57.00	2724.0
58.00	112.0
59.20	259.0
60.00	1039.0
61.00	4663.0
62.00	4849.0
63.00	3541.0
64.00	339.0
65.10	202.0
66.90	321.0
68.00	9772.0
69.00	9909.0
70.10	808.0
72.00	651.0
73.00	5013.0
74.00	16045.0
75.00	47504.0
76.00	4022.0
77.10	619.0
78.00	391.0
78.90	2526.0
80.00	786.0
80.90	2545.0
81.90	490.0
86.00	88.0
87.00	3888.0
88.00	3377.0
88.70	219.0
90.90	368.0
92.00	2579.0
93.10	3742.0
94.00	11217.0
95.00	89272.0
96.00	6052.0
97.10	151.0
103.00	388.0
103.90	458.0
104.90	227.0
105.90	334.0
106.90	101.0
109.10	53.0
110.00	135.0
110.90	264.0
112.10	115.0
113.00	117.0
115.00	227.0
115.90	239.0
117.00	637.0
117.90	416.0
118.90	686.0
125.20	473.0
125.80	151.0
126.90	72.0
128.00	287.0
128.80	182.0
129.80	359.0
130.80	184.0
133.10	1410.0
133.80	395.0
134.90	371.0
135.80	65.0
136.80	248.0
139.10	57.0
140.90	1035.0
142.00	114.0
142.90	903.0
143.80	52.0
144.80	105.0
145.90	205.0
146.90	243.0
147.90	205.0
148.80	148.0
149.90	68.0
152.70	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

154.90	210.0
155.90	66.0
156.80	127.0
158.90	156.0
160.90	159.0
162.90	263.0
164.80	282.0
170.10	57.0
171.00	111.0
172.00	378.0
173.90	67208.0
175.00	5723.0
175.90	64784.0
176.90	4592.0
178.00	176.0
179.00	336.0
180.10	157.0
188.80	180.0
191.00	1363.0
192.90	1984.0
194.00	411.0
195.10	208.0
202.90	276.0
204.00	81.0
204.90	517.0
206.00	143.0
206.90	1256.0
208.10	237.0
208.90	188.0
218.70	81.0
221.10	55.0
234.90	227.0
246.70	77.0
249.00	1157.0
250.00	393.0
251.00	631.0
251.90	103.0
252.70	87.0
265.00	1504.0
266.00	424.0
267.00	337.0
268.10	149.0
278.10	56.0
278.60	111.0
281.00	21536.0
282.00	5965.0
283.00	3659.0
284.10	768.0
285.00	238.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

m/z	Abundance
36.00	863.0
37.00	4101.0
38.10	3394.0
39.10	1356.0
39.90	323.0
41.10	77.0
42.00	82.0
44.00	718.0
45.00	963.0
46.00	68.0
47.00	999.0
48.00	524.0
49.00	2856.0
50.00	13958.0
51.00	4062.0
52.00	188.0
54.80	238.0
56.00	1195.0
57.00	1835.0
57.80	101.0
58.90	82.0
60.00	621.0
61.00	3621.0
62.00	3309.0
63.00	2521.0
64.10	281.0
64.80	103.0
65.20	99.0
67.00	243.0
68.00	6468.0
69.00	6860.0
70.00	505.0
72.00	500.0
73.00	3619.0
74.00	11620.0
75.00	34016.0
76.00	2884.0
77.10	582.0
77.80	273.0
78.90	1786.0
80.00	624.0
81.00	1966.0
81.90	461.0
82.90	96.0
86.00	78.0
87.00	2578.0
87.90	3080.0
91.00	269.0
91.90	1783.0
93.00	2816.0
94.00	7961.0
95.00	66144.0
96.00	4252.0
97.00	143.0
102.90	124.0
104.00	293.0
104.90	94.0
106.00	294.0
110.00	96.0
111.00	105.0
111.70	78.0
112.80	53.0
114.90	157.0
115.90	299.0
116.90	436.0
118.00	322.0
118.90	533.0
124.70	174.0
125.10	211.0
125.70	65.0
127.90	298.0
128.90	141.0
129.80	178.0
130.90	116.0
132.90	673.0
134.70	195.0
135.20	80.0
136.70	97.0
139.10	86.0
140.90	726.0
142.90	781.0
144.90	149.0
145.90	110.0
146.80	135.0
147.90	236.0
148.80	125.0
149.90	74.0
153.00	80.0
154.90	196.0
155.90	73.0
156.80	90.0
157.90	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26

158.90	122.0
160.80	138.0
163.00	186.0
164.90	118.0
171.00	95.0
172.00	337.0
173.90	54856.0
175.00	4503.0
176.00	53312.0
177.00	3432.0
177.90	198.0
179.00	218.0
188.80	89.0
190.90	522.0
191.90	215.0
193.00	759.0
193.80	189.0
194.20	108.0
195.00	95.0
202.90	150.0
205.00	171.0
206.90	637.0
208.10	108.0
209.10	127.0
218.70	55.0
234.80	103.0
249.00	531.0
249.80	163.0
250.90	196.0
265.00	752.0
265.80	298.0
267.10	190.0
278.90	102.0
281.10	10275.0
282.00	2658.0
283.00	1774.0
284.00	414.0
285.10	97.0

Instrument :
MSVOA_W
ClientSampleId :
BFB26