

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071524\
 Data File : VW029576.D
 Acq On : 15 Jul 2024 15:37
 Operator : SY/MD
 Sample : P3201-21
 Misc : 5.29g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4DA5

Quant Time: Jul 16 00:01:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jul 15 23:59:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	328757	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	213297	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	60807	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	81074	15.266	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.080%
7) Chloroethane-d5	2.893	69	64190	16.786	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.160%
11) 1,1-Dichloroethene-d2	4.021	65	38083	15.969	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.880%
21) 2-Butanone-d5	7.081	46	63574	39.877	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.760%
24) Chloroform-d	7.648	84	164965	17.357	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	69.440%
26) 1,2-Dichloroethane-d4	8.307	65	106984	19.191	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	76.760%
32) Benzene-d6	8.276	84	315306	24.676	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.720%
36) 1,2-Dichloropropane-d6	9.270	67	105617	25.852	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.400%
41) Toluene-d8	10.318	98	224159	19.948	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.800%
43) trans-1,3-Dichloroprop...	10.575	79	32744	18.927	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.720%
47) 2-Hexanone-d5	10.922	63	43013	57.939	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.880%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	67909	20.473	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.880%
66) 1,2-Dichlorobenzene-d4	13.848	152	35052	16.552	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	66.200%#
Target Compounds						
					Qvalue	
13) Acetone	4.124	43	43320	26.922	ug/L	96
14) Carbon disulfide	4.387	76	13583	1.023	ug/L	98
22) 2-Butanone	7.173	43	20222	9.573	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071524\
Data File : VW029576.D
Acq On : 15 Jul 2024 15:37
Operator : SY/MD
Sample : P3201-21
Misc : 5.29g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4DA5

Quant Time: Jul 16 00:01:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jul 15 23:59:48 2024
Response via : Initial Calibration

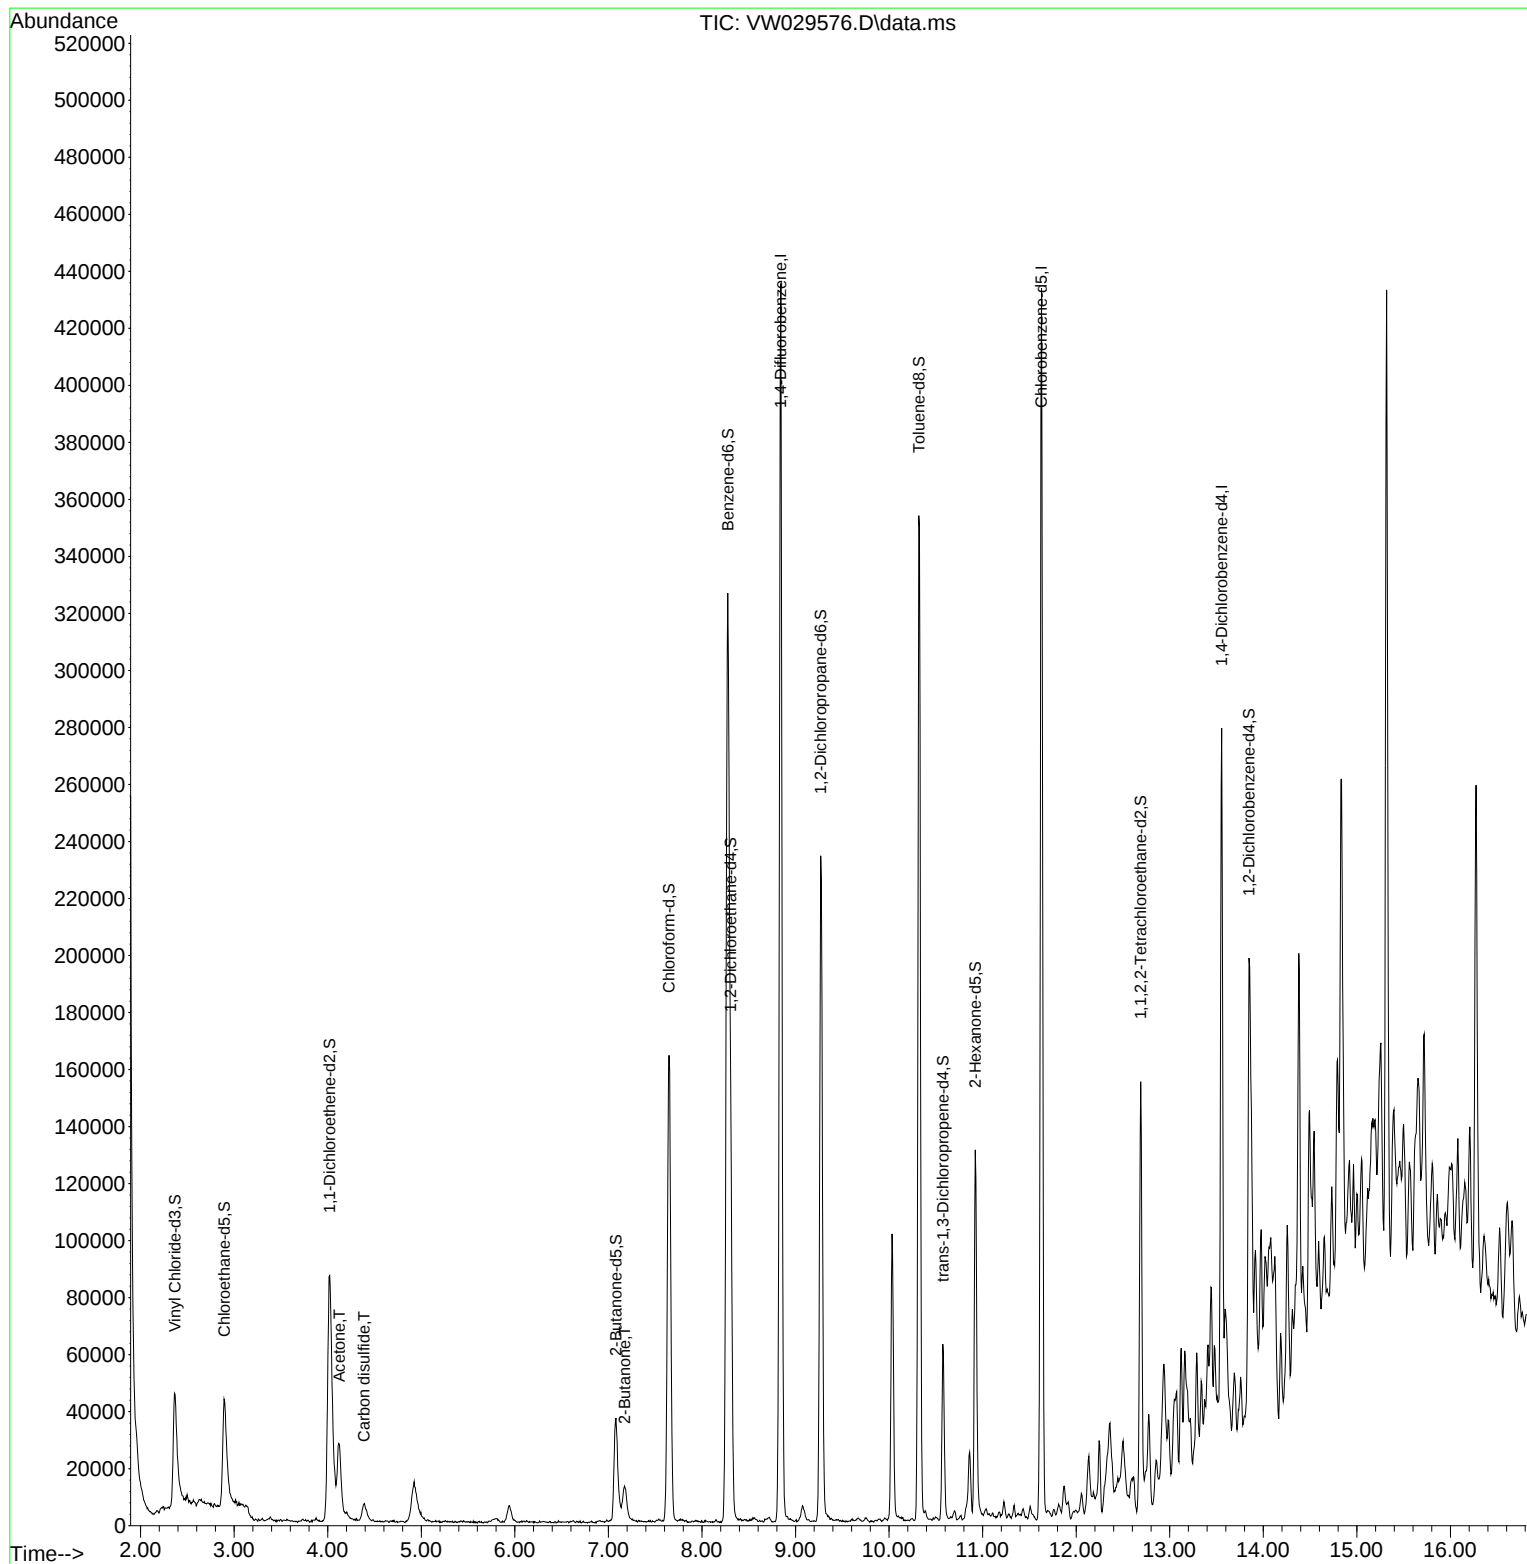

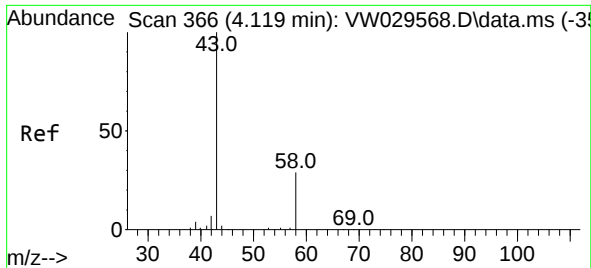

#13

Acetone

Concen: 26.922 ug/L

RT: 4.124 min Scan# 3

Delta R.T. 0.006 min

Lab File: VW029576.D

Acq: 15 Jul 2024 15:37

Instrument :

MSVOA_W

ClientSampleId :





A4DA5

Tgt Ion: 43 Resp: 43320

Ion Ratio Lower Upper

43 100

58 29.7 0.0 55.6

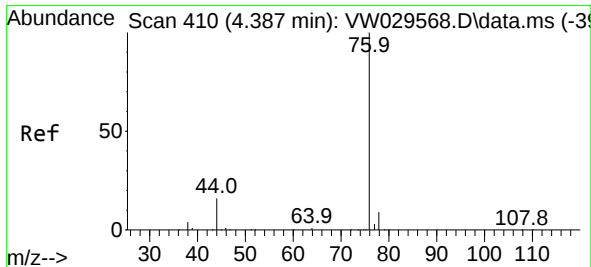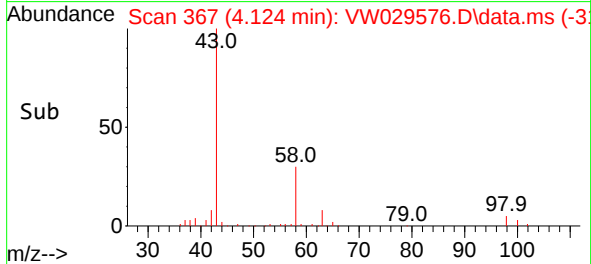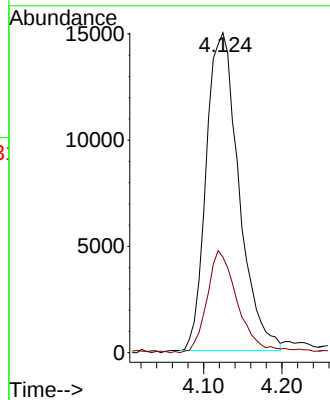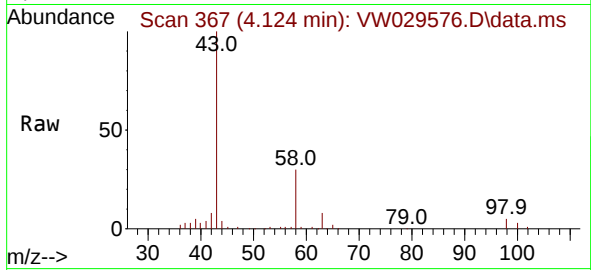

#14

Carbon disulfide

Concen: 1.023 ug/L

RT: 4.387 min Scan# 410

Delta R.T. -0.000 min

Lab File: VW029576.D




Acq: 15 Jul 2024 15:37


Tgt Ion: 76 Resp: 13583

Ion Ratio Lower Upper

76 100

78 8.1 7.0 10.4

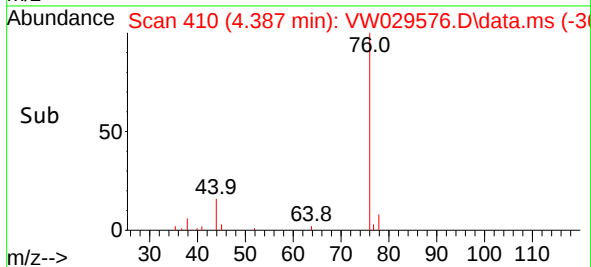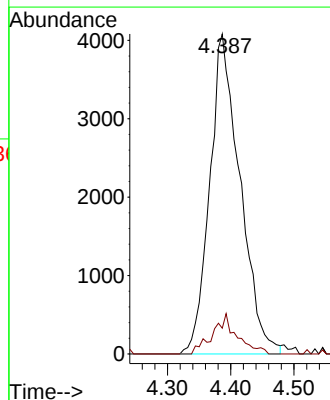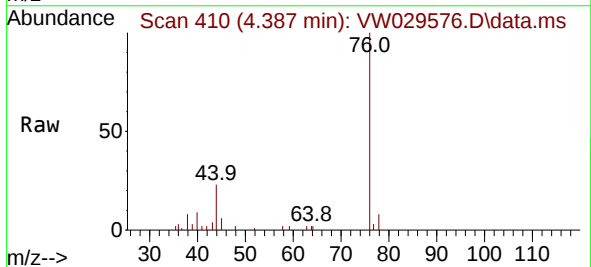

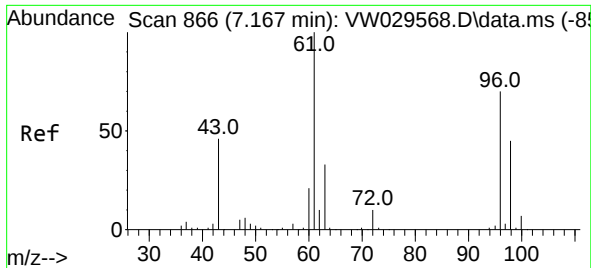

#22
 2-Butanone
 Concen: 9.573 ug/L
 RT: 7.173 min Scan# 80
 Delta R.T. 0.006 min
 Lab File: VW029576.D
 Acq: 15 Jul 2024 15:37

Instrument :
 MSVOA_W
 ClientSampleId :
 A4DA5

Tgt Ion: 43 Resp: 20222

Ion	Ratio	Lower	Upper
43	100		
72	22.0	12.0	36.1

