


Methylene Chloride

Response Ratio

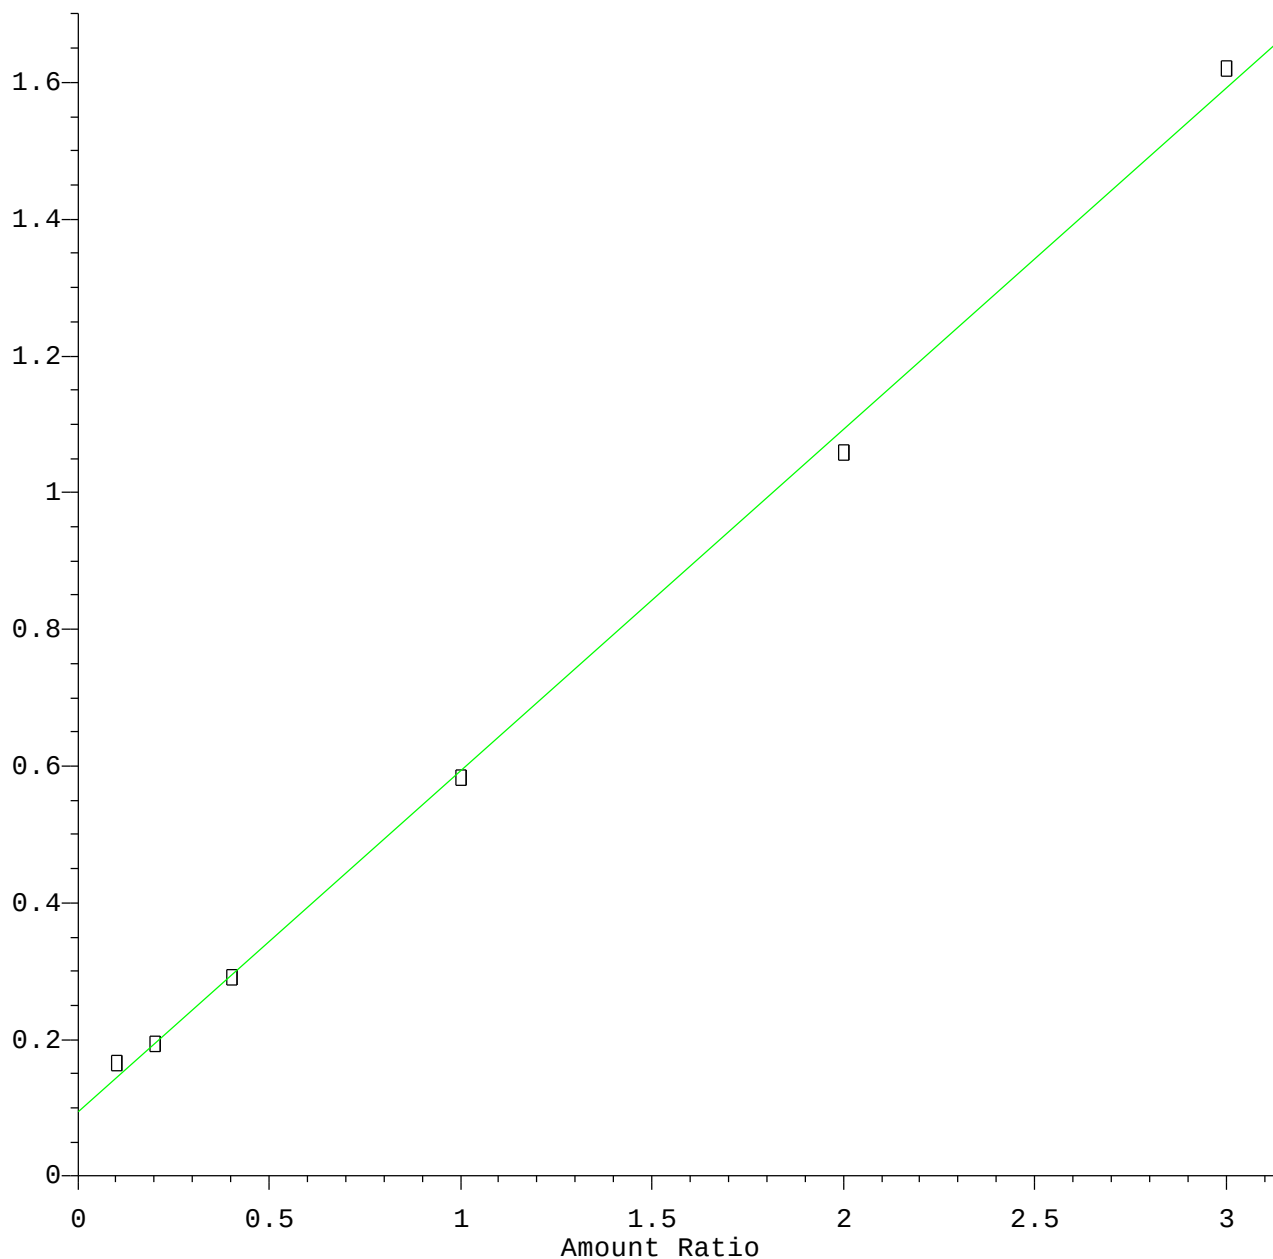

Resp Ratio = $5.00\text{e-}001 * \text{Amt} + 9.32\text{e-}002$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W071618S.M
Calibration Table Last Updated: Tue Jul 17 11:52:50 2018