


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW071618\
 Data File : VW003943.D
 Acq On : 16 Jul 2018 10:22
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W071618S.M
 Title : SW846 8260
 Last Update : Mon Jul 16 15:06:12 2018

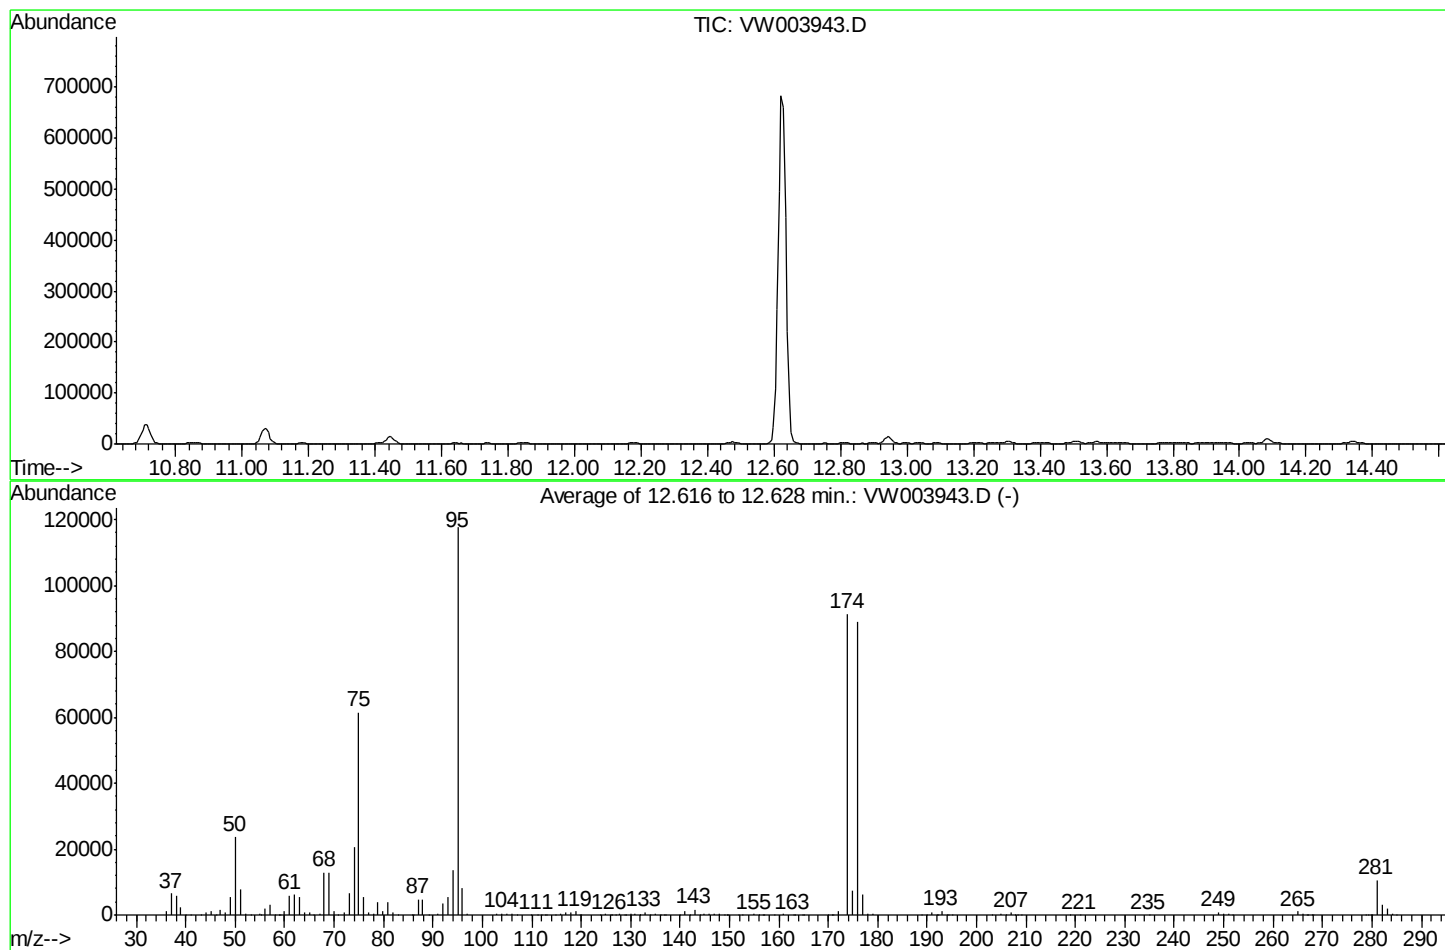

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	23816	PASS
75	95	30	60	52.3	61568	PASS
95	95	100	100	100.0	117674	PASS
96	95	5	9	6.8	8048	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.7	91434	PASS
175	174	5	9	8.0	7275	PASS
176	174	95	101	97.5	89176	PASS
177	176	5	9	7.1	6305	PASS