




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071624\
Data File : VW029595.D
Acq On : 16 Jul 2024 17:20
Operator : SY/MD
Sample : P3263-05
Misc : 5.21g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BA7

Manual IntegrationsAPPROVED

Reviewed By :Romaben
Patel

Quant Time: Jul 17 00:56:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 17 00:53:35 2024
Response via : Initial Calibration

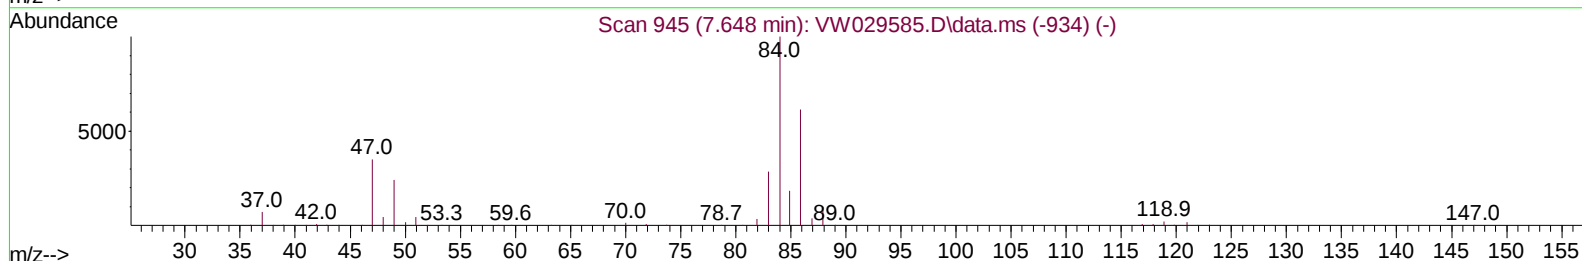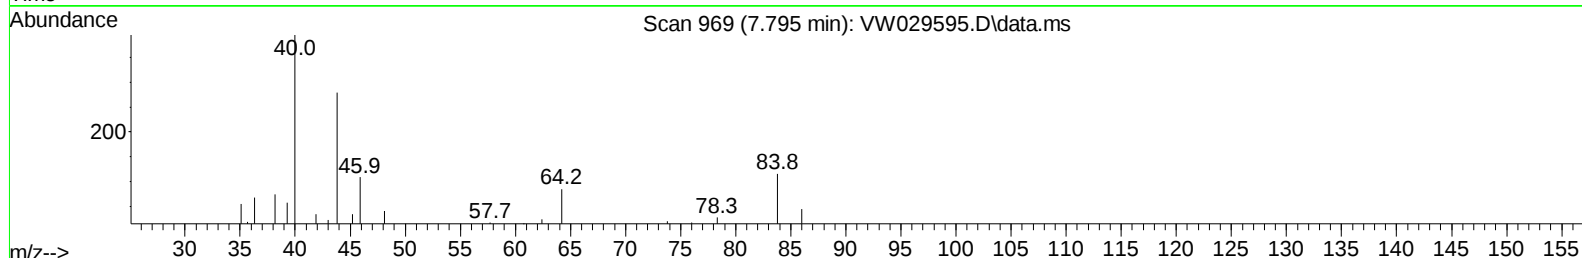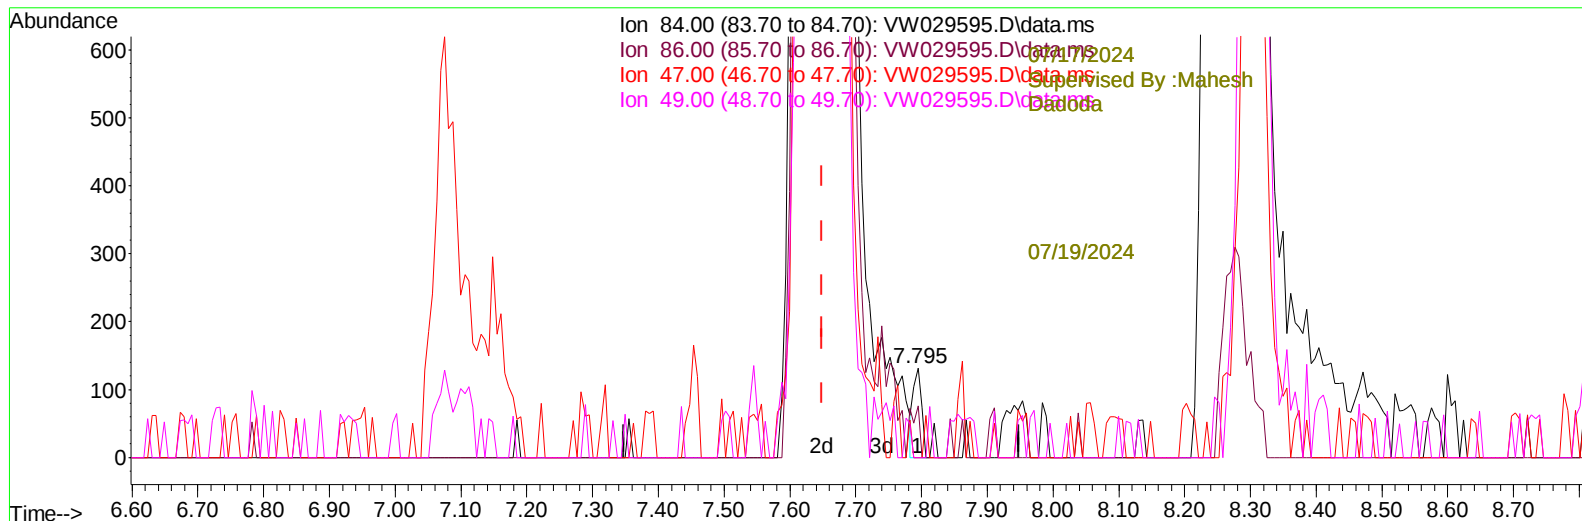

TIC: VW029595.D\data.ms

(24) Chloroform-d (S)

7.795min (+ 0.146) 0.01 ug/L

response 113

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	64.60
47.00	48.40	61.06
49.00	27.80	35.40




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071624\
 Data File : VW029595.D
 Acq On : 16 Jul 2024 17:20
 Operator : SY/MD
 Sample : P3263-05
 Misc : 5.21g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BA7

Manual IntegrationsAPPROVED

Quant Time: Jul 17 00:56:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 17 00:53:35 2024
 Response via : Initial Calibration

Reviewed By :Romaben
 Patel

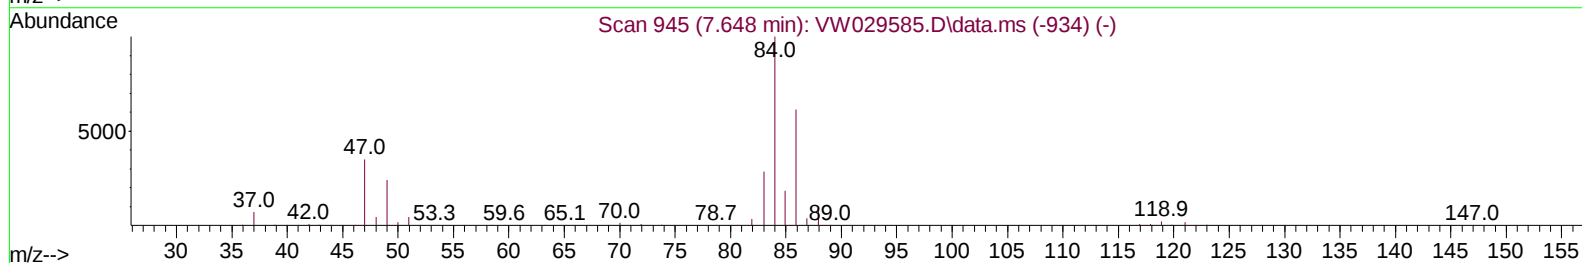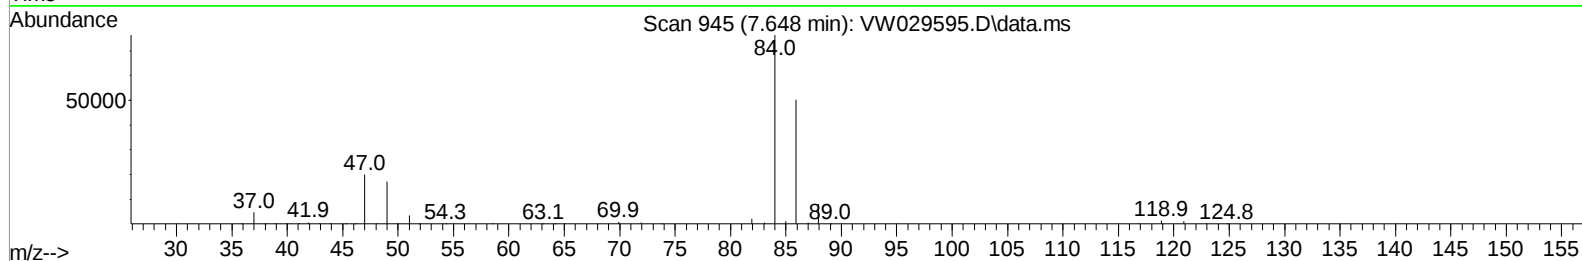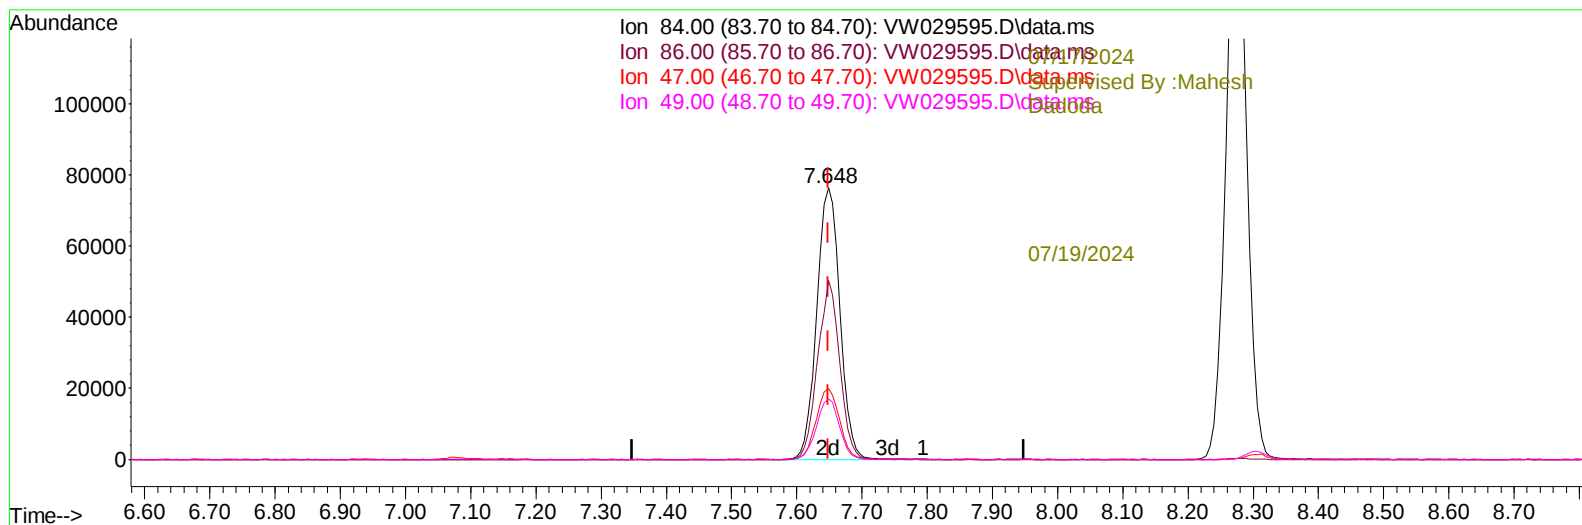

TIC: VW029595.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 15.14 ug/L m

response 188981

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	0.04#
47.00	48.40	0.04#
49.00	27.80	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071624\
 Data File : VW029595.D
 Acq On : 16 Jul 2024 17:20
 Operator : SY/MD
 Sample : P3263-05
 Misc : 5.21g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BA7

Manual IntegrationsAPPROVED

Quant Time: Jul 17 00:56:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 17 00:53:35 2024
 Response via : Initial Calibration

Reviewed By :Romaben
 Patel

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----07/17/2024							
Supervised By :Mahesh							
Padoda							
Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		431899	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		394769	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		179947	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		83162	11.919	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	47.680%		
7) Chloroethane-d5	2.899	69		67982	13.532	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	54.120%		
11) 1,1-Dichloroethene-d2	4.021	65		42540	13.578	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	54.320%		
21) 2-Butanone-d5	7.081	46		54351	25.950	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	51.900%		
24) Chloroform-d	7.648	84		188981m	15.136	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	60.560%		
26) 1,2-Dichloroethane-d4	8.307	65		111430	15.215	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	60.880%#		
32) Benzene-d6	8.276	84		357070	15.099	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	60.400%		
36) 1,2-Dichloropropane-d6	9.276	67		119423	15.794	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	63.160%#		
41) Toluene-d8	10.325	98		312090	15.006	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	60.040%		
43) trans-1,3-Dichloroprop...	10.575	79		41994	13.115	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	52.480%		
47) 2-Hexanone-d5	10.922	63		38693	28.161	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	56.320%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		91479	14.901	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	59.600%		
66) 1,2-Dichlorobenzene-d4	13.848	152		95724	15.275	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	61.080%#		
Target Compounds							
16) Methylene chloride	4.923	84		24365	3.151	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071624\
Data File : VW029595.D
Acq On : 16 Jul 2024 17:20
Operator : SY/MD
Sample : P3263-05
Misc : 5.21g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BA7

Manual IntegrationsAPPROVED

Quant Time: Jul 17 00:56:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 17 00:53:35 2024
Response via : Initial Calibration

Reviewed By :Romaben
Patel

