




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071624\
Data File : VW029600.D
Acq On : 16 Jul 2024 19:21
Operator : SY/MD
Sample : P3263-10
Misc : 5.47g/10mL/MSVOA_W/SoIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BD6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 07/17/2024
Supervised By :Mahesh Dadoda 07/19/2024

Quant Time: Jul 17 00:58:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 17 00:53:35 2024
Response via : Initial Calibration

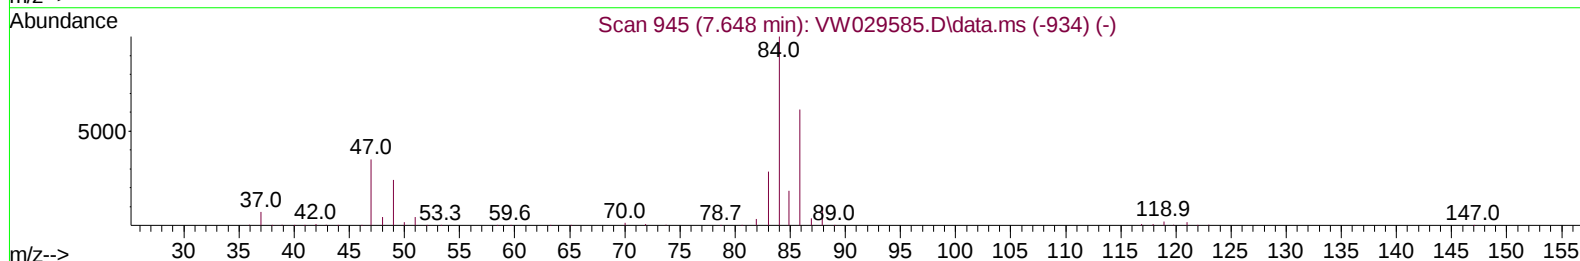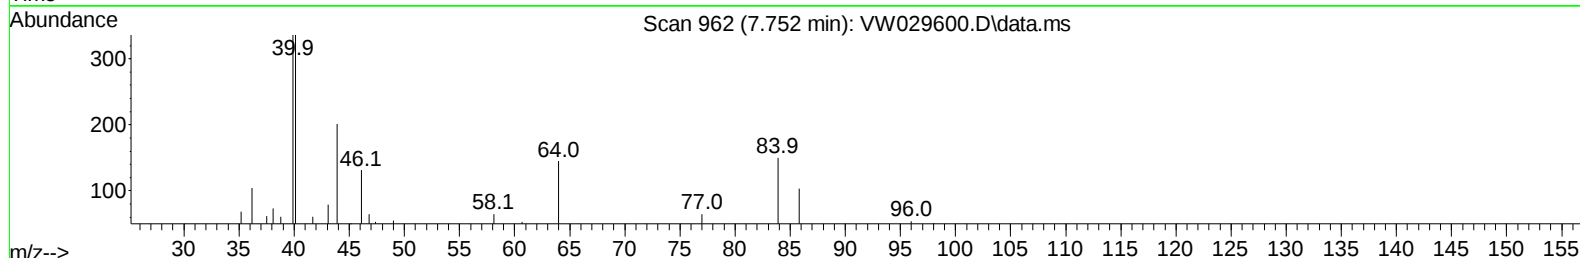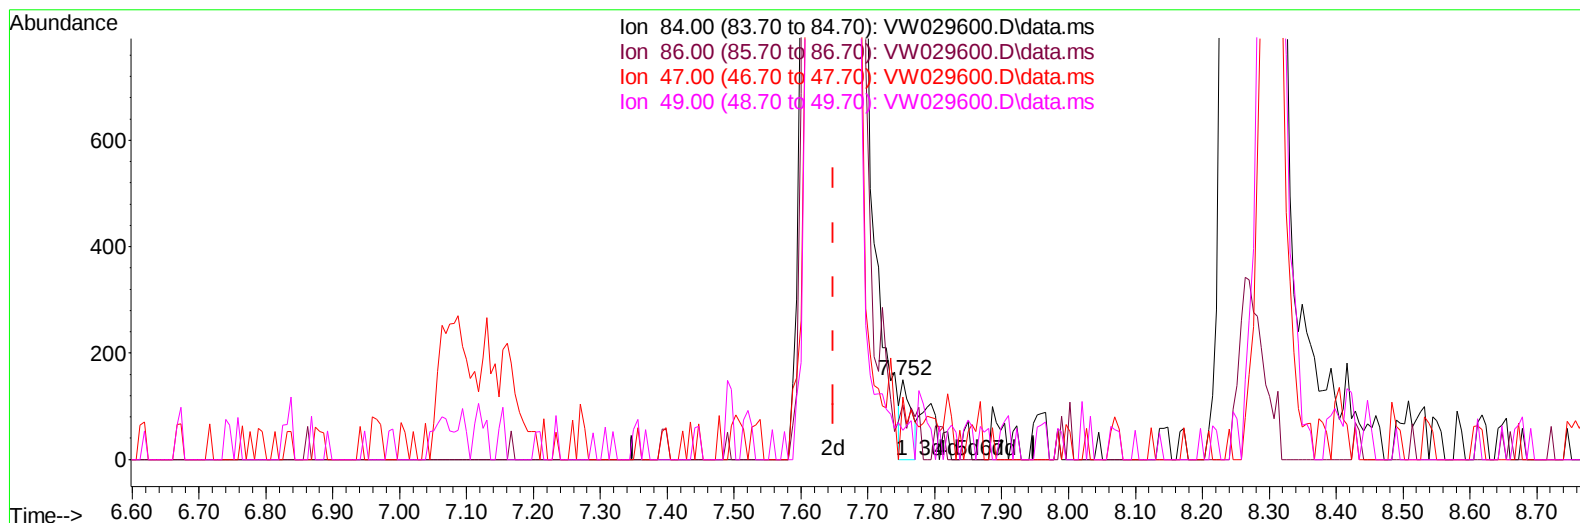

TIC: VW029600.D\data.ms

(24) Chloroform-d (S)

7.752min (+ 0.104) 0.01 ug/L

response 157

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	54.14
47.00	48.40	43.31
49.00	27.80	31.85




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071624\
Data File : VW029600.D
Acq On : 16 Jul 2024 19:21
Operator : SY/MD
Sample : P3263-10
Misc : 5.47g/10mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BD6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 07/17/2024
Supervised By :Mahesh Dadoda 07/19/2024

Quant Time: Jul 17 00:58:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 17 00:53:35 2024
Response via : Initial Calibration

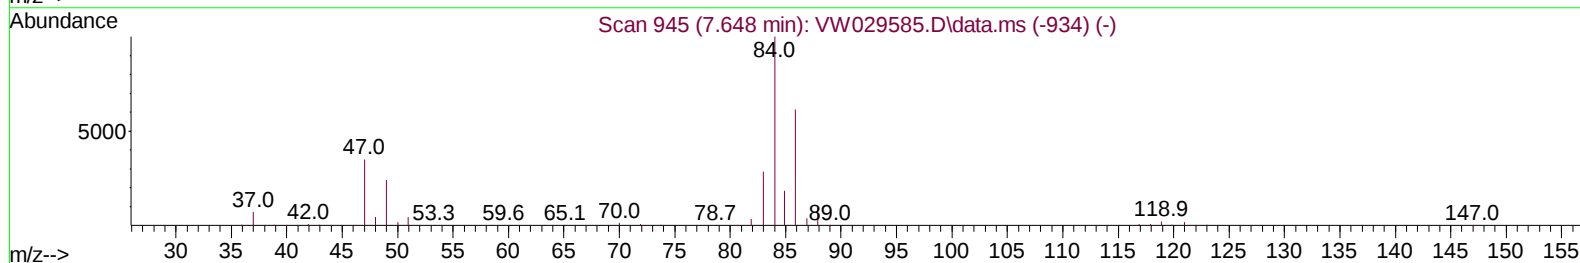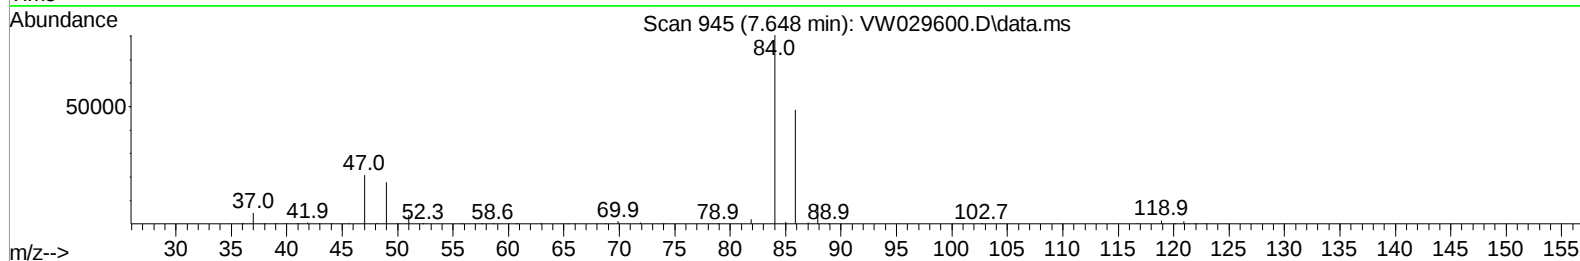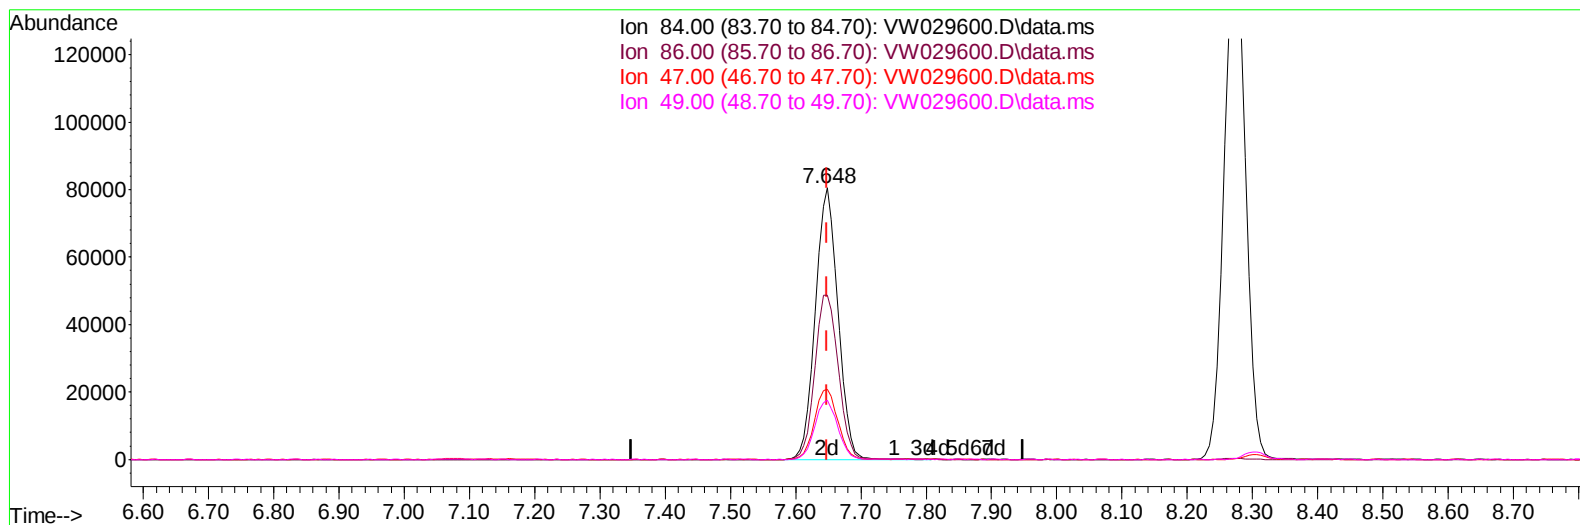

TIC: VW029600.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.000) 17.12 ug/L m

response 193321

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	0.04#
47.00	48.40	0.04#
49.00	27.80	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071624\
 Data File : VW029600.D
 Acq On : 16 Jul 2024 19:21
 Operator : SY/MD
 Sample : P3263-10
 Misc : 5.47g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4BD6

Manual IntegrationsAPPROVED

Quant Time: Jul 17 00:58:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 17 00:53:35 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/17/2024
 Supervised By :Mahesh Dadoda 07/19/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	390601	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	324885	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	114876	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	83299	13.201	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	52.800%	
7) Chloroethane-d5	2.893	69	67337	14.821	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	59.280%	
11) 1,1-Dichloroethene-d2	4.015	65	40815	14.405	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	57.600%	
21) 2-Butanone-d5	7.081	46	27963	14.763	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	29.520%	
24) Chloroform-d	7.648	84	193321m	17.120	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	68.480%	
26) 1,2-Dichloroethane-d4	8.301	65	113254	17.099	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	68.400%#	
32) Benzene-d6	8.270	84	353205	18.148	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	72.600%	
36) 1,2-Dichloropropane-d6	9.270	67	121139	19.467	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	77.880%	
41) Toluene-d8	10.319	98	284839	16.641	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	66.560%	
43) trans-1,3-Dichloroprop...	10.575	79	31295	11.876	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	47.520%	
47) 2-Hexanone-d5	10.922	63	19737	17.455	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	34.900%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	81007	16.033	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	64.120%	
66) 1,2-Dichlorobenzene-d4	13.848	152	65295	16.321	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	65.280%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071624\
Data File : VW029600.D
Acq On : 16 Jul 2024 19:21
Operator : SY/MD
Sample : P3263-10
Misc : 5.47g/10mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4BD6

Manual IntegrationsAPPROVED

Quant Time: Jul 17 00:58:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 17 00:53:35 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/17/2024
Supervised By :Mahesh Dadoda 07/19/2024

