




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071724\
Data File : VW029610.D
Acq On : 17 Jul 2024 12:44
Operator : SY/MD
Sample : P3263-12 RE
Misc : 5.30g/10mL/MSVOA_W/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CG6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:19:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 18 02:17:40 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
Supervised By :Mahesh Dadoda 07/19/2024

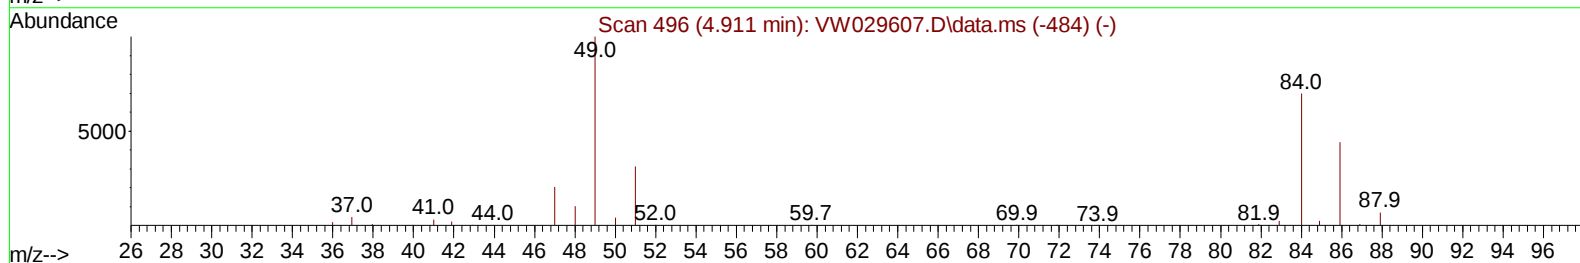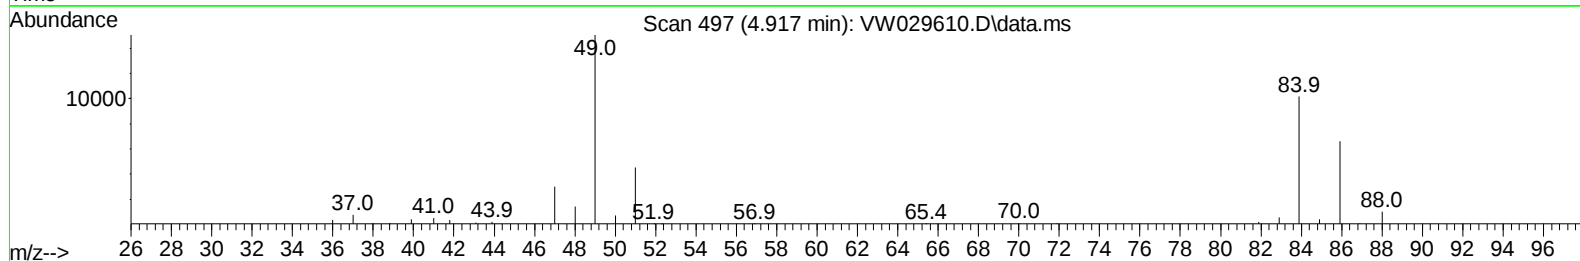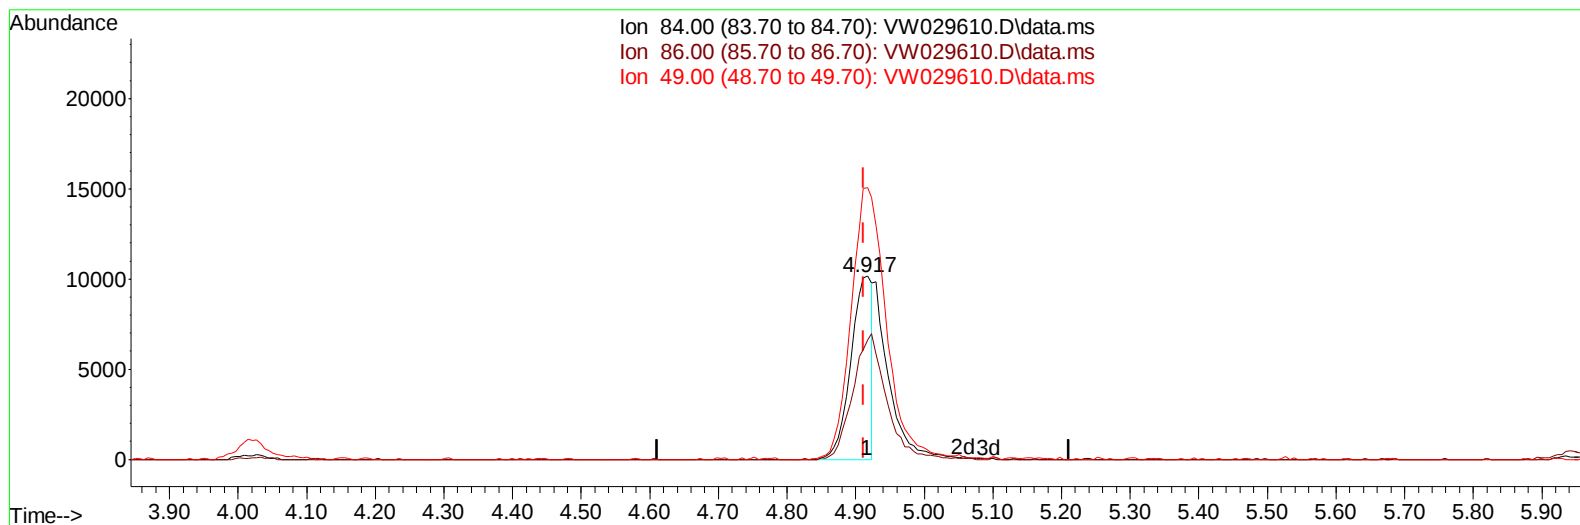

TIC: VW029610.D\data.ms

(16) Methylene chloride (T)

4.917min (+ 0.006) 4.70 ug/L

response 21957

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	66.00	65.02
49.00	138.20	148.13
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071724\
 Data File : VW029610.D
 Acq On : 17 Jul 2024 12:44
 Operator : SY/MD
 Sample : P3263-12 RE
 Misc : 5.30g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CG6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:19:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 18 02:17:40 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
 Supervised By :Mahesh Dadoda 07/19/2024

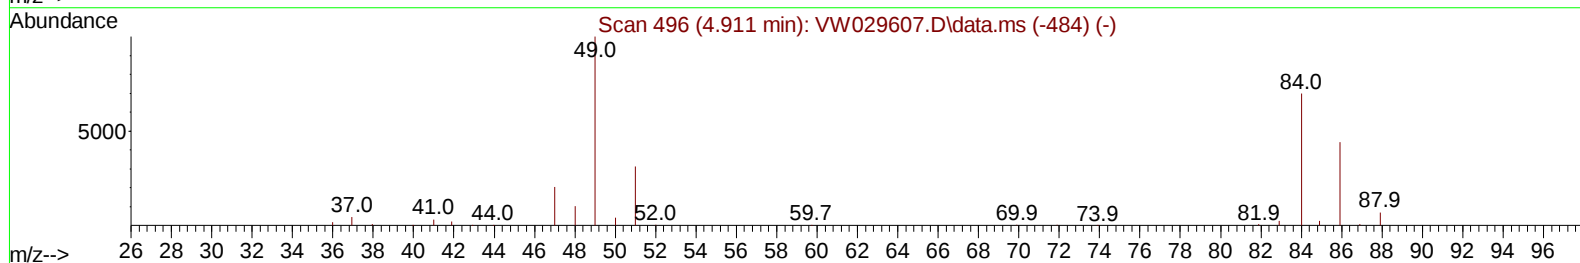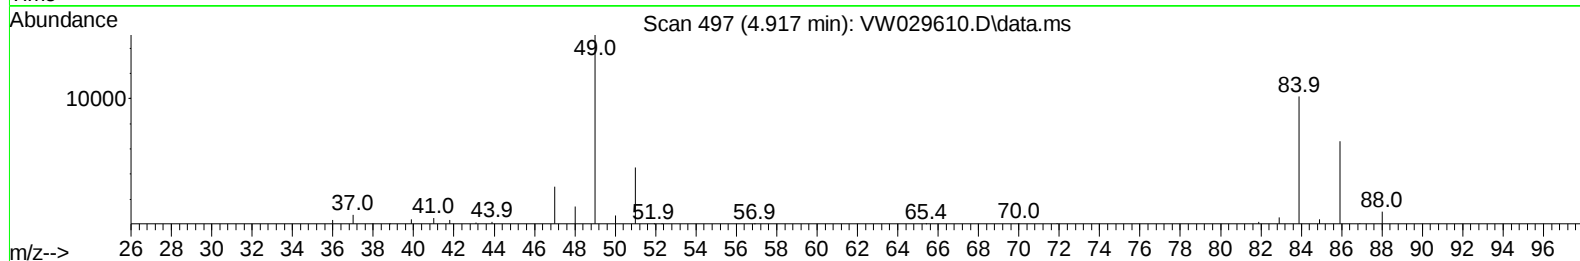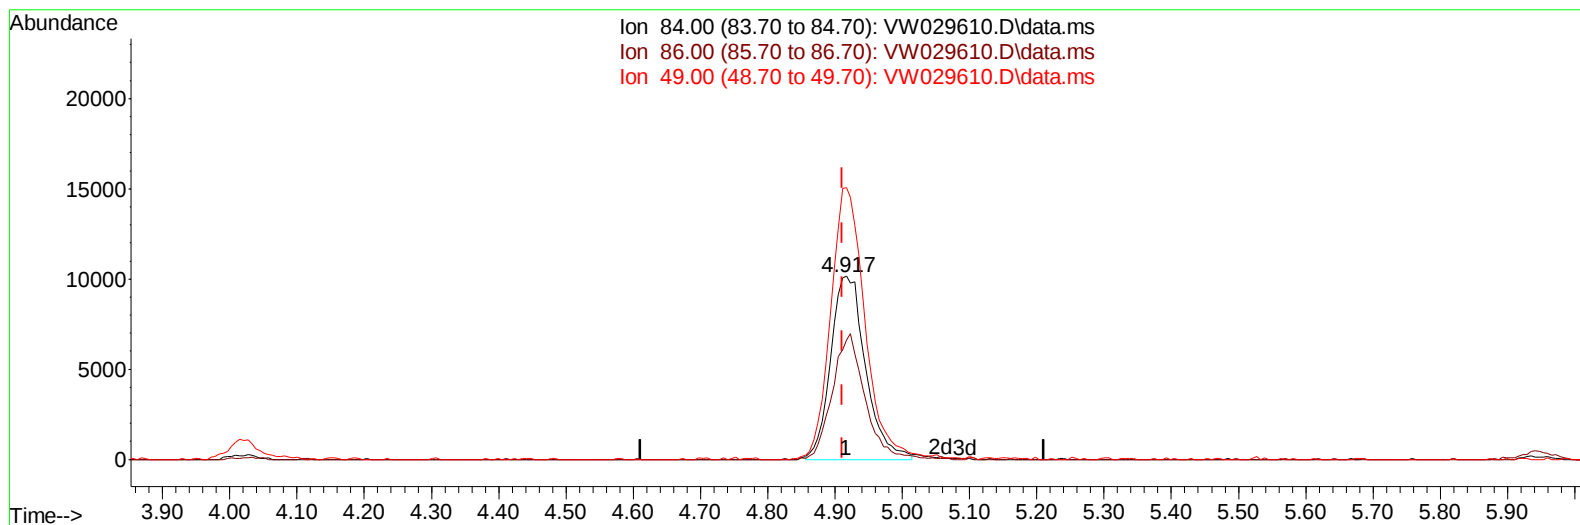

TIC: VW029610.D\data.ms

(16) Methylene chloride (T)

4.917min (+ 0.006) 7.85 ug/L m

response 36668

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	66.00	65.02
49.00	138.20	148.13
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071724\
 Data File : VW029610.D
 Acq On : 17 Jul 2024 12:44
 Operator : SY/MD
 Sample : P3263-12 RE
 Misc : 5.30g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CG6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:19:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 18 02:17:40 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
 Supervised By :Mahesh Dadoda 07/19/2024

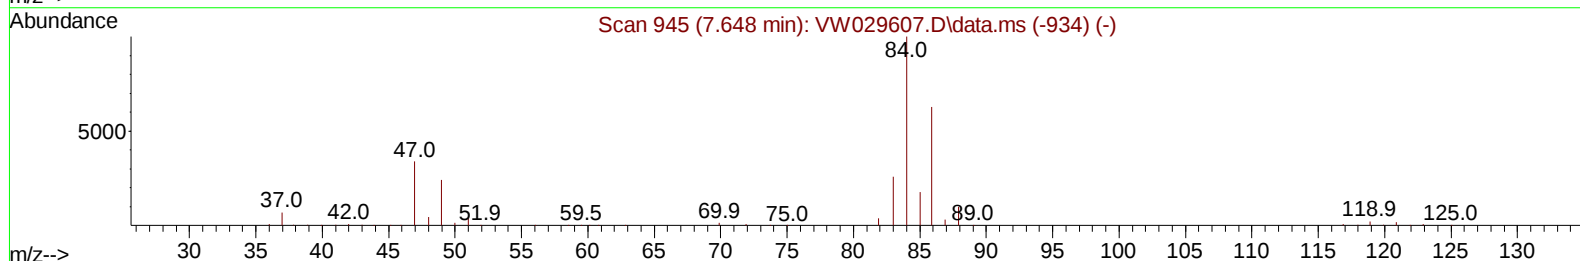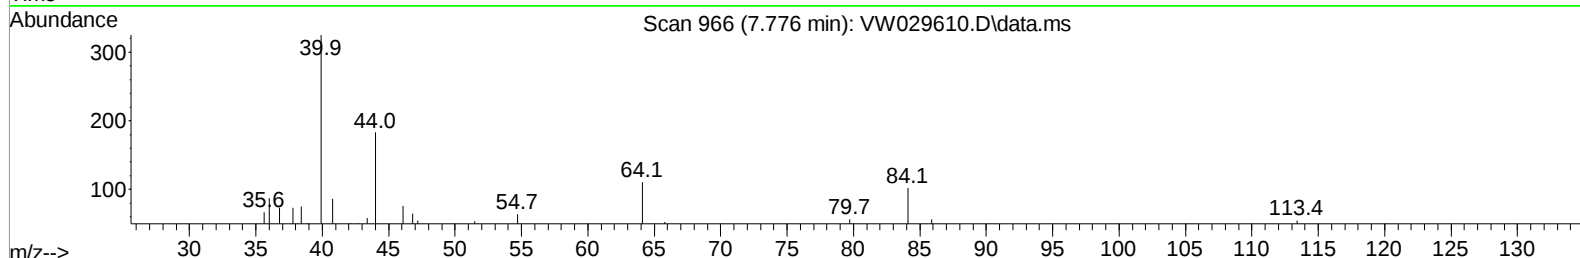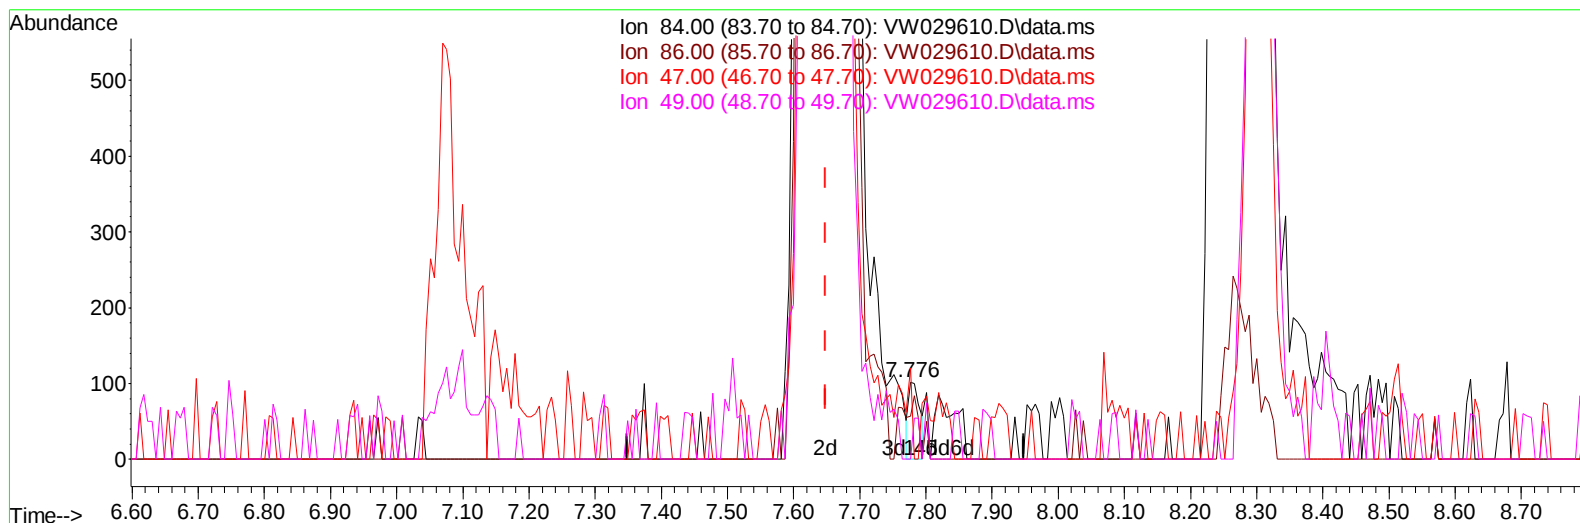

TIC: VW029610.D\data.ms

(24) Chloroform-d (S)

7.776min (+ 0.128) 0.02 ug/L

response 121

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	59.50
47.00	48.40	36.36
49.00	27.80	32.23




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071724\
Data File : VW029610.D
Acq On : 17 Jul 2024 12:44
Operator : SY/MD
Sample : P3263-12 RE
Misc : 5.30g/10mL/MSVOA_W/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CG6RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 07/18/2024
Supervised By :Mahesh Dadoda 07/19/2024

Quant Time: Jul 18 02:19:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 18 02:17:40 2024
Response via : Initial Calibration

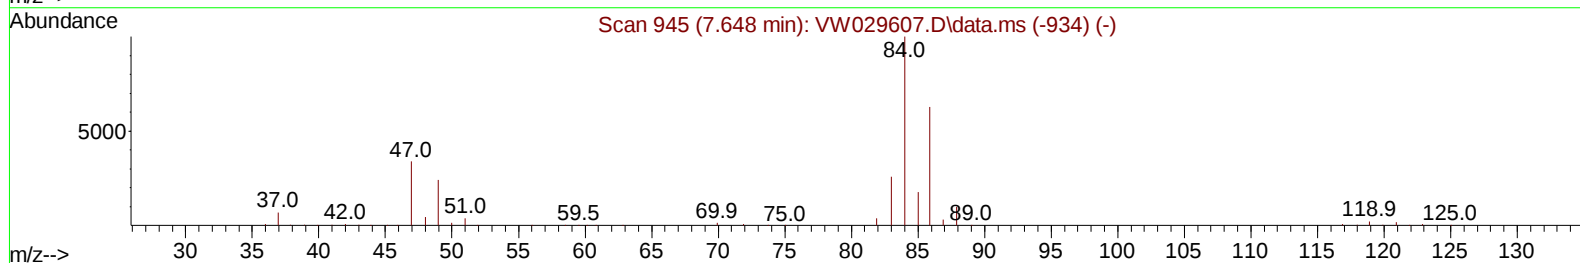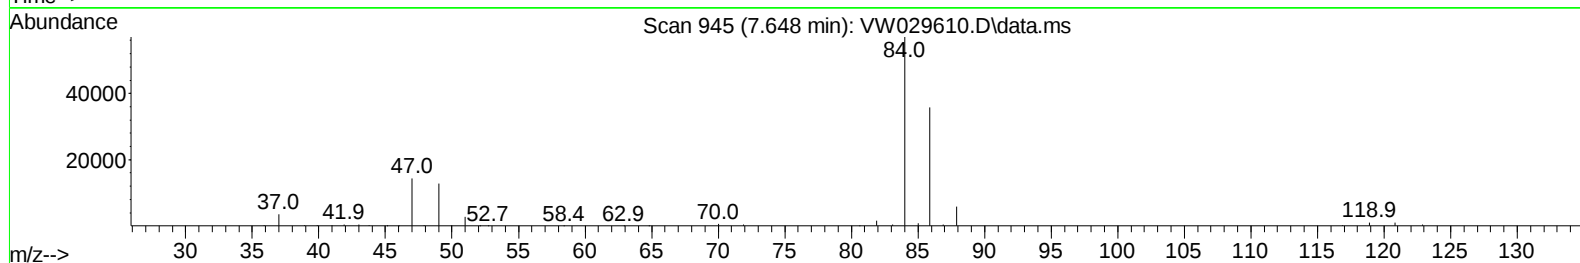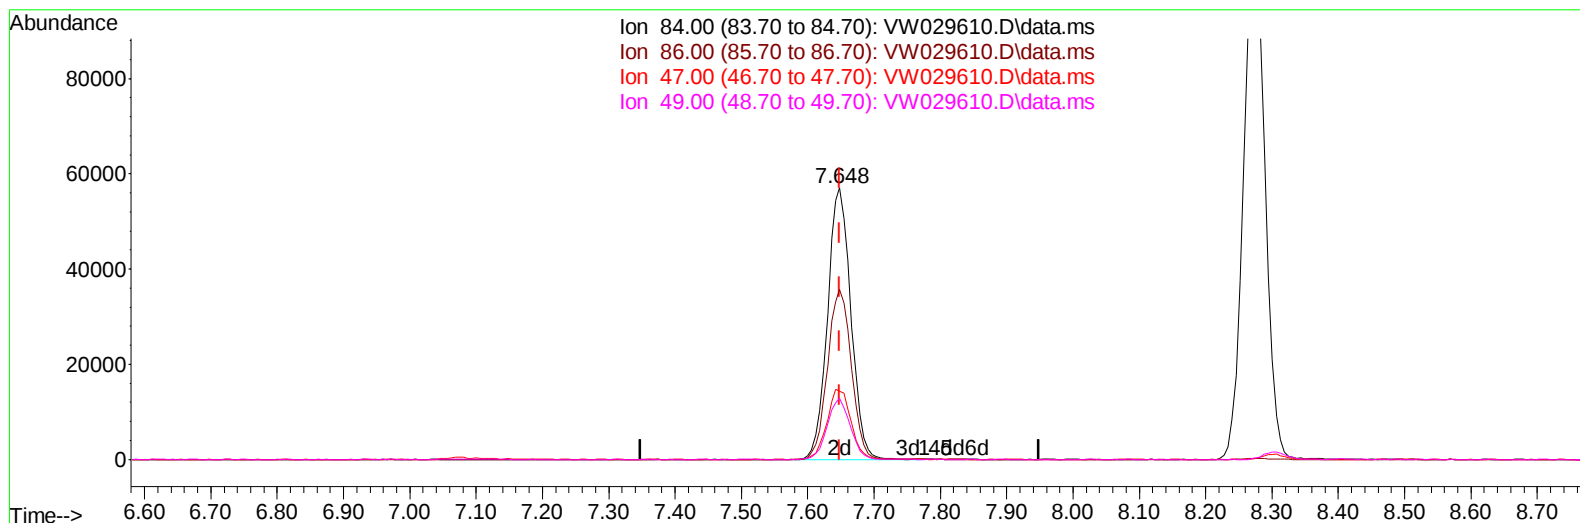

TIC: VW029610.D\data.ms

(24) Chloroform-d (S)

7.648min (-0.000) 18.57 ug/L m

response 139968

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	0.05#
47.00	48.40	0.03#
49.00	27.80	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071724\
 Data File : VW029610.D
 Acq On : 17 Jul 2024 12:44
 Operator : SY/MD
 Sample : P3263-12 RE
 Misc : 5.30g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CG6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:19:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 18 02:17:40 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
 Supervised By :Mahesh Dadoda 07/19/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		260761	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		135222	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		24703	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		81367	19.316	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	77.280%		
7) Chloroethane-d5	2.899	69		65775	21.685	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	86.760%		
11) 1,1-Dichloroethene-d2	4.021	65		33536	17.729	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	70.920%		
21) 2-Butanone-d5	7.075	46		44411	35.121	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	70.240%		
24) Chloroform-d	7.648	84		139968m	18.567	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	74.280%		
26) 1,2-Dichloroethane-d4	8.301	65		84679	19.151	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	76.600%		
32) Benzene-d6	8.270	84		246001	30.368	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	121.480%		
36) 1,2-Dichloropropane-d6	9.270	67		83008	32.049	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	128.200%#		
41) Toluene-d8	10.319	98		154854	21.737	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	86.960%		
43) trans-1,3-Dichloroprop...	10.575	79		18425	16.799	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	67.200%		
47) 2-Hexanone-d5	10.922	63		9555	20.302	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	40.600%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		33980	16.159	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	64.640%		
66) 1,2-Dichlorobenzene-d4	13.848	152		14510	16.866	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	67.480%#		
Target Compounds							
16) Methylene chloride	4.917	84		36668m	7.854	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071724\
Data File : VW029610.D
Acq On : 17 Jul 2024 12:44
Operator : SY/MD
Sample : P3263-12 RE
Misc : 5.30g/10mL/MSVOA_W/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CG6RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 07/18/2024
Supervised By :Mahesh Dadoda 07/19/2024

Quant Time: Jul 18 02:19:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 18 02:17:40 2024
Response via : Initial Calibration

