




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071724\
Data File : VW029615.D
Acq On : 17 Jul 2024 14:44
Operator : SY/MD
Sample : P3263-19
Misc : 5.42g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CK9

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:21:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 18 02:17:40 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
Supervised By :Mahesh Dadoda 07/19/2024

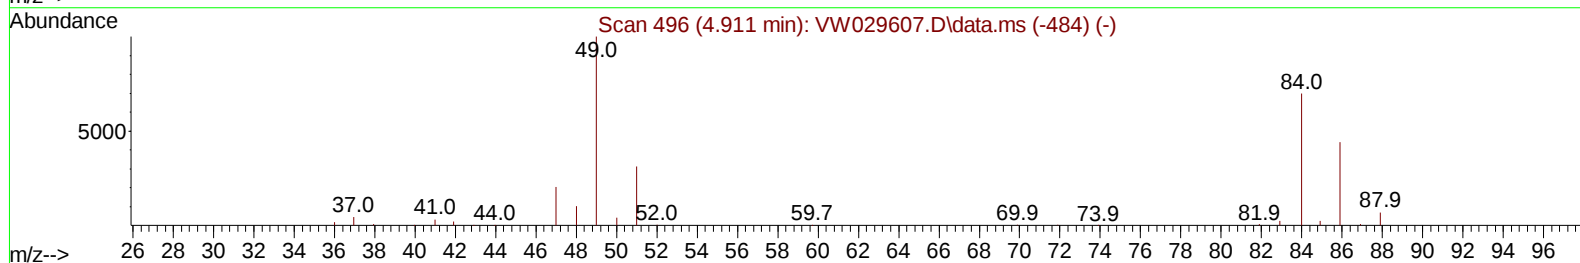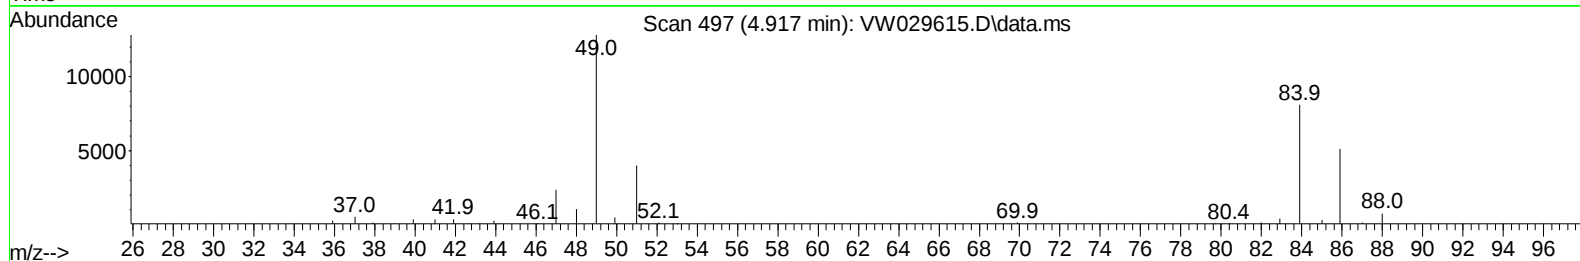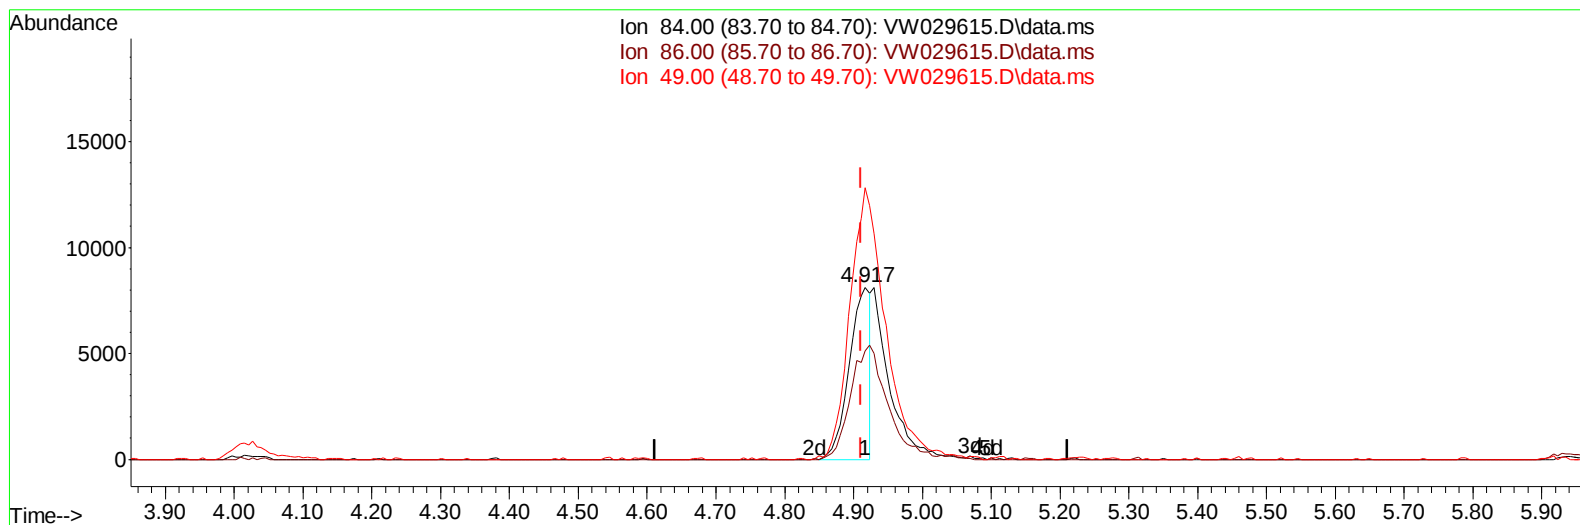

TIC: VW029615.D\data.ms

(16) Methylene chloride (T)

4.917min (+ 0.006) 4.19 ug/L

response 17231

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	66.00	63.20
49.00	138.20	157.78
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071724\
Data File : VW029615.D
Acq On : 17 Jul 2024 14:44
Operator : SY/MD
Sample : P3263-19
Misc : 5.42g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CK9

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:21:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 18 02:17:40 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
Supervised By :Mahesh Dadoda 07/19/2024

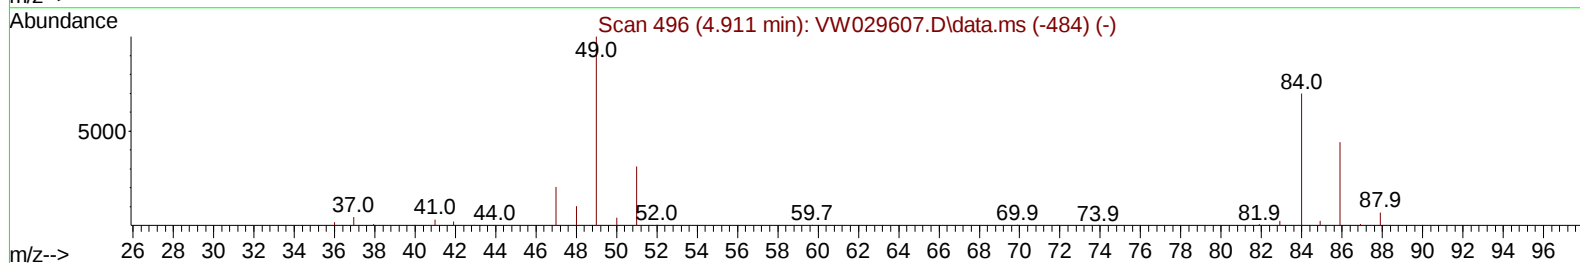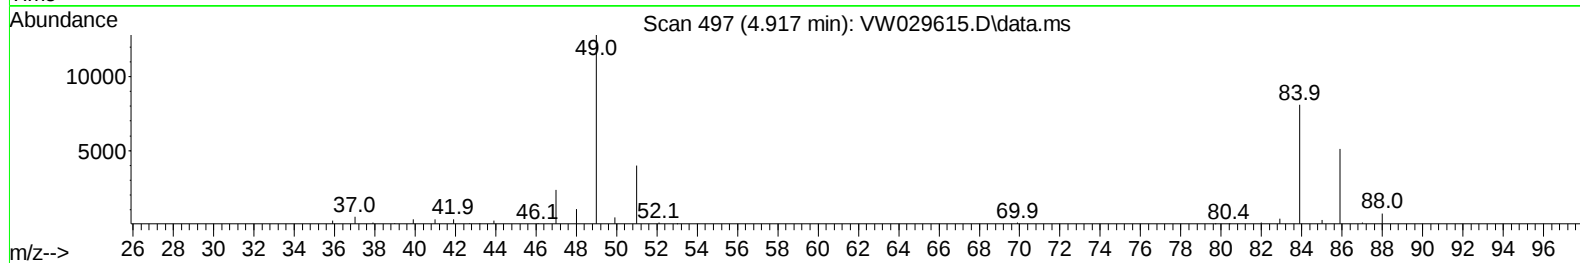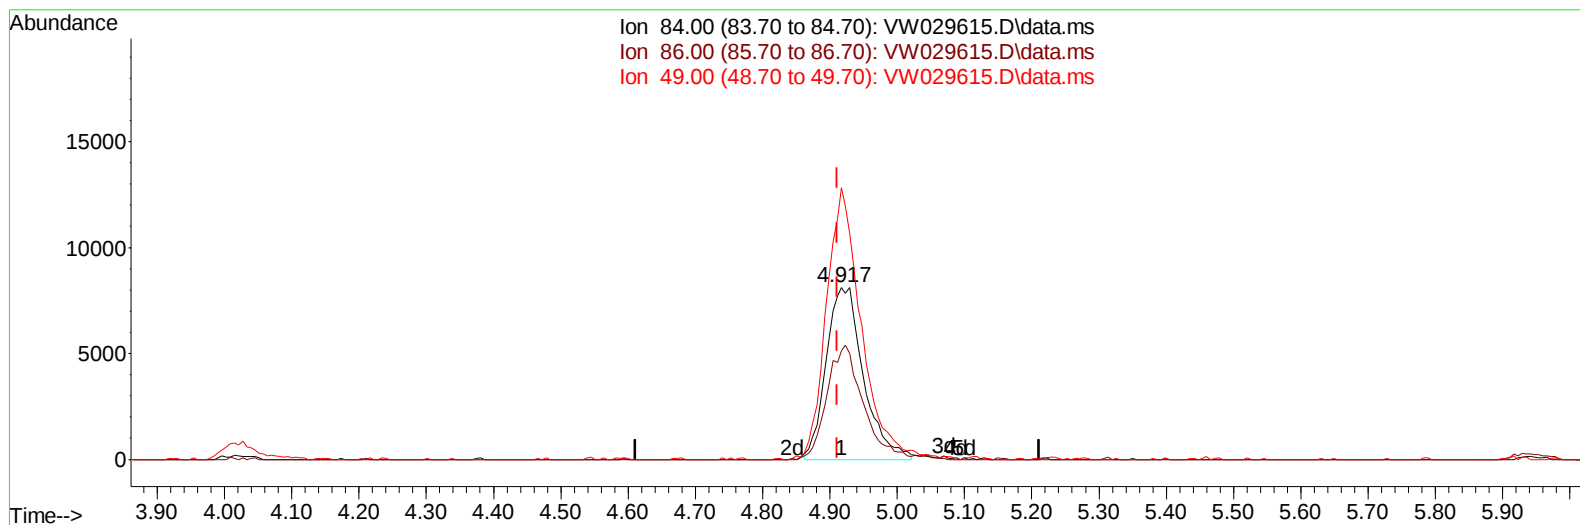

TIC: VW029615.D\data.ms

(16) Methylene chloride (T)

4.917min (+ 0.006) 7.58 ug/L m

response 31176

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	66.00	63.20
49.00	138.20	157.78
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071724\
 Data File : VW029615.D
 Acq On : 17 Jul 2024 14:44
 Operator : SY/MD
 Sample : P3263-19
 Misc : 5.42g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4CK9

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:21:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 18 02:17:40 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
 Supervised By :Mahesh Dadoda 07/19/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	229583	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	127263	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	23426	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	67656	18.242	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	72.960%	
7) Chloroethane-d5	2.893	69	54589	20.442	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	81.760%	
11) 1,1-Dichloroethene-d2	4.015	65	27327	16.408	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	65.640%	
21) 2-Butanone-d5	7.081	46	25644	23.034	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	46.060%	
24) Chloroform-d	7.648	84	118659	17.878	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	71.520%	
26) 1,2-Dichloroethane-d4	8.307	65	73476	18.874	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	75.480%	
32) Benzene-d6	8.276	84	195617	25.659	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	102.640%	
36) 1,2-Dichloropropane-d6	9.276	67	70547	28.941	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	115.760%	
41) Toluene-d8	10.325	98	123794	18.464	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	73.840%	
43) trans-1,3-Dichloroprop...	10.581	79	9870	9.562	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	38.240%	
47) 2-Hexanone-d5	10.922	63	2974	6.714	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	13.420%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	27340	13.814	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	55.240%	
66) 1,2-Dichlorobenzene-d4	13.848	152	10872	13.326	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	53.320%#	
Target Compounds						
13) Acetone	4.125	43	5219	4.645	ug/L	96
16) Methylene chloride	4.917	84	31176m	7.585	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071724\
Data File : VW029615.D
Acq On : 17 Jul 2024 14:44
Operator : SY/MD
Sample : P3263-19
Misc : 5.42g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4CK9

Manual IntegrationsAPPROVED

Quant Time: Jul 18 02:21:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 18 02:17:40 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/18/2024
Supervised By :Mahesh Dadoda 07/19/2024

