

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071725\
 Data File : VW031888.D
 Acq On : 17 Jul 2025 14:53
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Quant Time: Jul 18 02:53:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 01 03:35:17 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.965	168	196467	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.849	114	415084	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.629	117	392346	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	193116	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	184808	65.546	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	131.100%
35) Dibromofluoromethane	7.898	113	160409	59.222	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	118.440%
50) Toluene-d8	10.325	98	571272	56.675	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	113.340%
62) 4-Bromofluorobenzene	12.617	95	241851	65.200	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	130.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071725\
Data File : VW031888.D
Acq On : 17 Jul 2025 14:53
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Quant Time: Jul 18 02:53:14 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W063025S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 01 03:35:17 2025
Response via : Initial Calibration




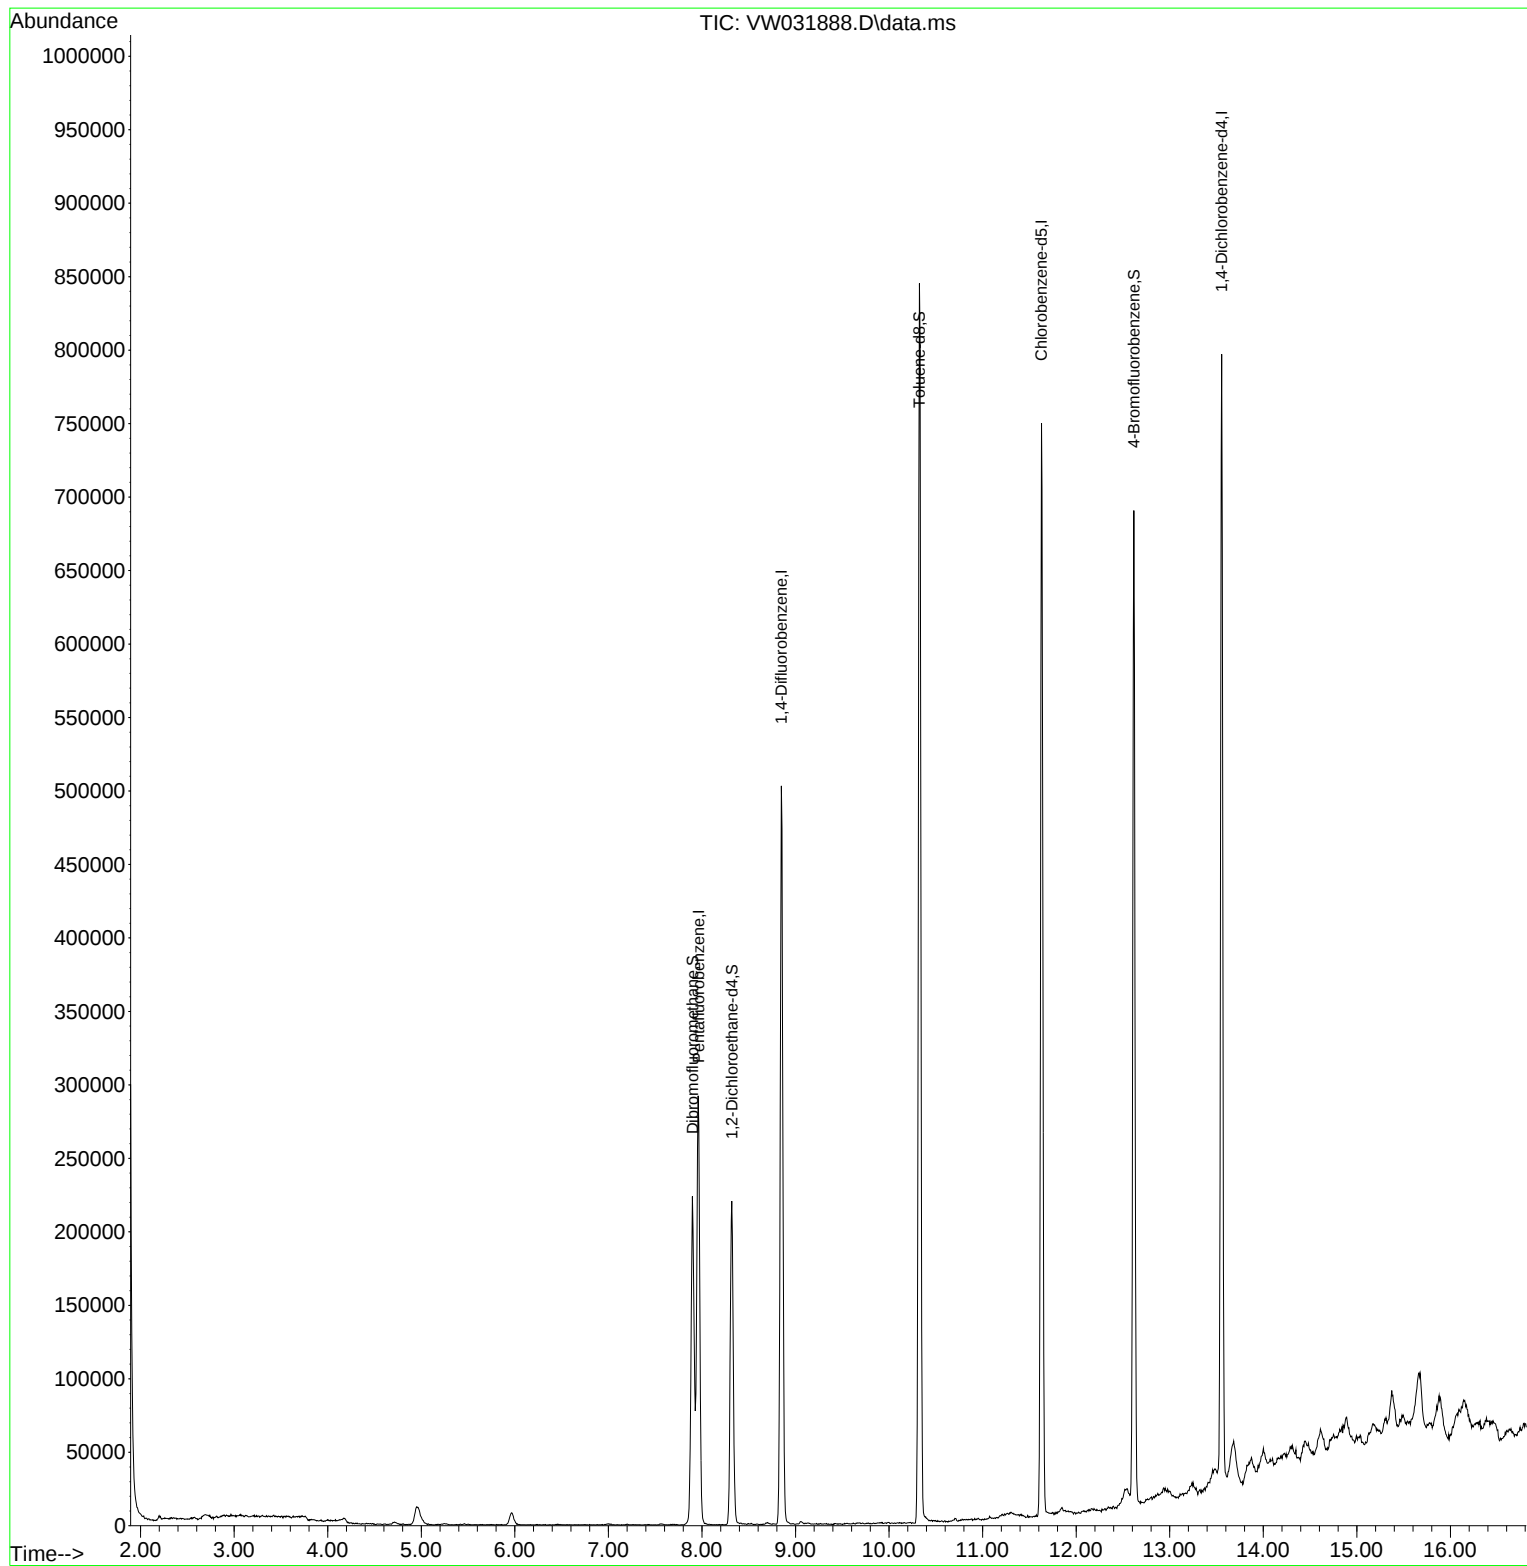




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.965 min Scan# 997
Delta R.T. 0.000 min
Lab File: VW031888.D
Acq: 17 Jul 2025 14:53




Instrument :
MSVOA_W
ClientSampleId :
VIBLK


Tgt Ion:168 Resp: 196467
Ion Ratio Lower Upper
168 100
99 63.3 49.4 74.2

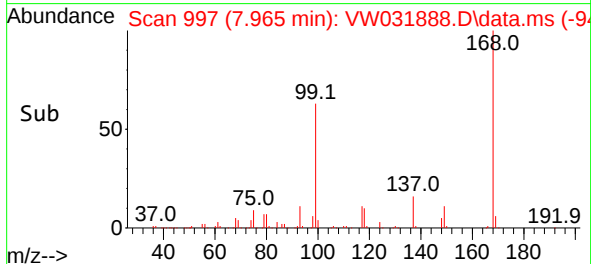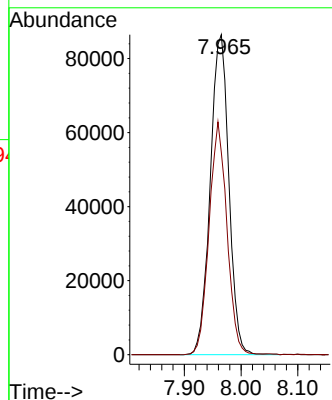

#33
1,2-Dichloroethane-d4
Concen: 65.546 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. 0.000 min
Lab File: VW031888.D
Acq: 17 Jul 2025 14:53

Tgt Ion: 65 Resp: 184808
Ion Ratio Lower Upper
65 100
67 51.5 0.0 99.4

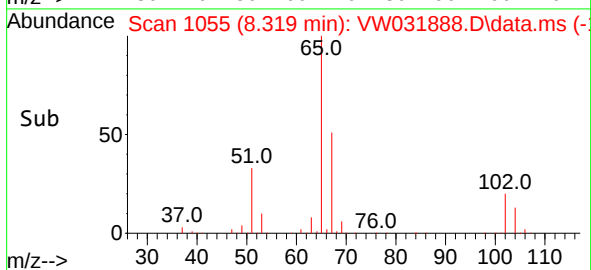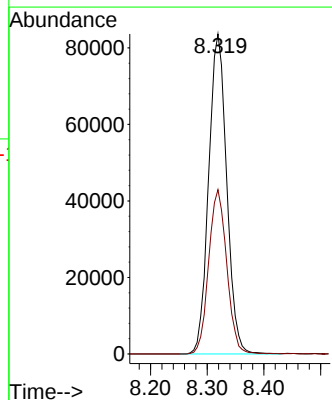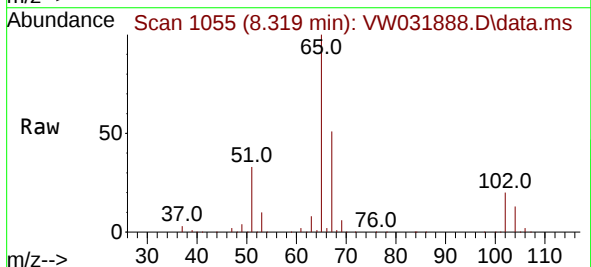

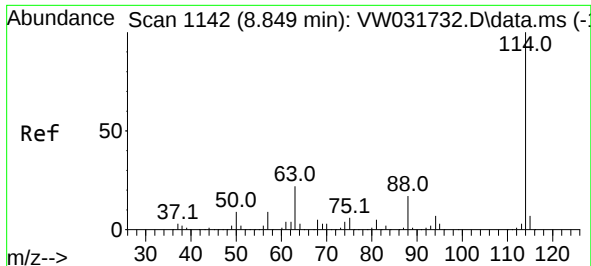

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.849 min Scan# 1142

Delta R.T. 0.000 min

Lab File: VW031888.D

Acq: 17 Jul 2025 14:53

Instrument :

MSVOA_W

ClientSampleId :

VIBLK





Tgt Ion:114 Resp: 415084

Ion Ratio Lower Upper

114 100

63 20.9 0.0 43.6

88 16.1 0.0 34.2

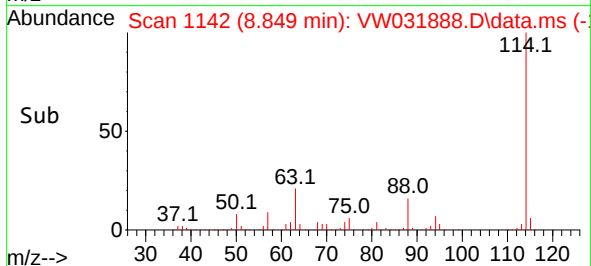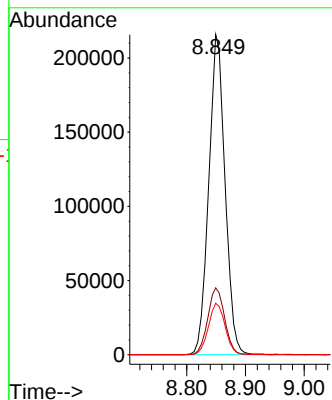

#35

Dibromofluoromethane

Concen: 59.222 ug/l

RT: 7.898 min Scan# 986

Delta R.T. -0.006 min

Lab File: VW031888.D

Acq: 17 Jul 2025 14:53




Tgt Ion:113 Resp: 160409


Ion Ratio Lower Upper

113 100

111 101.7 82.1 123.1

192 15.5 13.8 20.6


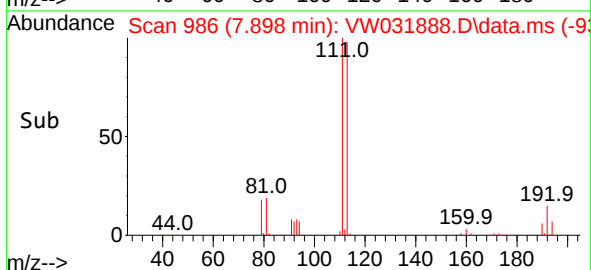
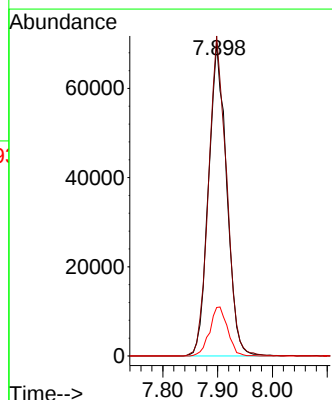
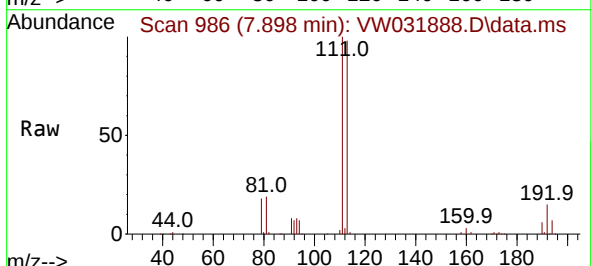


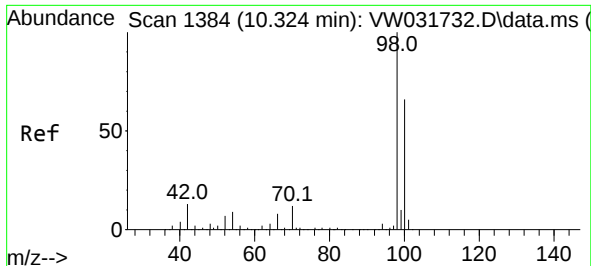

#50
Toluene-d8
Concen: 56.675 ug/l
RT: 10.325 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW031888.D
Acq: 17 Jul 2025 14:53




Instrument :
MSVOA_W
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 571272
Ion Ratio Lower Upper
98 100
100 64.9 53.0 79.4

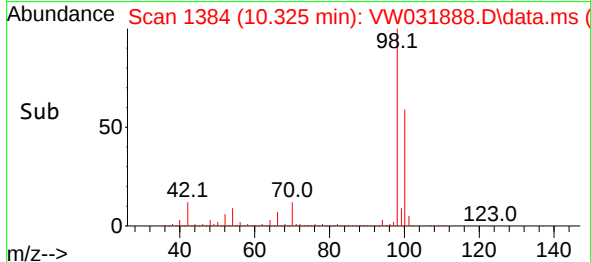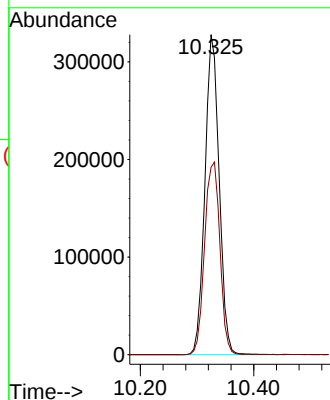

#62
4-Bromofluorobenzene
Concen: 65.200 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. 0.000 min
Lab File: VW031888.D
Acq: 17 Jul 2025 14:53

Tgt Ion: 95 Resp: 241851
Ion Ratio Lower Upper
95 100
174 67.7 0.0 133.8
176 61.8 0.0 126.0

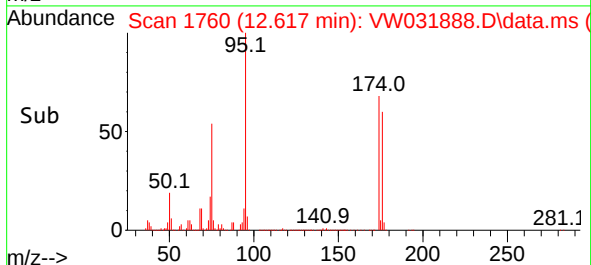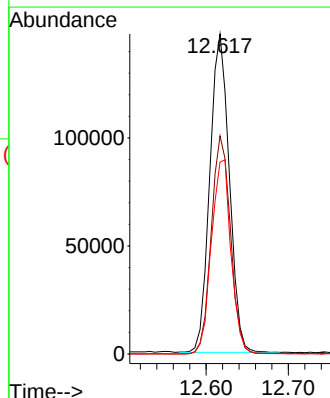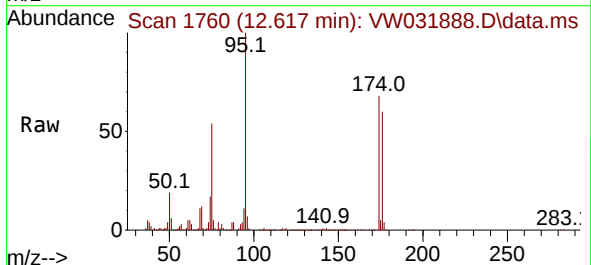



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.629 min Scan# 11

Delta R.T. 0.000 min

Lab File: VW031888.D

Acq: 17 Jul 2025 14:53

Instrument :

MSVOA_W

ClientSampleId :

VIBLK





Tgt Ion:117 Resp: 392346

Ion Ratio Lower Upper

117 100

82 60.0 48.6 72.8

119 30.5 23.9 35.9

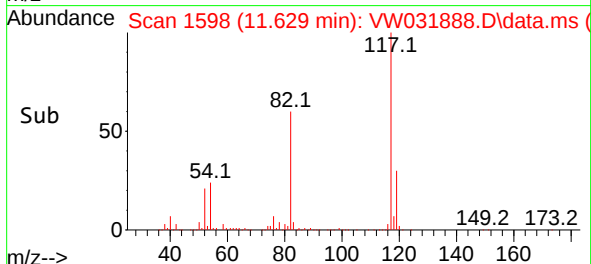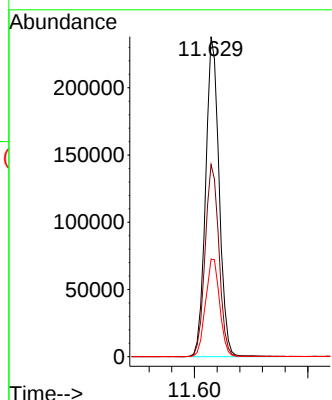

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.556 min Scan# 1914

Delta R.T. 0.000 min

Lab File: VW031888.D

Acq: 17 Jul 2025 14:53

Tgt Ion:152 Resp: 193116

Ion Ratio Lower Upper

152 100

115 67.8 31.9 95.7

150 152.8 0.0 356.4

