

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW071919\
 Data File : VW011377.D
 Acq On : 19 Jul 2019 14:55
 Operator : SY/VA
 Sample : K3863-24
 Misc : 0.12G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A52W5

Quant Time: Jul 20 01:35:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 20 00:46:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	339836	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	308565	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	139765	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	125722	24.23	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.92%
7) Chloroethane-d5	2.89	69	86500	23.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.04%
10) 1,1-Dichloroethene-d2	4.01	63	200860	18.28	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.12%
20) 2-Butanone-d5	7.07	46	123485	60.41	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.82%
24) Chloroform-d	7.65	84	223520	24.00	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	8.31	65	150610	26.26	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.04%
29) Benzene-d6	8.27	84	476883	25.09	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.36%
33) 1,2-Dichloropropane-d6	9.27	67	158701	25.64	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.56%
37) Toluene-d8	10.32	98	414839	24.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.96%
38) trans-1,3-Dichloropropene-	10.58	79	65808	25.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.00%
39) 2-Hexanone-d5	10.92	63	89539	63.08	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.16%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	146842	28.68	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.72%
61) 1,2-Dichlorobenzene-d4	13.85	152	139440	25.99	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.96%


Target Compounds					Ovalue
13) Acetone	4.12	43	6598	3.305 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW071919\
Data File : VW011377.D
Acq On : 19 Jul 2019 14:55
Operator : SY/VA
Sample : K3863-24
Misc : 0.12G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A52W5

Quant Time: Jul 20 01:35:26 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070219S.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 20 00:46:56 2019
Response via : Initial Calibration

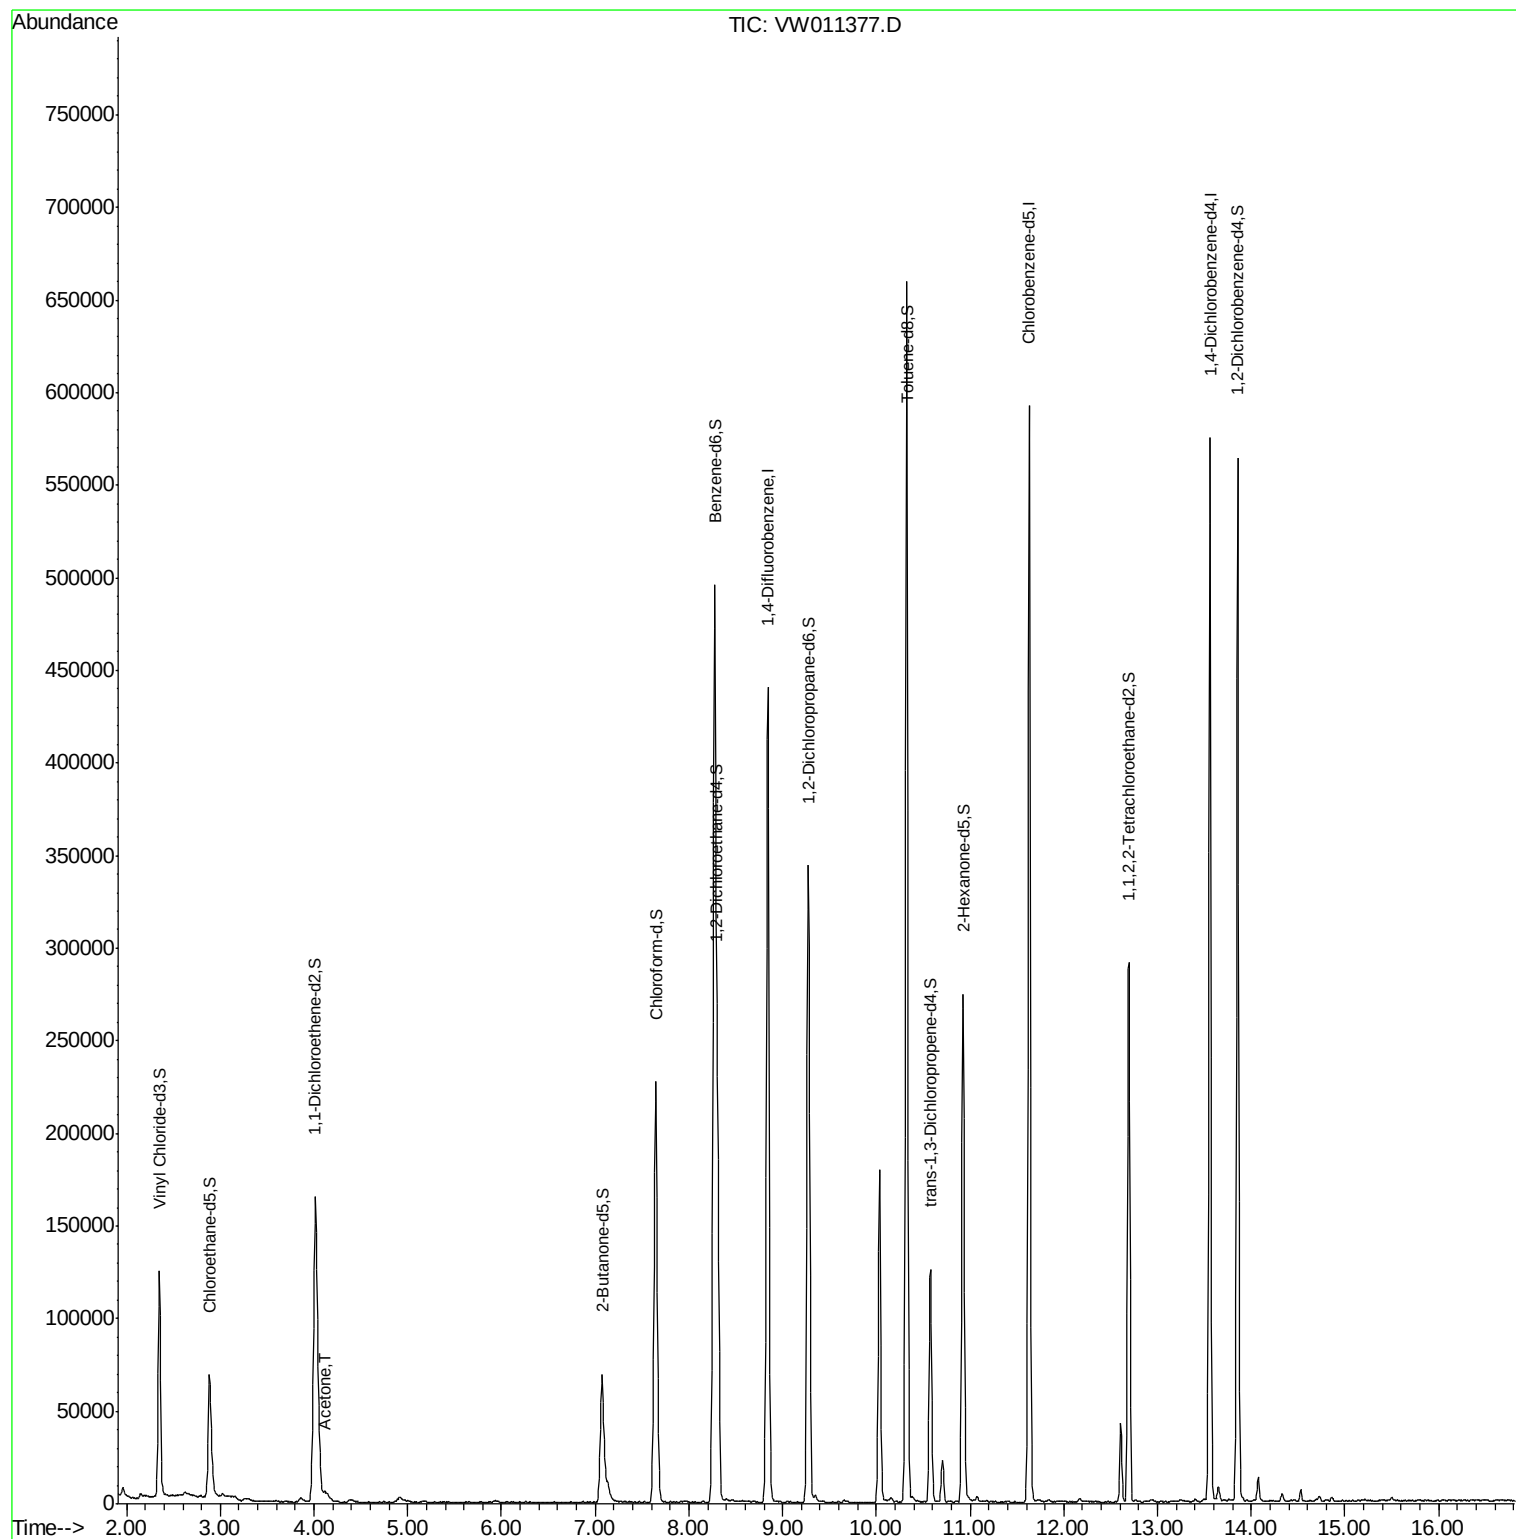

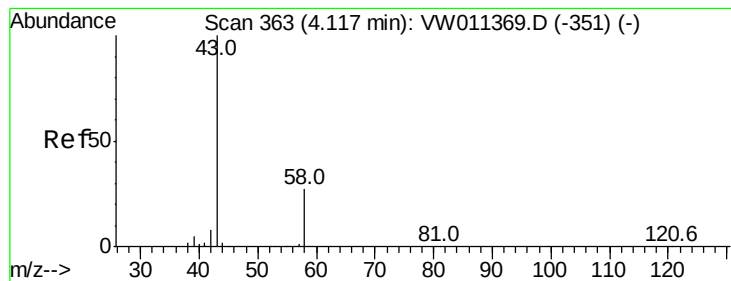

#13
 Acetone
 Concen: 3.305 ug/L
 RT: 4.12 min Scan# 363
 Delta R.T. 0.00 min
 Lab File: VW011377.D
 Acq: 19 Jul 2019 14:55

Instrument :
 MSVOA_W
 ClientSampleId :
 A52W5

Tot Ion: 43 Resp: 6598
 Ion Ratio Lower Upper
 43 100
 58 24.6 0.0 55.0

