

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
 Data File : VW023921.D
 Acq On : 20 Jul 2022 08:31
 Operator : SY/VA
 Sample : N3745-05
 Misc : 5.95g/10mL/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5D18

Quant Time: Jul 20 09:11:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 20 06:30:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.836	114	396145	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	376519	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	170944	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	157370	15.554	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.200%
7) Chloroethane-d5	2.879	69	105637	15.650	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.600%
11) 1,1-Dichloroethene-d2	4.007	63	135420	16.437	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.760%
21) 2-Butanone-d5	7.074	46	66045	42.083	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.160%
24) Chloroform-d	7.647	84	255085	22.117	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.480%
26) 1,2-Dichloroethane-d4	8.299	65	142392	20.186	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.760%
32) Benzene-d6	8.269	84	475676	24.303	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.200%
36) 1,2-Dichloropropane-d6	9.275	67	144637	24.533	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.120%
41) Toluene-d8	10.323	98	439590	22.142	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.560%
43) trans-1,3-Dichloroprop...	10.579	79	56360	20.394	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.560%
47) 2-Hexanone-d5	10.921	63	54532	43.987	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.980%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	133009	20.415	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.640%
66) 1,2-Dichlorobenzene-d4	13.853	152	145154	23.787	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.160%
Target Compounds					Qvalue	
13) Acetone	4.123	43	15995	14.415	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
Data File : VW023921.D
Acq On : 20 Jul 2022 08:31
Operator : SY/VA
Sample : N3745-05
Misc : 5.95g/10mL/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5D18

Quant Time: Jul 20 09:11:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 20 06:30:31 2022
Response via : Initial Calibration

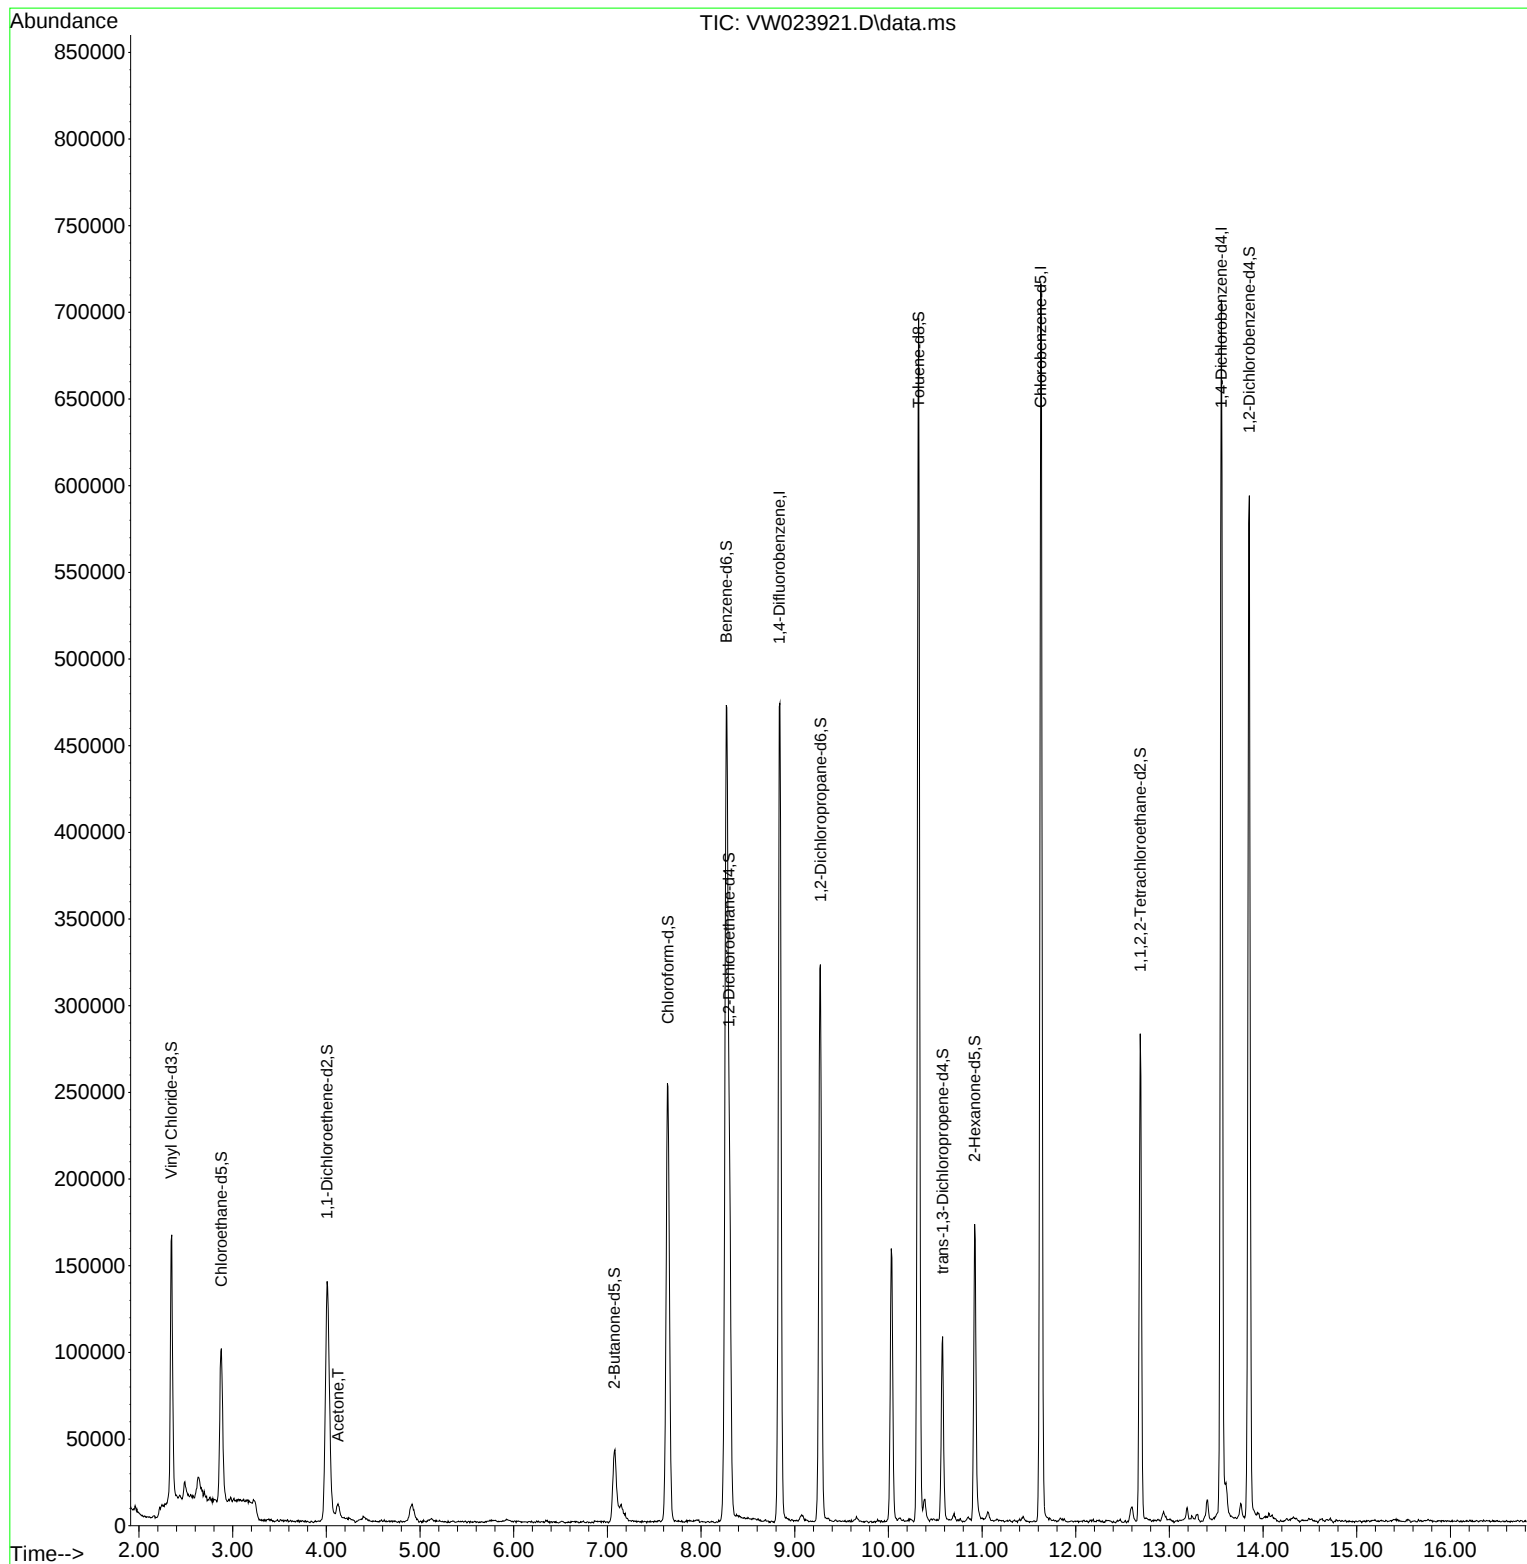

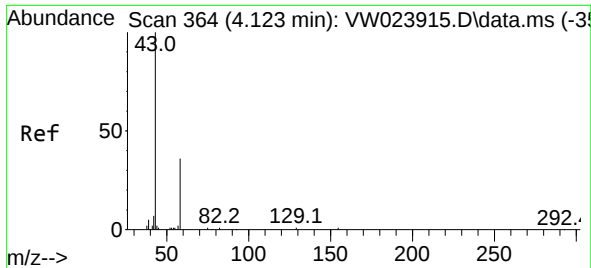

#13
 Acetone
 Concen: 14.415 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW023921.D
 Acq: 20 Jul 2022 08:31

Instrument :
 MSVOA_W
 ClientSampleId :
 F5D18

Tgt Ion: 43 Resp: 15995
 Ion Ratio Lower Upper
 43 100
 58 28.4 0.0 64.2

