




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
 Data File : VW023880.D
 Acq On : 19 Jul 2022 13:28
 Operator : SY/VA
 Sample : N3709-09
 Misc : 6.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B25

Manual IntegrationsAPPROVED

Quant Time: Jul 20 01:19:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 20 01:17:09 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/21/2022
 Supervised By :Mahesh Dadoda 07/21/2022

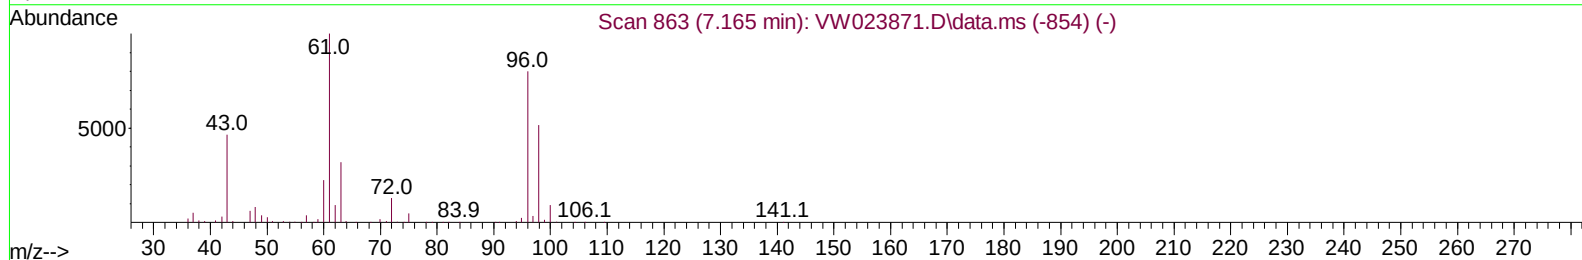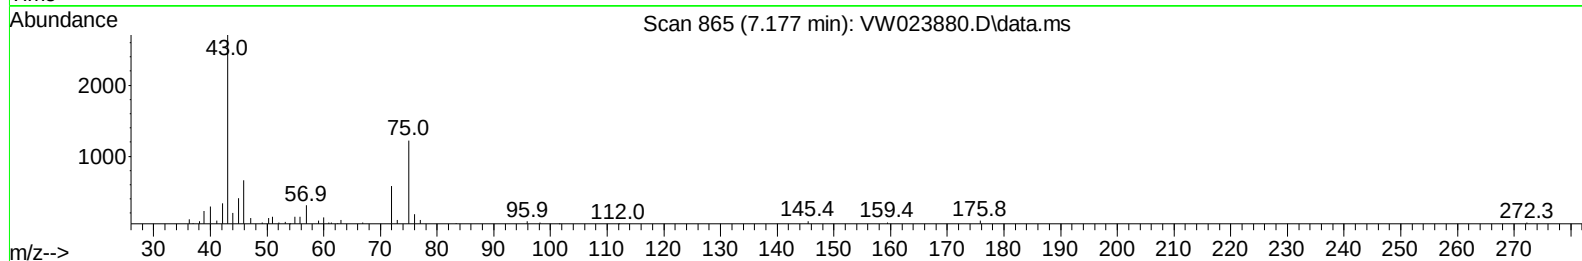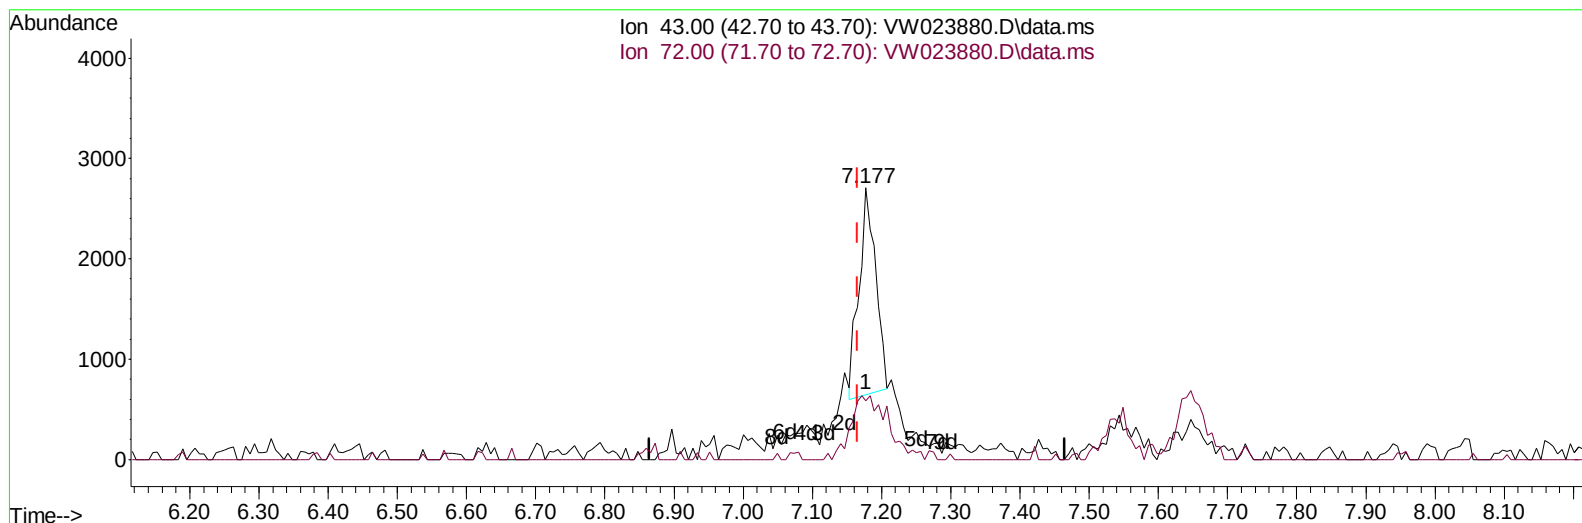

TIC: VW023880.D\data.ms

(22) 2-Butanone (T)

7.177min (+ 0.012) 1.94 ug/L

response 3471

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.40	20.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
 Data File : VW023880.D
 Acq On : 19 Jul 2022 13:28
 Operator : SY/VA
 Sample : N3709-09
 Misc : 6.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B25

Manual IntegrationsAPPROVED

Quant Time: Jul 20 01:19:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 20 01:17:09 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/21/2022
 Supervised By :Mahesh Dadoda 07/21/2022

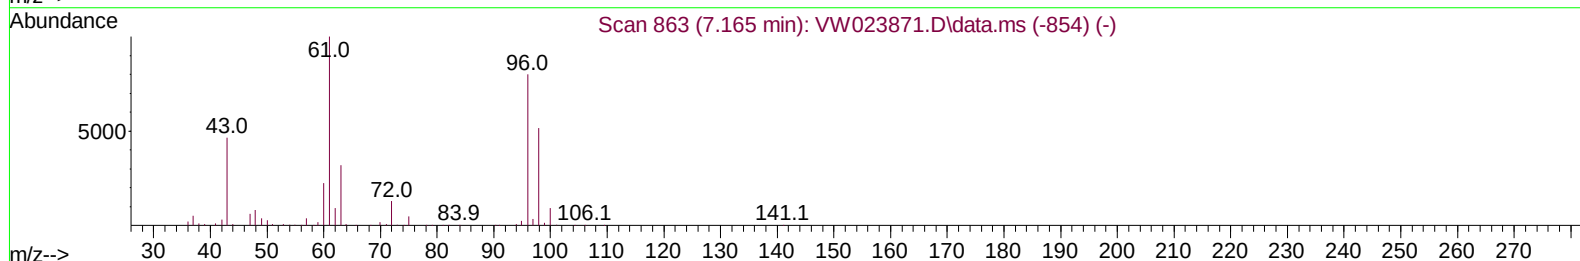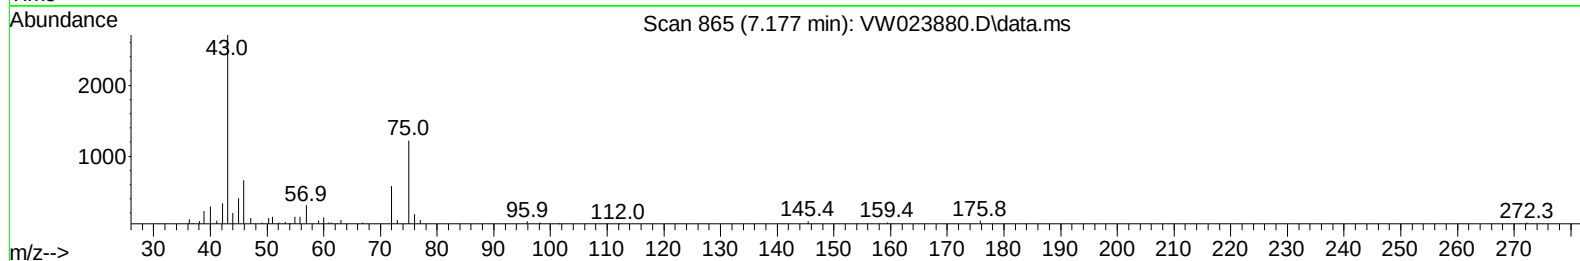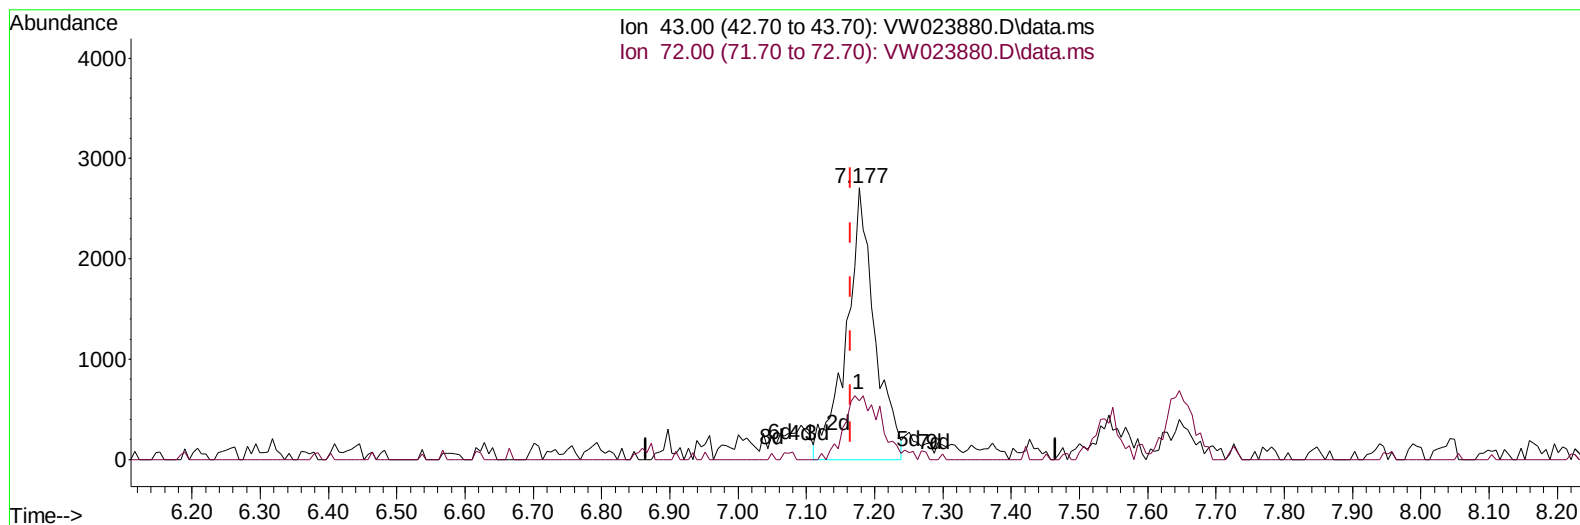

TIC: VW023880.D\data.ms

(22) 2-Butanone (T)

7.177min (+ 0.012) 4.36 ug/L m

response 7815

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.40	9.20#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
 Data File : VW023880.D
 Acq On : 19 Jul 2022 13:28
 Operator : SY/VA
 Sample : N3709-09
 Misc : 6.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B25

Manual IntegrationsAPPROVED

Quant Time: Jul 20 01:19:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 20 01:17:09 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/21/2022
 Supervised By :Mahesh Dadoda 07/21/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	389272	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	357267	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	161232	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	95934	9.649	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	38.600%	
7) Chloroethane-d5	2.879	69	78120	11.778	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	47.120%	
11) 1,1-Dichloroethene-d2	4.007	63	97892	12.091	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	48.360%	
21) 2-Butanone-d5	7.080	46	83883	54.393	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.780%	
24) Chloroform-d	7.647	84	234004	20.647	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.600%	
26) 1,2-Dichloroethane-d4	8.305	65	131175	18.924	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	75.680%	
32) Benzene-d6	8.275	84	394117	21.221	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	84.880%	
36) 1,2-Dichloropropane-d6	9.274	67	134593	24.059	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	96.240%	
41) Toluene-d8	10.323	98	353928	18.788	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	75.160%	
43) trans-1,3-Dichloroprop...	10.579	79	49991	19.064	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	76.240%	
47) 2-Hexanone-d5	10.927	63	67112	57.051	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	114.100%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	143299	23.179	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	92.720%	
66) 1,2-Dichlorobenzene-d4	13.853	152	138613	24.083	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	96.320%	
Target Compounds						
						Qvalue
13) Acetone	4.123	43	22677	20.798	ug/L	69
14) Carbon disulfide	4.385	76	12164	1.002	ug/L	96
22) 2-Butanone	7.177	43	7815m	4.361	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
Data File : VW023880.D
Acq On : 19 Jul 2022 13:28
Operator : SY/VA
Sample : N3709-09
Misc : 6.92g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
H0B25

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/21/2022
Supervised By :Mahesh Dadoda 07/21/2022

Quant Time: Jul 20 01:19:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 20 01:17:09 2022
Response via : Initial Calibration

