




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
 Data File : VW023952.D
 Acq On : 20 Jul 2022 21:50
 Operator : SY/VA
 Sample : N3741-08
 Misc : 5.67g/10mL/MSVOA_W/SOIL
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B33

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/21/2022
 Supervised By :Mahesh Dadoda 07/21/2022

Quant Time: Jul 21 00:27:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 21 00:18:55 2022
 Response via : Initial Calibration

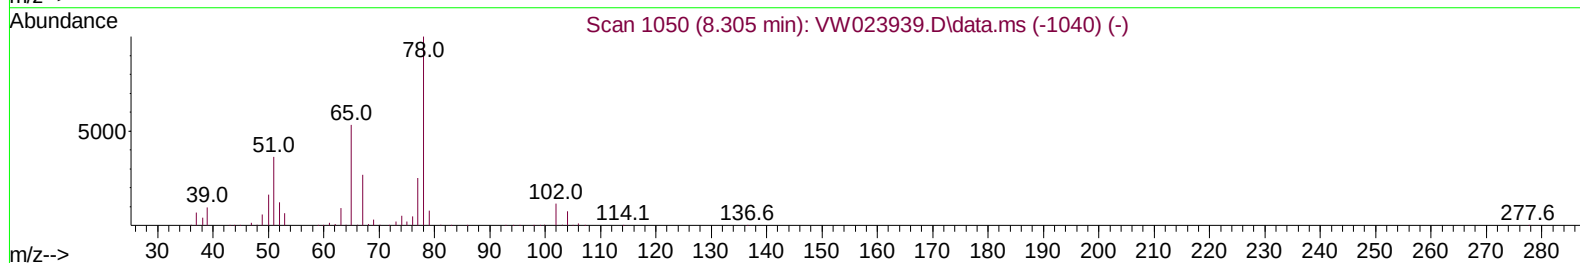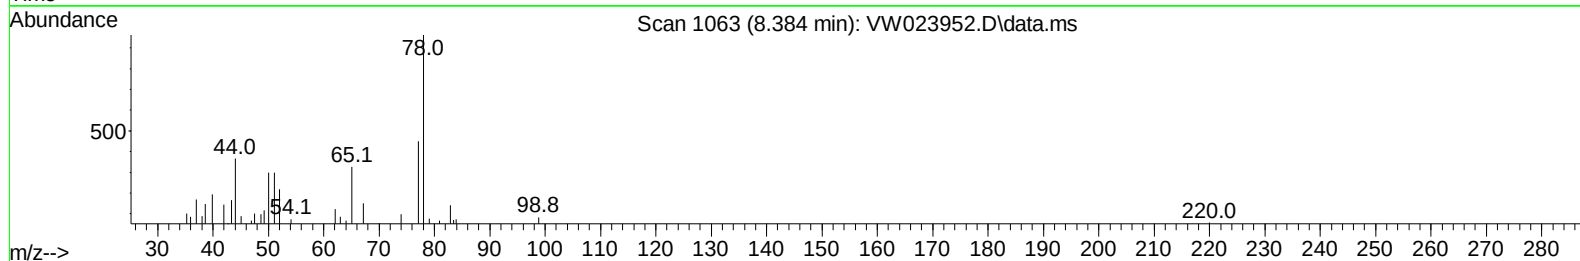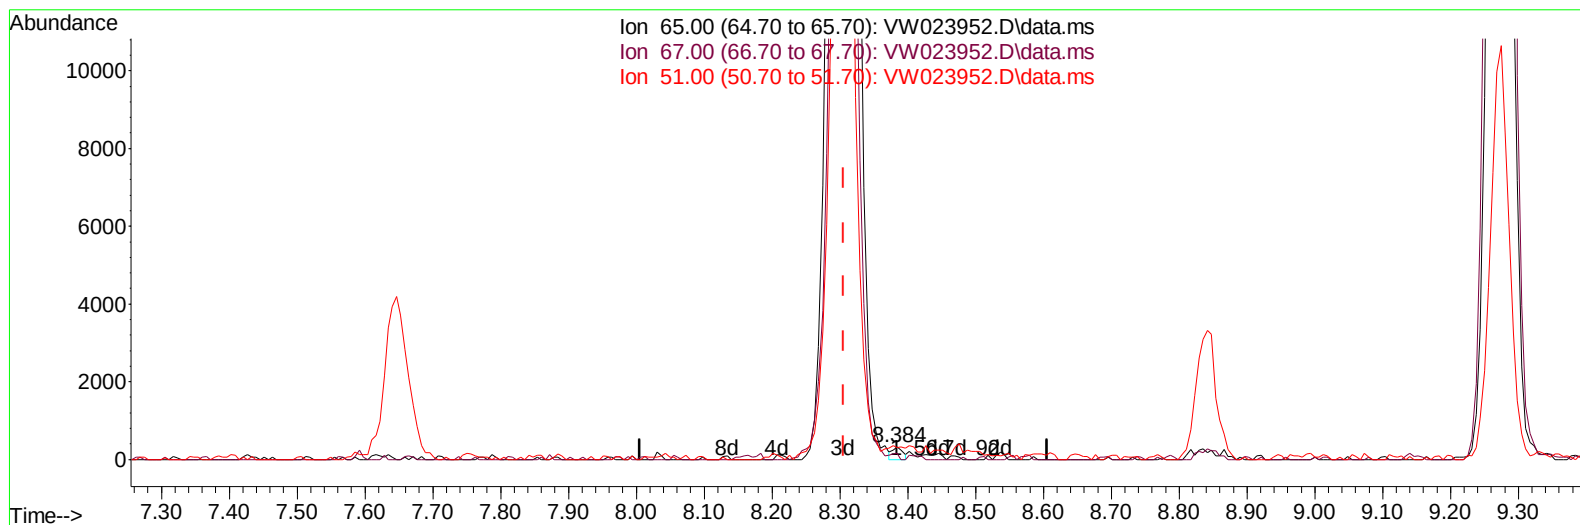

TIC: VW023952.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.384min (+ 0.079) 0.06 ug/L

response 340

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	44.41
51.00	92.20	112.65
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
 Data File : VW023952.D
 Acq On : 20 Jul 2022 21:50
 Operator : SY/VA
 Sample : N3741-08
 Misc : 5.67g/10mL/MSVOA_W/SOIL
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B33

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/21/2022
 Supervised By :Mahesh Dadoda 07/21/2022

Quant Time: Jul 21 00:27:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 21 00:18:55 2022
 Response via : Initial Calibration

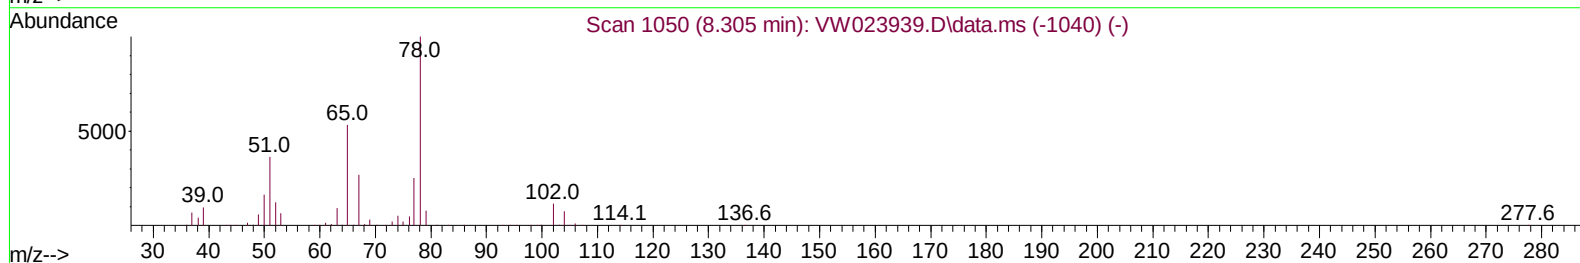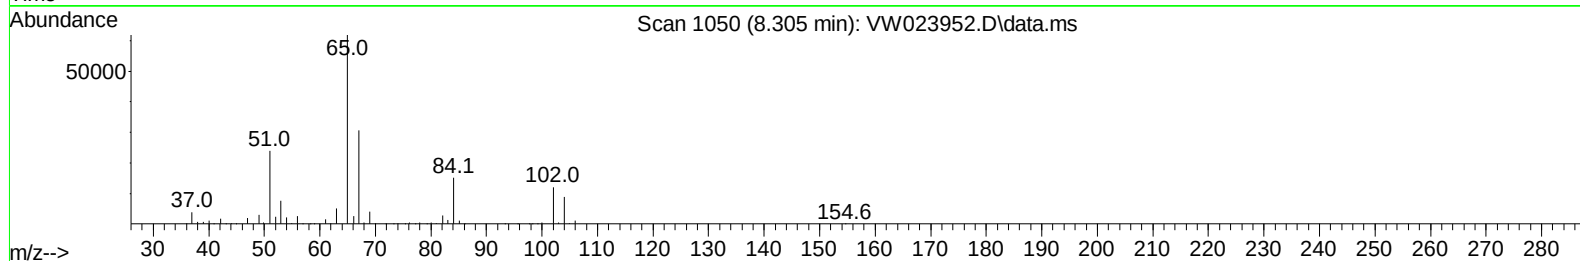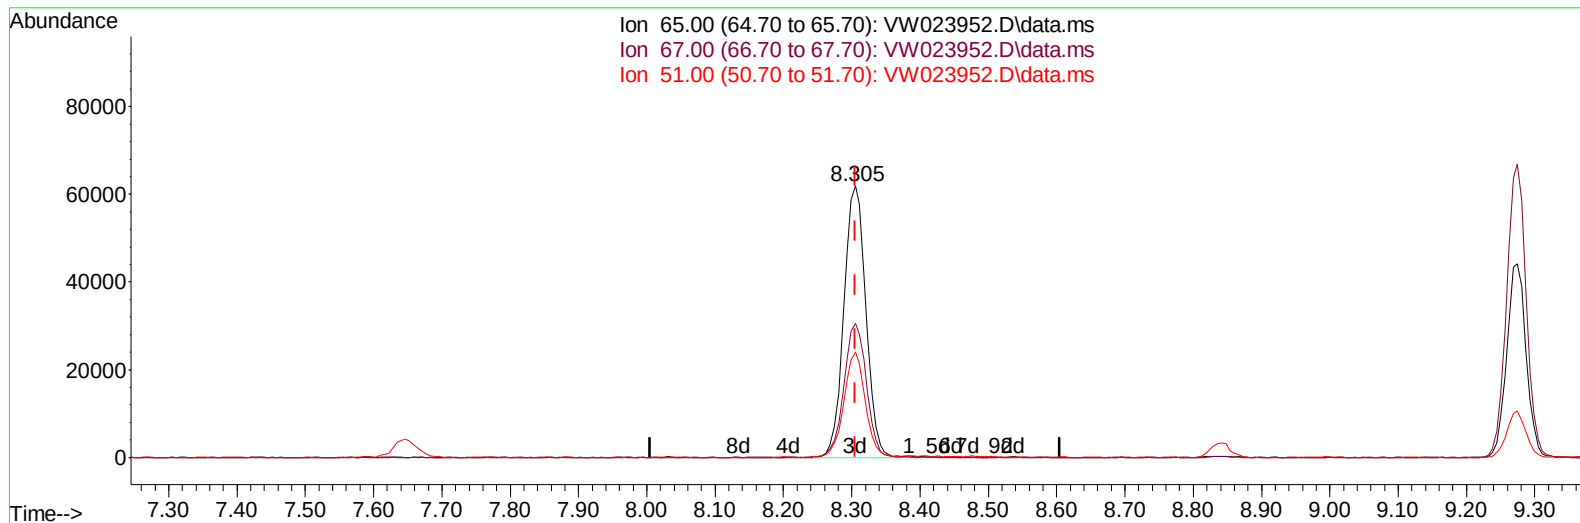

TIC: VW023952.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 25.94 ug/L m

response 138206

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.11#
51.00	92.20	0.28#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
 Data File : VW023952.D
 Acq On : 20 Jul 2022 21:50
 Operator : SY/VA
 Sample : N3741-08
 Misc : 5.67g/10mL/MSVOA_W/SOIL
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B33

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/21/2022
 Supervised By :Mahesh Dadoda 07/21/2022

Quant Time: Jul 21 00:27:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 21 00:18:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	299191	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	257725	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	75085	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	150656	19.715	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	78.880%		
7) Chloroethane-d5	2.873	69	109065	21.394	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.560%		
11) 1,1-Dichloroethene-d2	4.013	63	114138	18.343	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	73.360%		
21) 2-Butanone-d5	7.080	46	46750	39.442	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	78.880%		
24) Chloroform-d	7.647	84	234254	26.892	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	107.560%		
26) 1,2-Dichloroethane-d4	8.305	65	138206m	25.941	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.760%		
32) Benzene-d6	8.274	84	417934	31.195	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	124.800%		
36) 1,2-Dichloropropane-d6	9.274	67	133130	32.989	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	131.960%#		
41) Toluene-d8	10.323	98	365738	26.914	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	107.640%		
43) trans-1,3-Dichloroprop...	10.579	79	41377	21.874	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	87.480%		
47) 2-Hexanone-d5	10.920	63	37196	43.833	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	87.660%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	113677	25.489	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	101.960%		
66) 1,2-Dichlorobenzene-d4	13.853	152	79402	29.623	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	118.480%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
Data File : VW023952.D
Acq On : 20 Jul 2022 21:50
Operator : SY/VA
Sample : N3741-08
Misc : 5.67g/10mL/MSVOA_W/SOIL
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
H0B33

Manual IntegrationsAPPROVED

Quant Time: Jul 21 00:27:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 21 00:18:55 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/21/2022
Supervised By :Mahesh Dadoda 07/21/2022

