

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
 Data File : VW023898.D
 Acq On : 19 Jul 2022 21:41
 Operator : SY/VA
 Sample : N3743-02
 Misc : 6.16g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C88

Quant Time: Jul 20 03:00:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 20 02:42:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	323187	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	299226	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	130299	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	90574	10.973	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	43.880%		
7) Chloroethane-d5	2.879	69	67209	12.205	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	48.800%		
11) 1,1-Dichloroethene-d2	4.007	63	78815	11.726	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	46.920%		
21) 2-Butanone-d5	7.080	46	57689	45.057	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	90.120%		
24) Chloroform-d	7.647	84	199434	21.195	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.760%		
26) 1,2-Dichloroethane-d4	8.305	65	109843	19.087	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	76.360%		
32) Benzene-d6	8.269	84	331869	21.336	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.360%		
36) 1,2-Dichloropropane-d6	9.275	67	112684	24.050	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	96.200%		
41) Toluene-d8	10.323	98	294254	18.650	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	74.600%		
43) trans-1,3-Dichloroprop...	10.573	79	40623	18.497	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	74.000%		
47) 2-Hexanone-d5	10.921	63	48336	49.060	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.120%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	114697	22.151	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	88.600%		
66) 1,2-Dichlorobenzene-d4	13.853	152	105442	22.669	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.680%		
Target Compounds						Qvalue
16) Methylene chloride	4.909	84	25018	4.950	ug/L	92
20) cis-1,2-Dichloroethene	7.165	96	104177	22.623	ug/L #	93
34) Trichloroethene	9.092	95	124647	27.759	ug/L	98
46) Tetrachloroethene	10.860	164	179692	51.755	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
Data File : VW023898.D
Acq On : 19 Jul 2022 21:41
Operator : SY/VA
Sample : N3743-02
Misc : 6.16g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C88

Quant Time: Jul 20 03:00:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 20 02:42:08 2022
Response via : Initial Calibration




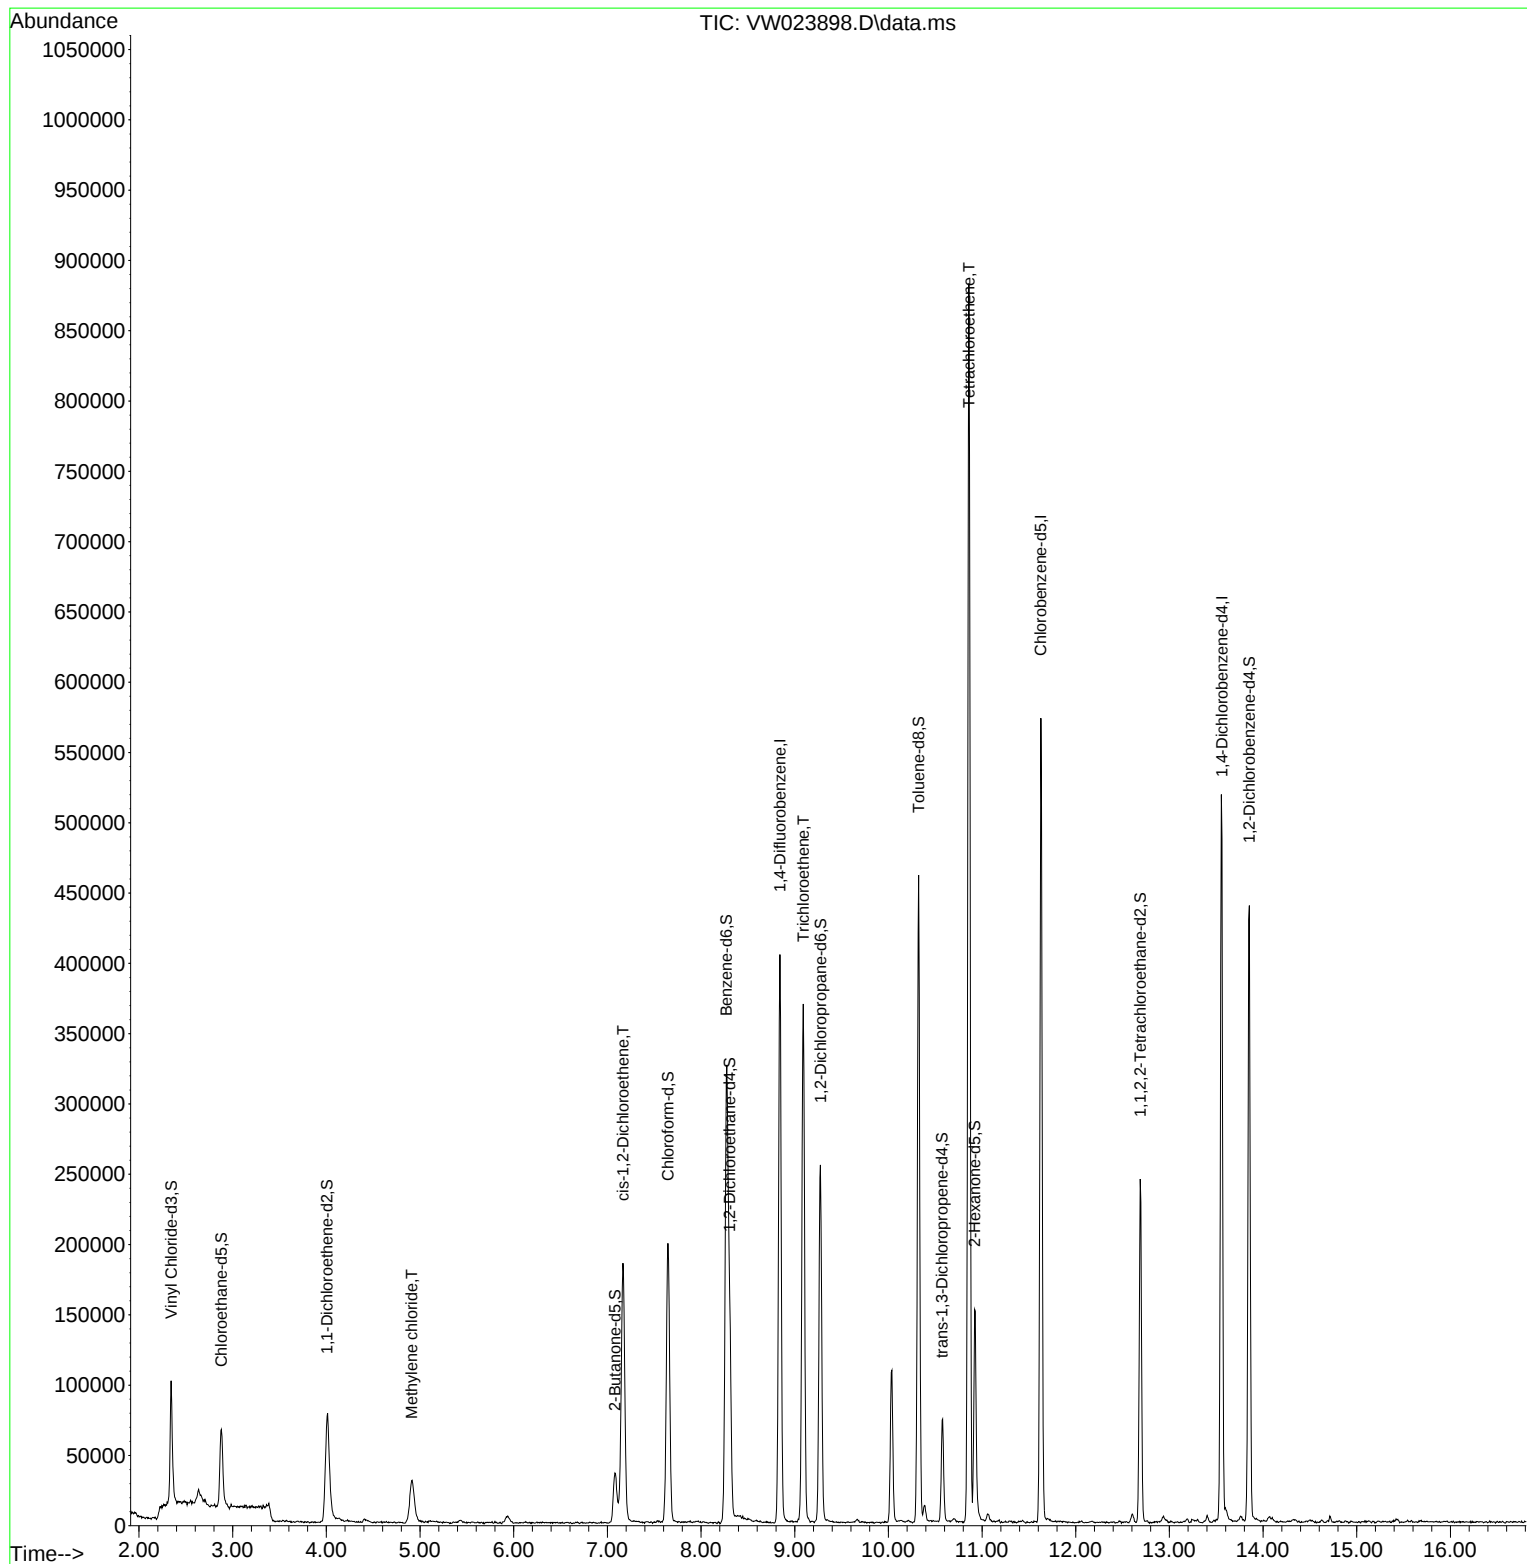


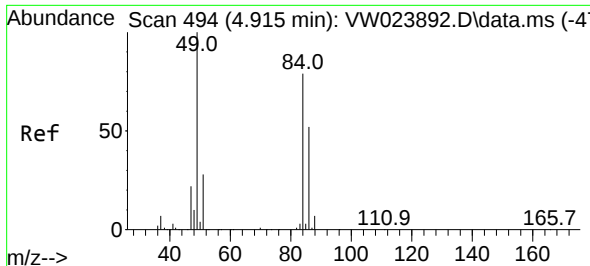

#16
Methylene chloride
Concen: 4.950 ug/L
RT: 4.909 min Scan# 494
Delta R.T. -0.006 min
Lab File: VW023898.D
Acq: 19 Jul 2022 21:41




Instrument :
MSVOA_W
ClientSampleId :
F5C88


Tgt Ion:	84	Resp:	25018
Ion	Ratio	Lower	Upper
84	100		
86	67.3	42.8	79.6
49	113.1	85.4	158.6

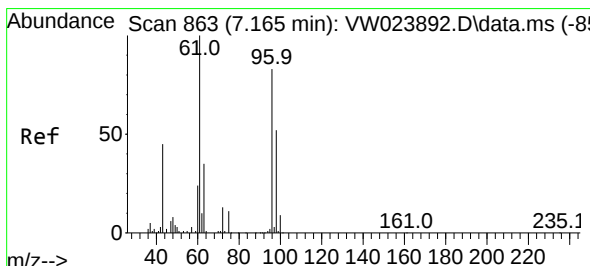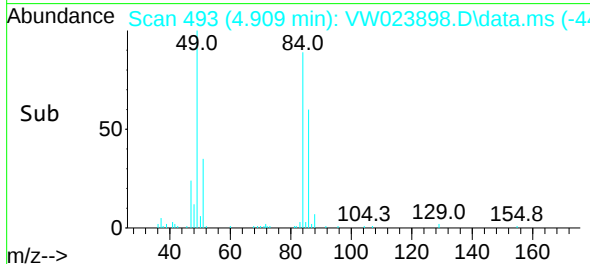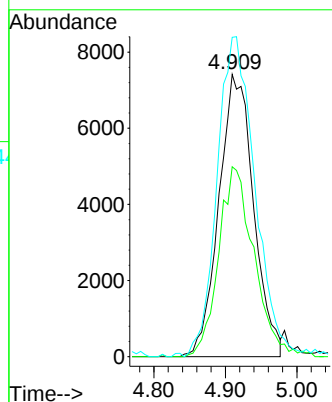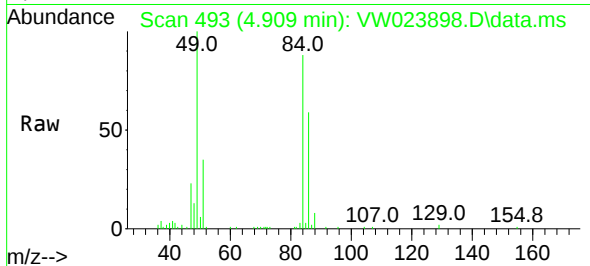

#20
cis-1,2-Dichloroethene
Concen: 22.623 ug/L
RT: 7.165 min Scan# 863
Delta R.T. 0.000 min
Lab File: VW023898.D
Acq: 19 Jul 2022 21:41

Tgt Ion:	96	Resp:	104177
Ion	Ratio	Lower	Upper
96	100		
61	120.8	90.6	168.2
68	0.0	0.2	0.4

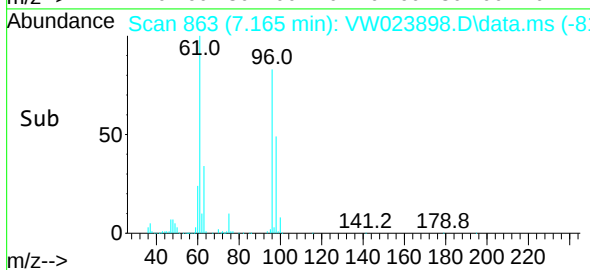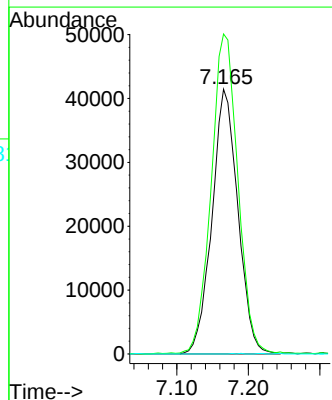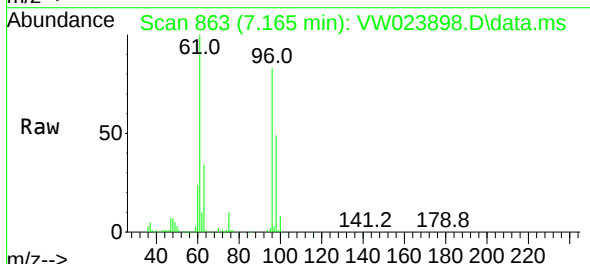

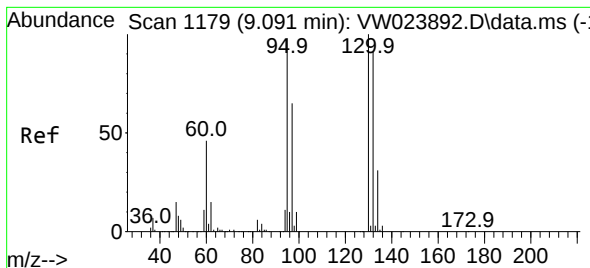

#34

Trichloroethene

Concen: 27.759 ug/L

RT: 9.092 min Scan# 1179

Delta R.T. 0.000 min

Lab File: VW023898.D

Acq: 19 Jul 2022 21:41

Instrument :

MSVOA_W

ClientSampleId :

F5C88

Tgt Ion: 95 Resp: 124647





Ion Ratio Lower Upper

95 100

97 67.7 45.6 84.8

132 103.7 69.9 129.7

130 107.3 75.4 140.0

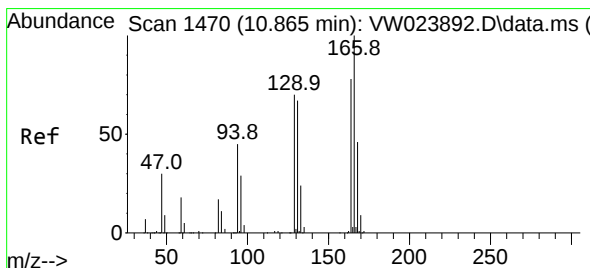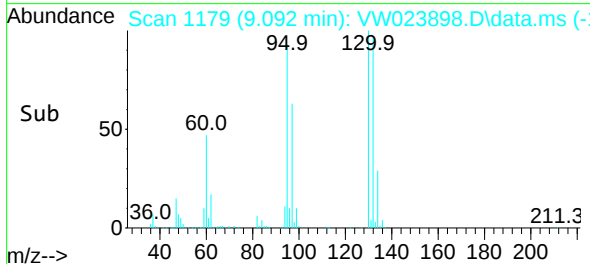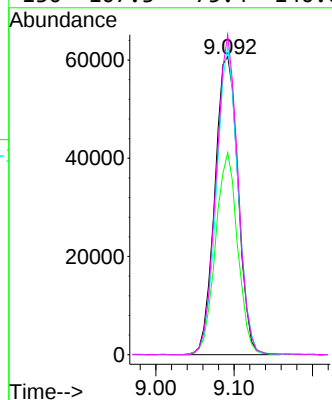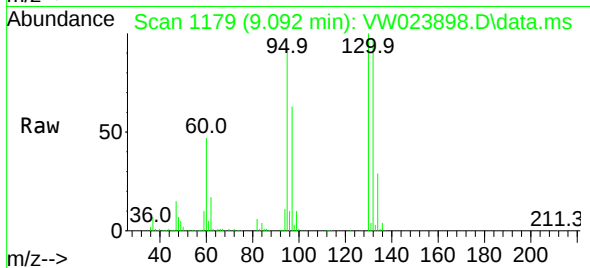

#46

Tetrachloroethene

Concen: 51.755 ug/L

RT: 10.860 min Scan# 1469

Delta R.T. -0.006 min

Lab File: VW023898.D

Acq: 19 Jul 2022 21:41

Tgt Ion:164 Resp: 179692

Ion Ratio Lower Upper

164 100

129 105.6 72.4 134.5

131 93.5 67.8 125.8

166 122.9 88.9 165.1

