
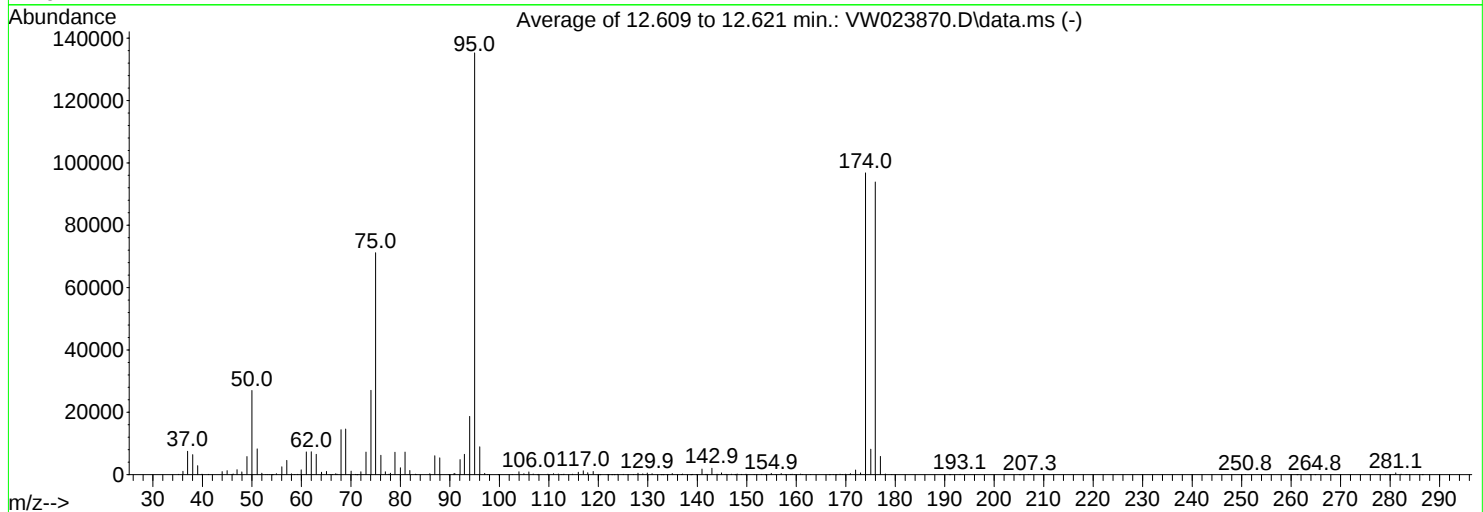


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW071922\
Data File : VW023870.D
Acq On : 19 Jul 2022 07:22
Operator : SY/VA
Sample : BFB589
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB589

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Title : SFAM01.0
Last Update : Thu Jul 21 00:18:55 2022

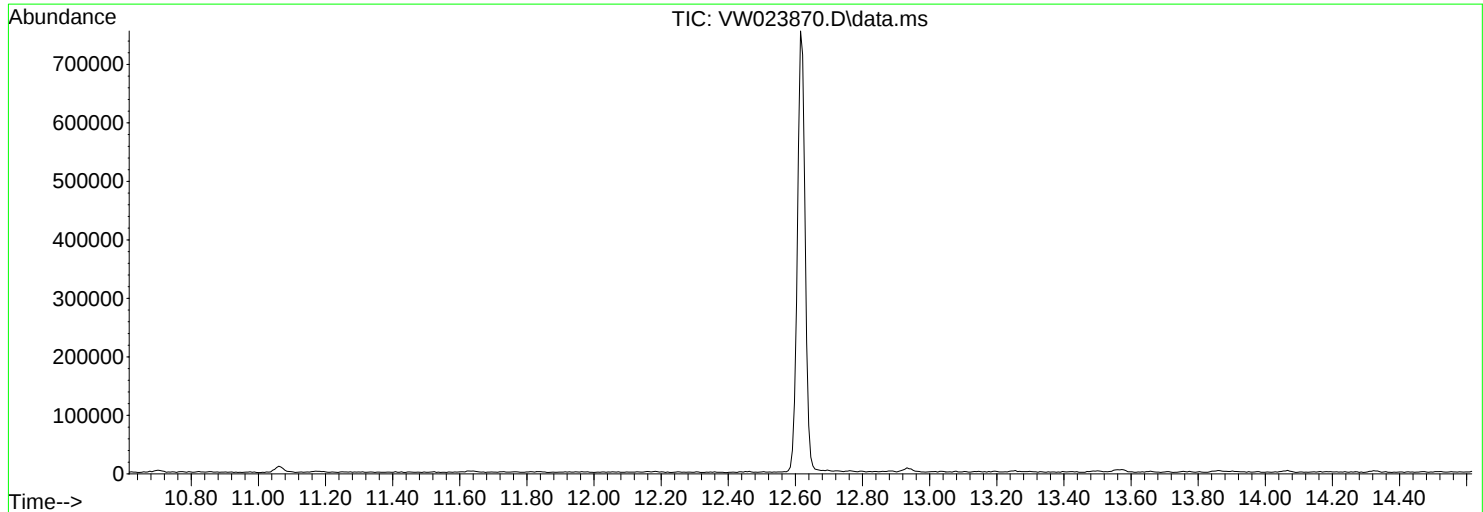

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	26994	PASS
75	95	30	80	52.6	71176	PASS
95	95	100	100	100.0	135296	PASS
96	95	5	9	6.6	8954	PASS
173	174	0.00	2	0.6	570	PASS
174	95	50	120	71.5	96779	PASS
175	174	5	9	8.5	8180	PASS
176	174	95	105	97.0	93853	PASS
177	176	5	10	6.2	5833	PASS

m/z	Abundance
36.10	157.0
37.40	204.0
39.10	109.0
39.80	283.0
41.00	215.0
41.90	105.0
43.00	102.0
44.00	437.0
45.00	93.0
45.70	72.0
47.60	54.0
49.00	53.0
50.20	139.0
51.60	54.0
52.70	99.0
54.10	71.0
55.00	109.0
58.30	60.0
62.90	54.0
64.10	57.0
68.90	53.0
70.20	67.0
72.80	76.0
75.30	105.0
82.50	51.0
82.90	85.0
96.50	65.0
98.70	96.0
118.60	75.0
128.90	55.0
235.70	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB589

m/z	Abundance
35.20	63.0
36.10	1233.0
37.00	7387.0
38.00	5585.0
39.10	2662.0
39.90	441.0
40.90	116.0
41.30	137.0
41.80	130.0
43.00	173.0
44.00	1062.0
45.00	942.0
46.00	277.0
46.90	1584.0
48.00	729.0
49.00	5252.0
50.00	23528.0
51.00	7653.0
52.00	456.0
52.90	141.0
54.10	124.0
55.00	494.0
56.00	2161.0
57.00	4015.0
58.00	234.0
58.70	54.0
59.20	171.0
59.90	1235.0
61.00	6492.0
62.00	6392.0
63.10	5981.0
64.10	586.0
65.10	964.0
65.80	186.0
66.90	313.0
68.00	12168.0
69.00	12611.0
70.10	892.0
70.90	141.0
72.10	826.0
73.10	6458.0
74.10	23416.0
75.00	61360.0
76.00	5266.0
76.90	751.0
77.70	544.0
78.90	6399.0
80.00	1480.0
81.00	6165.0
81.90	1078.0
83.00	223.0
86.00	301.0
87.00	5398.0
87.90	4566.0
90.80	747.0
92.00	3838.0
92.90	5564.0
94.00	16504.0
95.00	111360.0
96.00	7350.0
97.00	292.0
98.70	60.0
102.60	76.0
103.90	822.0
104.90	233.0
105.90	580.0
106.80	164.0
108.00	82.0
110.00	139.0
110.90	198.0
112.00	112.0
112.90	210.0
114.80	164.0
115.90	760.0
117.00	1158.0
117.80	506.0
118.90	757.0
120.00	57.0
123.20	55.0
123.80	121.0
125.20	95.0
127.10	84.0
127.90	564.0
129.10	282.0
129.90	430.0
130.80	279.0
134.90	336.0
136.80	200.0
138.70	60.0
141.00	1328.0
141.70	256.0
142.90	1627.0

Instrument :
MSVOA_W
ClientSampleId :
BFB589

144.10	175.0
144.90	549.0
145.90	123.0
147.00	96.0
147.60	67.0
148.10	279.0
149.00	103.0
149.90	171.0
152.00	76.0
154.90	342.0
157.00	374.0
158.80	119.0
161.00	148.0
162.90	128.0
168.90	152.0
170.00	115.0
171.00	504.0
172.00	1264.0
173.00	1711.0
174.00	72488.0
175.00	6655.0
175.90	70048.0
177.00	4243.0
177.90	126.0
179.30	87.0
193.20	115.0
205.10	60.0
206.90	108.0
279.10	55.0
280.00	130.0
281.20	624.0
282.30	199.0
283.20	168.0
283.90	104.0
286.50	66.0

Instrument :
MSVOA_W
ClientSampleId :
BFB589

m/z	Abundance
35.20	199.0
36.00	1400.0
37.00	8103.0
38.00	7739.0
39.10	3290.0
40.00	447.0
40.80	119.0
41.30	124.0
43.00	100.0
44.00	1626.0
45.00	1765.0
46.20	387.0
47.00	1655.0
48.00	1376.0
49.00	6276.0
50.00	32272.0
51.00	9159.0
52.00	433.0
52.90	311.0
54.20	171.0
54.90	472.0
56.00	2820.0
57.00	5005.0
58.00	346.0
59.20	71.0
60.00	1927.0
61.00	8062.0
62.00	7895.0
63.00	7314.0
64.00	1029.0
65.00	1091.0
67.20	419.0
68.00	16408.0
69.00	16248.0
70.10	1621.0
71.00	105.0
72.00	937.0
73.00	8219.0
74.00	30384.0
75.00	79816.0
76.10	7107.0
76.90	975.0
78.00	800.0
78.90	7604.0
80.00	2743.0
80.90	8383.0
81.90	1535.0
83.10	209.0
85.90	332.0
87.00	6384.0
87.90	6260.0
89.80	77.0
91.00	612.0
92.00	5760.0
93.00	7129.0
94.00	19824.0
95.00	150912.0
96.10	10410.0
97.00	534.0
97.60	66.0
99.80	68.0
102.60	67.0
104.00	965.0
104.90	322.0
105.90	1093.0
106.90	253.0
107.90	166.0
109.80	116.0
110.90	288.0
111.90	236.0
113.10	201.0
114.70	143.0
116.00	955.0
116.90	1298.0
117.80	614.0
118.90	1261.0
119.90	92.0
120.30	82.0
121.80	130.0
122.70	66.0
123.90	103.0
125.00	228.0
126.00	111.0
127.10	53.0
128.00	372.0
129.10	354.0
129.90	567.0
130.90	349.0
133.10	59.0
133.90	63.0
135.00	443.0
136.10	111.0

Instrument :
MSVOA_W
ClientSampleId :
BFB589

137.00	368.0
139.00	78.0
140.90	1869.0
141.90	243.0
143.00	2293.0
143.90	236.0
144.90	764.0
145.90	208.0
146.80	220.0
147.80	403.0
149.00	161.0
149.70	194.0
152.10	103.0
153.10	103.0
153.80	86.0
154.90	493.0
157.00	364.0
158.90	124.0
159.20	107.0
159.70	137.0
160.90	330.0
167.40	70.0
168.00	73.0
168.90	137.0
169.90	216.0
170.90	462.0
172.00	1738.0
174.00	104296.0
175.10	9227.0
176.00	107480.0
177.00	6613.0
178.00	128.0
179.30	56.0
191.00	70.0
193.00	125.0
196.00	53.0
202.20	95.0
207.30	108.0
250.70	52.0
263.80	51.0
279.00	53.0
281.00	369.0
281.20	367.0
282.10	233.0
283.40	99.0

Instrument :
MSVOA_W
ClientSampleId :
BFB589

m/z	Abundance
36.10	1067.0
37.00	6991.0
38.10	5965.0
39.00	2995.0
40.10	423.0
41.20	105.0
44.00	1526.0
45.10	1402.0
46.20	309.0
47.10	1476.0
47.80	510.0
49.00	6104.0
50.00	25600.0
51.10	8034.0
52.00	526.0
53.10	147.0
53.50	99.0
55.00	335.0
56.10	2547.0
57.10	4739.0
58.10	184.0
58.60	118.0
59.30	160.0
60.00	1538.0
61.00	7352.0
62.00	7773.0
63.10	6418.0
64.00	853.0
65.00	1025.0
66.30	158.0
67.00	662.0
68.00	14735.0
69.00	15200.0
69.90	1032.0
71.20	90.0
71.90	1073.0
73.10	7082.0
74.10	27432.0
75.00	72352.0
76.10	6336.0
77.00	1043.0
78.00	598.0
78.90	7503.0
80.00	2413.0
81.00	7142.0
81.90	1455.0
82.80	178.0
83.30	106.0
85.90	340.0
86.90	6456.0
88.00	5404.0
91.00	605.0
92.10	4948.0
93.00	6954.0
94.00	19664.0
95.00	143616.0
96.00	9103.0
97.10	395.0
97.70	95.0
103.90	1048.0
105.00	315.0
106.00	984.0
106.90	262.0
107.70	91.0
109.70	217.0
111.00	398.0
111.80	219.0
112.50	160.0
113.00	206.0
114.80	148.0
116.00	573.0
117.00	1210.0
117.90	691.0
119.00	1116.0
119.90	124.0
122.00	58.0
123.90	87.0
128.10	469.0
128.90	351.0
129.90	510.0
130.80	287.0
132.70	67.0
135.00	267.0
136.00	121.0
137.00	255.0
139.10	164.0
139.90	238.0
141.00	2242.0
142.10	309.0
142.90	2191.0
144.20	157.0
144.90	366.0

Instrument :
MSVOA_W
ClientSampleId :
BFB589

145.60	268.0
146.20	226.0
147.00	147.0
148.00	355.0
148.80	57.0
149.90	165.0
151.50	145.0
152.90	141.0
154.00	137.0
155.00	385.0
155.90	156.0
156.90	317.0
157.80	87.0
159.10	305.0
160.80	182.0
161.30	135.0
166.70	90.0
167.50	89.0
168.70	146.0
169.30	213.0
170.00	105.0
170.70	374.0
172.00	1518.0
174.00	113552.0
175.00	8657.0
176.00	104032.0
177.00	6644.0
178.00	359.0
193.10	86.0
196.00	70.0
207.20	78.0
250.80	56.0
261.20	59.0
264.80	81.0
280.80	230.0
281.20	283.0
282.20	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB589