




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
 Data File : VW023980.D
 Acq On : 21 Jul 2022 14:24
 Operator : SY/VA
 Sample : N3722-12
 Misc : 5.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C47

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:31:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 01:28:21 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
 Supervised By :Semsettin Yesilyurt 07/22/2022

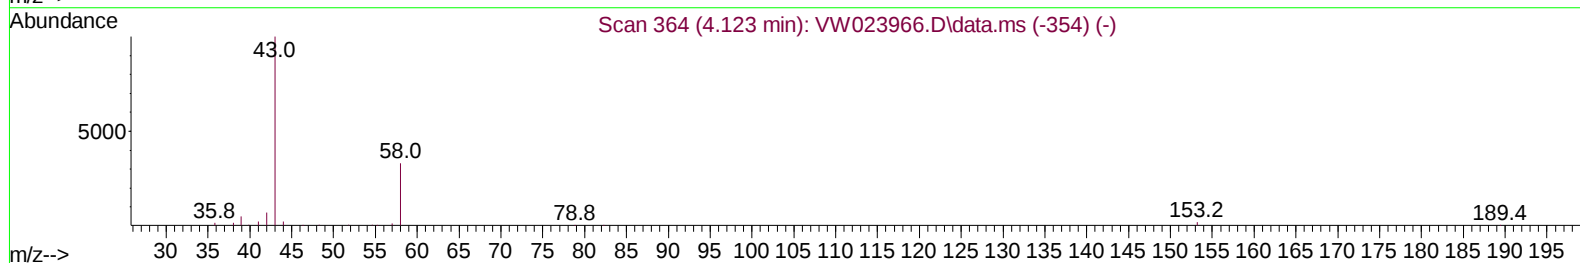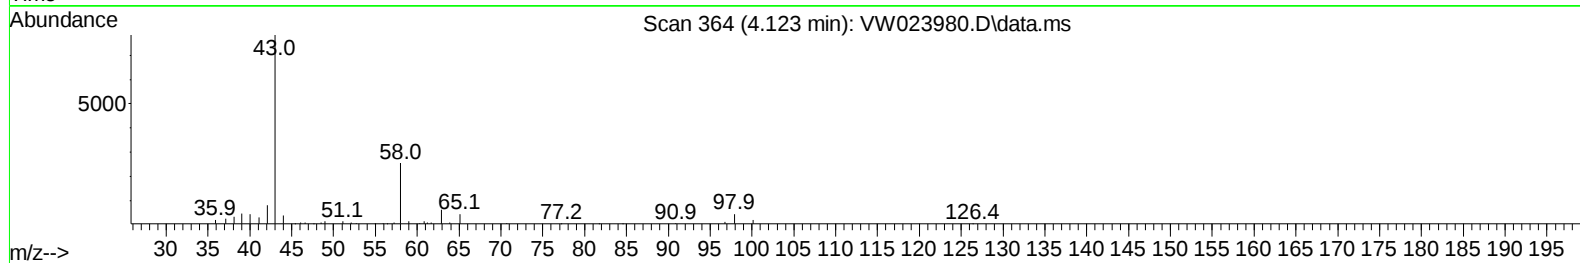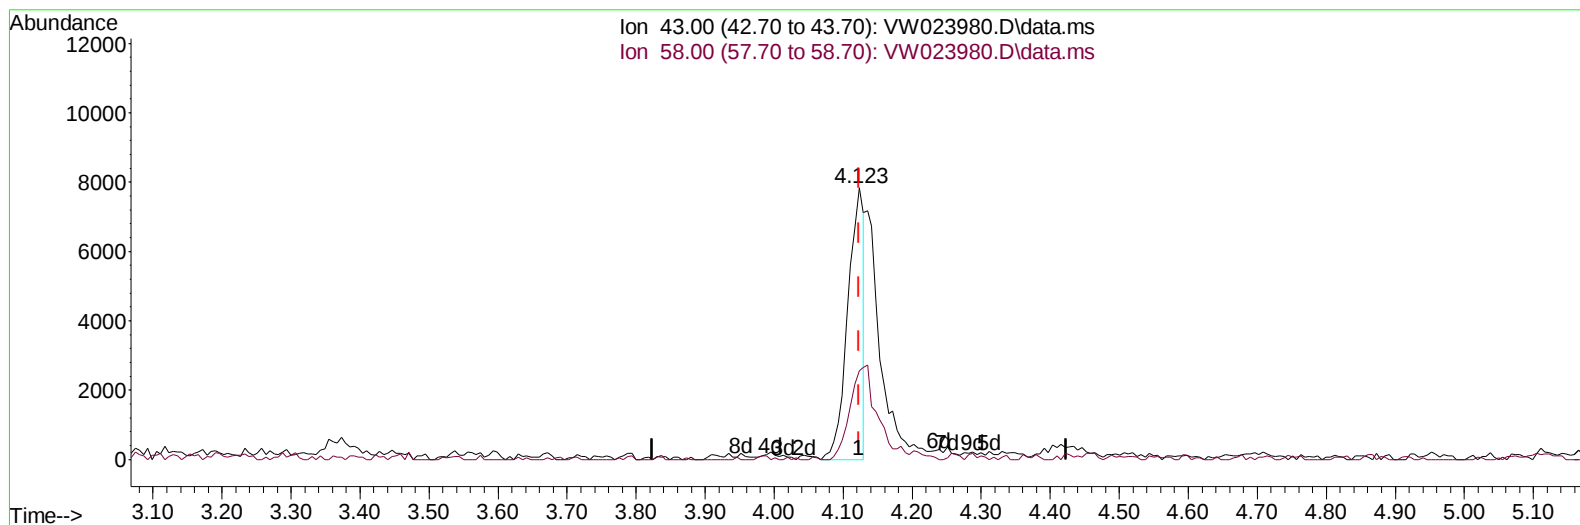

TIC: VW023980.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 13.80 ug/L

response 12783

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	55.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
 Data File : VW023980.D
 Acq On : 21 Jul 2022 14:24
 Operator : SY/VA
 Sample : N3722-12
 Misc : 5.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C47

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:31:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 01:28:21 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
 Supervised By :Semsettin Yesilyurt 07/22/2022

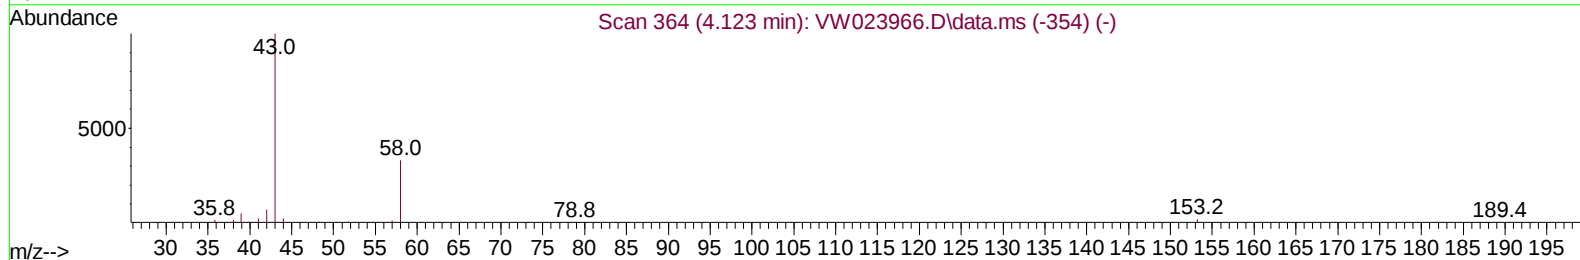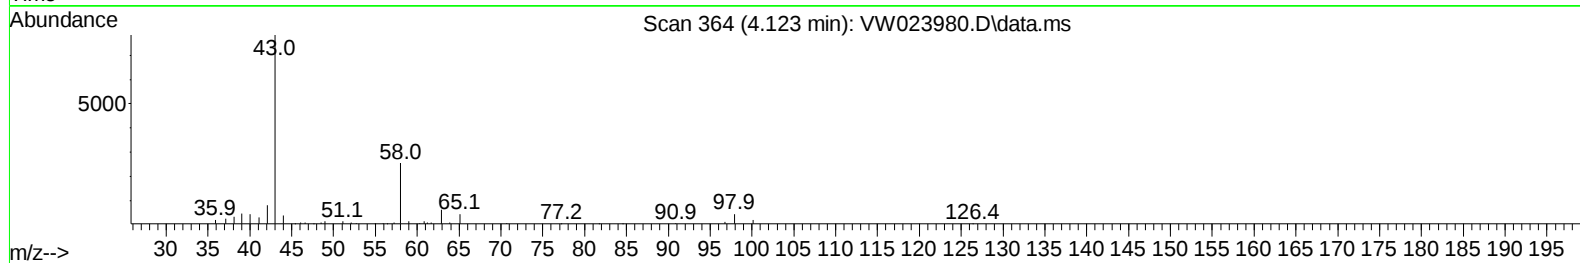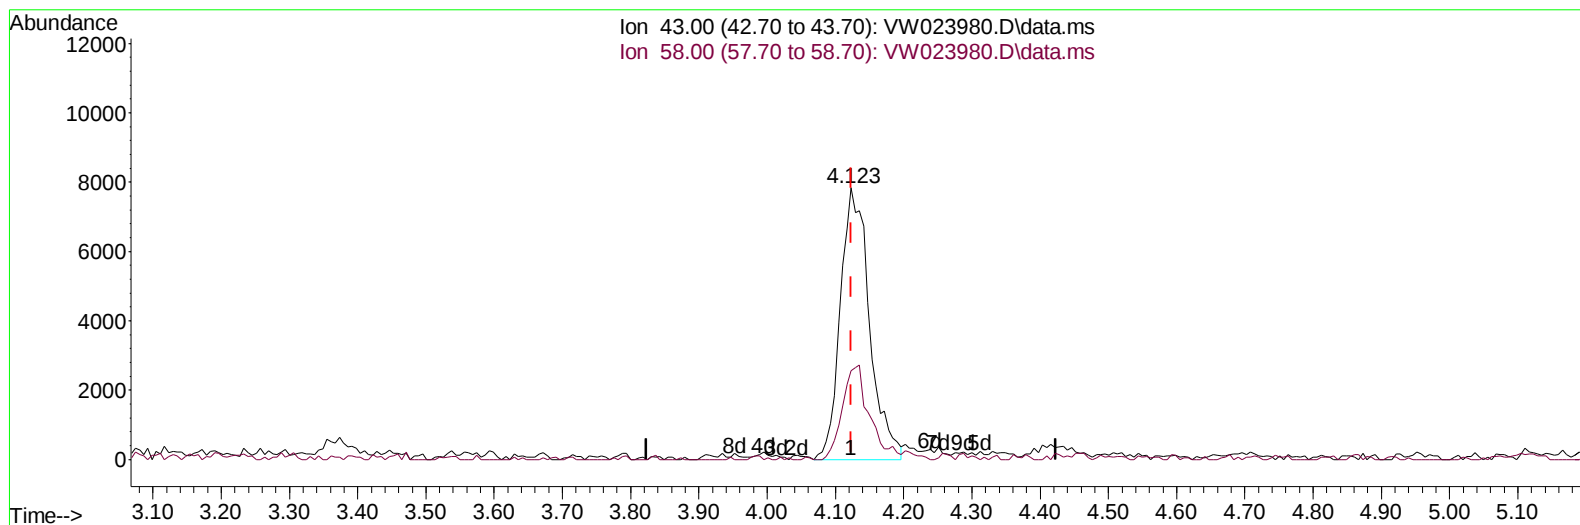

TIC: VW023980.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 25.04 ug/L m

response 23198

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	30.39
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
 Data File : VW023980.D
 Acq On : 21 Jul 2022 14:24
 Operator : SY/VA
 Sample : N3722-12
 Misc : 5.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C47

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:31:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 01:28:21 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
 Supervised By :Semsettin Yesilyurt 07/22/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	330707	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	310868	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	128080	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	130127	15.406	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	61.640%	
7) Chloroethane-d5	2.879	69	102004	18.102	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	72.400%	
11) 1,1-Dichloroethene-d2	4.007	63	100946	14.677	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	58.720%	
21) 2-Butanone-d5	7.080	46	60329	46.048	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	92.100%	
24) Chloroform-d	7.647	84	206322	21.428	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	85.720%	
26) 1,2-Dichloroethane-d4	8.305	65	119996	20.377	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	81.520%	
32) Benzene-d6	8.269	84	378296	23.410	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	93.640%	
36) 1,2-Dichloropropane-d6	9.274	67	119013	24.450	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	97.800%	
41) Toluene-d8	10.323	98	338563	20.655	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	82.600%	
43) trans-1,3-Dichloroprop...	10.573	79	43994	19.282	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.120%	
47) 2-Hexanone-d5	10.927	63	50604	49.439	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.880%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	114886	21.357	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	85.440%	
66) 1,2-Dichlorobenzene-d4	13.853	152	107429	23.496	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	94.000%	
Target Compounds						
					Qvalue	
13) Acetone	4.123	43	23198m	25.044	ug/L	
16) Methylene chloride	4.909	84	22877	4.424	ug/L	86
20) cis-1,2-Dichloroethene	7.171	96	5960	1.265	ug/L #	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
Data File : VW023980.D
Acq On : 21 Jul 2022 14:24
Operator : SY/VA
Sample : N3722-12
Misc : 5.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C47

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/22/2022
Supervised By :Semsettin Yesilyurt 07/22/2022

Quant Time: Jul 22 01:31:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 22 01:28:21 2022
Response via : Initial Calibration

