




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
Data File : VW023982.D
Acq On : 21 Jul 2022 15:13
Operator : SY/VA
Sample : N3722-14RE
Misc : 6.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C50RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:32:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 22 01:28:21 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
Supervised By :Semsettin Yesilyurt 07/22/2022

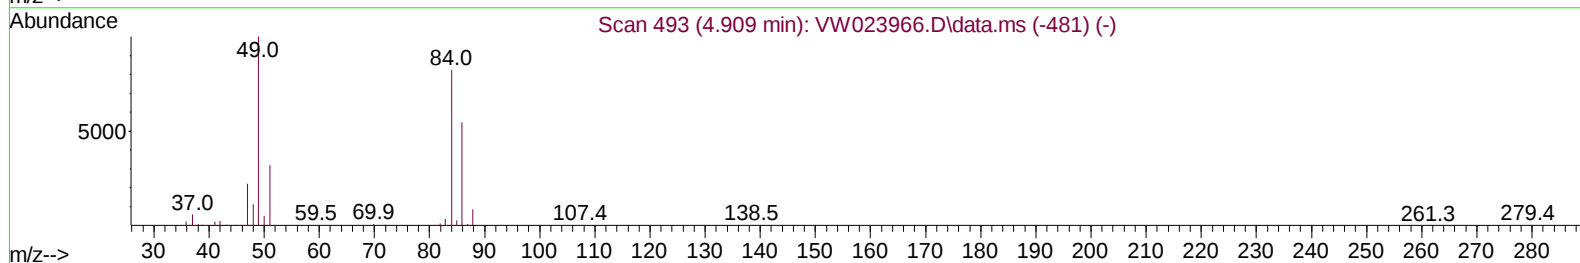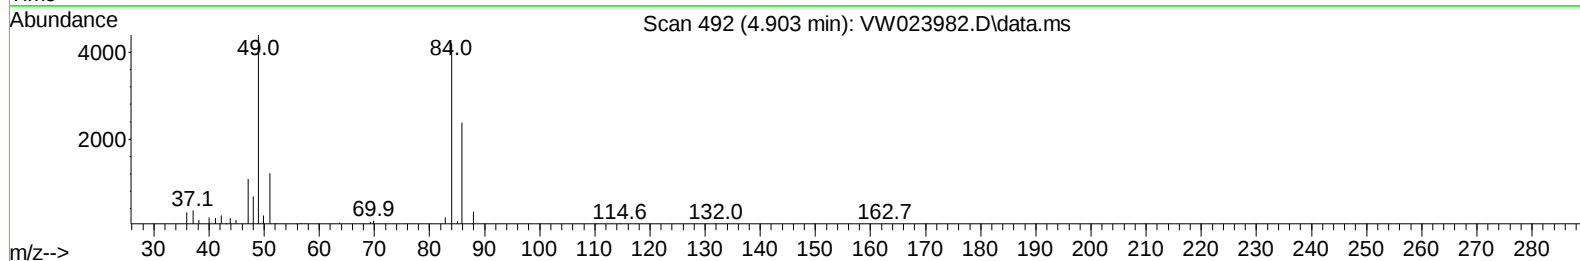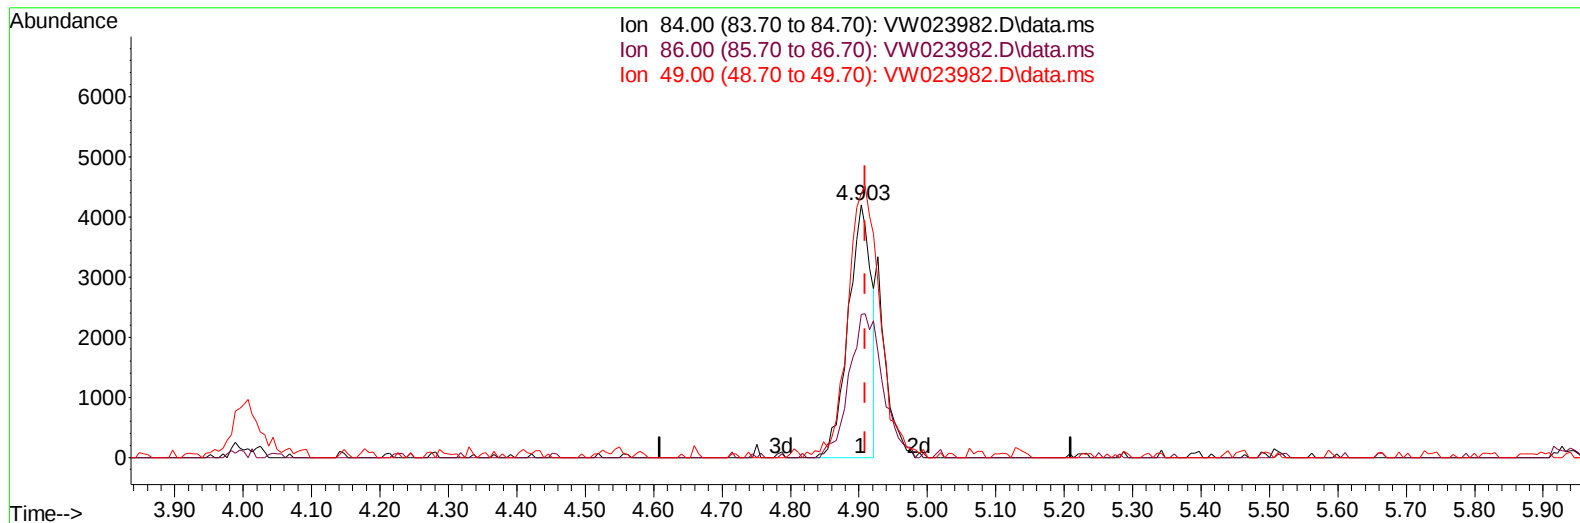

TIC: VW023982.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.006) 4.13 ug/L

response 9845

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	56.78
49.00	122.00	104.69
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
Data File : VW023982.D
Acq On : 21 Jul 2022 15:13
Operator : SY/VA
Sample : N3722-14RE
Misc : 6.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C50RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:32:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 22 01:28:21 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
Supervised By :Semsettin Yesilyurt 07/22/2022

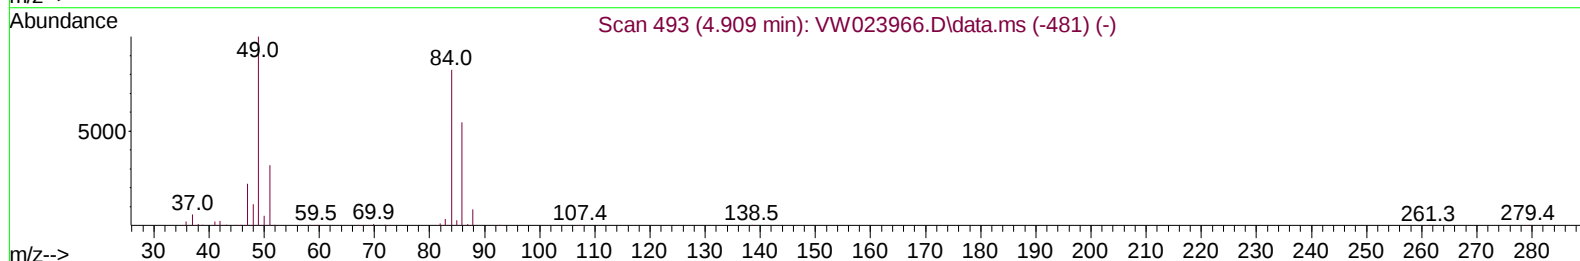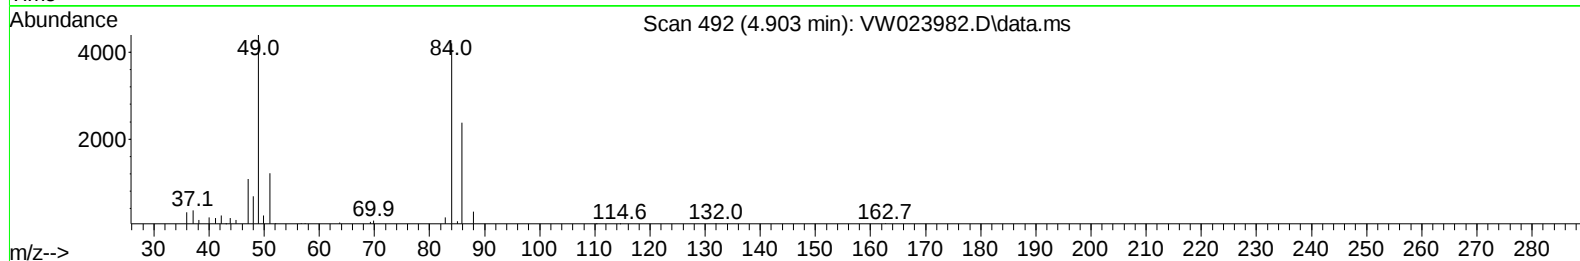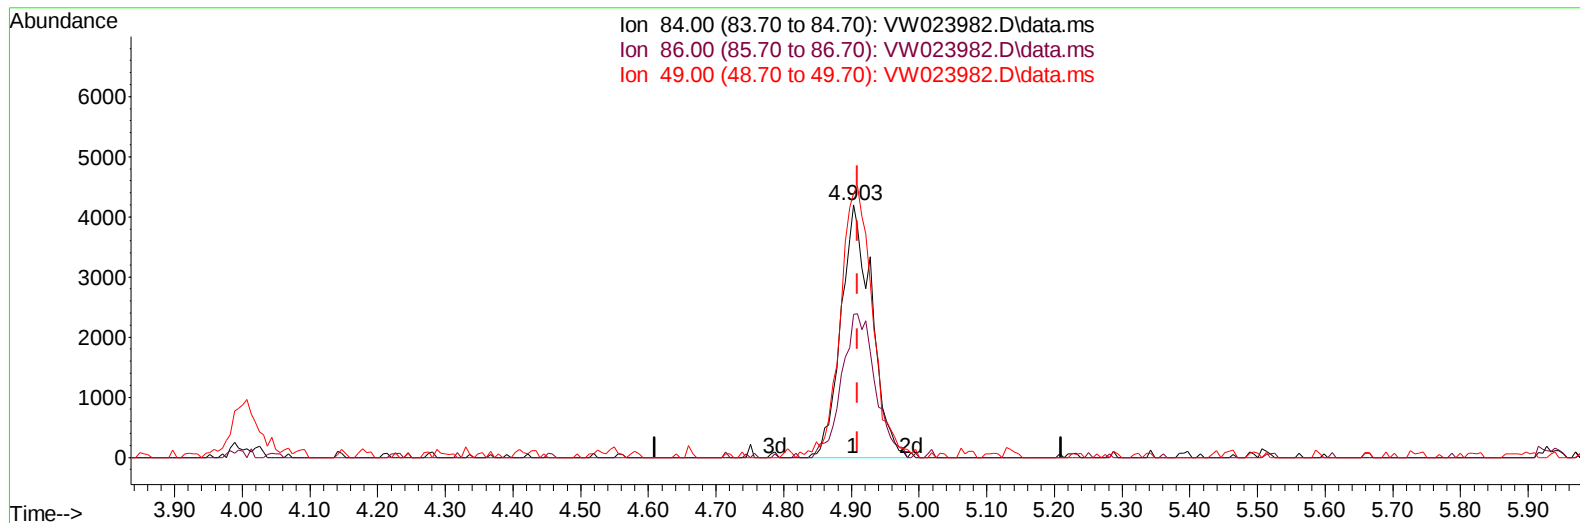

TIC: VW023982.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.006) 5.57 ug/L m

response 13273

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	56.78
49.00	122.00	104.69
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
 Data File : VW023982.D
 Acq On : 21 Jul 2022 15:13
 Operator : SY/VA
 Sample : N3722-14RE
 Misc : 6.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C50RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:32:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 01:28:21 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
 Supervised By :Semsettin Yesilyurt 07/22/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		152328	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117		152357	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		58254	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.336	65		71586	18.400	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	73.600%		
7) Chloroethane-d5	2.873	69		45962	17.708	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	70.840%		
11) 1,1-Dichloroethene-d2	4.001	63		56740	17.910	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	71.640%		
21) 2-Butanone-d5	7.080	46		32654	54.110	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	108.220%		
24) Chloroform-d	7.646	84		115578	26.061	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	104.240%		
26) 1,2-Dichloroethane-d4	8.305	65		65812	24.263	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	97.040%		
32) Benzene-d6	8.274	84		196912	24.863	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	99.440%		
36) 1,2-Dichloropropane-d6	9.274	67		63344	26.552	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	106.200%		
41) Toluene-d8	10.323	98		170028	21.165	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	84.680%		
43) trans-1,3-Dichloroprop...	10.579	79		21457	19.188	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	76.760%		
47) 2-Hexanone-d5	10.926	63		23379	46.604	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	93.200%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		63143	23.950	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	95.800%		
66) 1,2-Dichlorobenzene-d4	13.853	152		54950	26.424	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	105.680%		
Target Compounds							
						Qvalue	
13) Acetone	4.123	43		12126	28.421	ug/L	98
14) Carbon disulfide	4.367	76		13718	2.888	ug/L	98
16) Methylene chloride	4.903	84		13273m	5.572	ug/L	
42) Toluene	10.384	91		10842	1.098	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
Data File : VW023982.D
Acq On : 21 Jul 2022 15:13
Operator : SY/VA
Sample : N3722-14RE
Misc : 6.39g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C50RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:32:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 22 01:28:21 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
Supervised By :Semsettin Yesilyurt 07/22/2022

