




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
 Data File : VW023985.D
 Acq On : 21 Jul 2022 16:28
 Operator : SY/VA
 Sample : N3721-20RE
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C62RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:32:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 01:28:21 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
 Supervised By :Semsettin Yesilyurt 07/22/2022

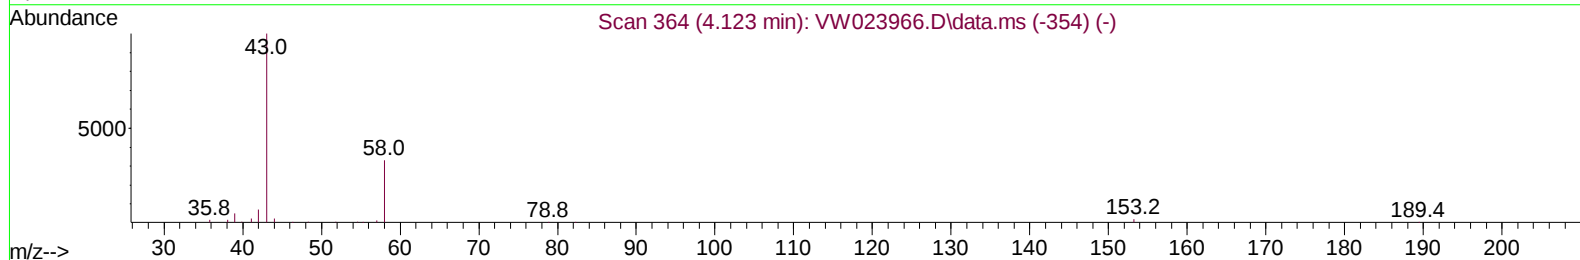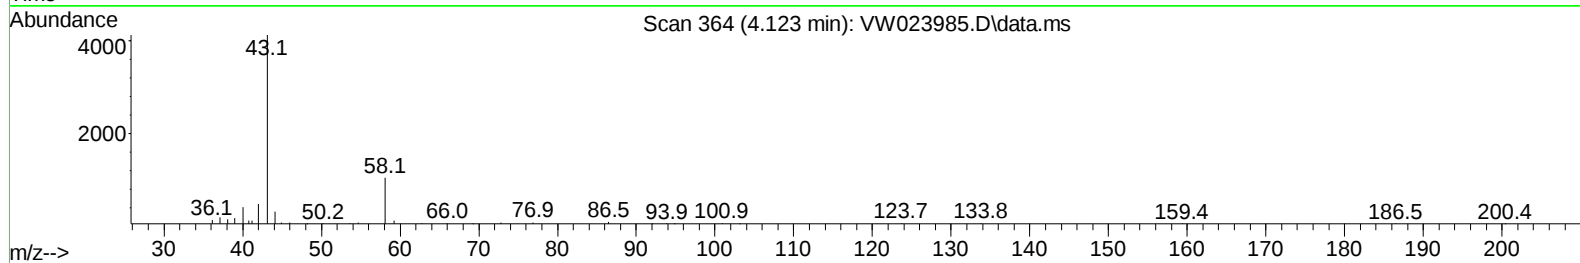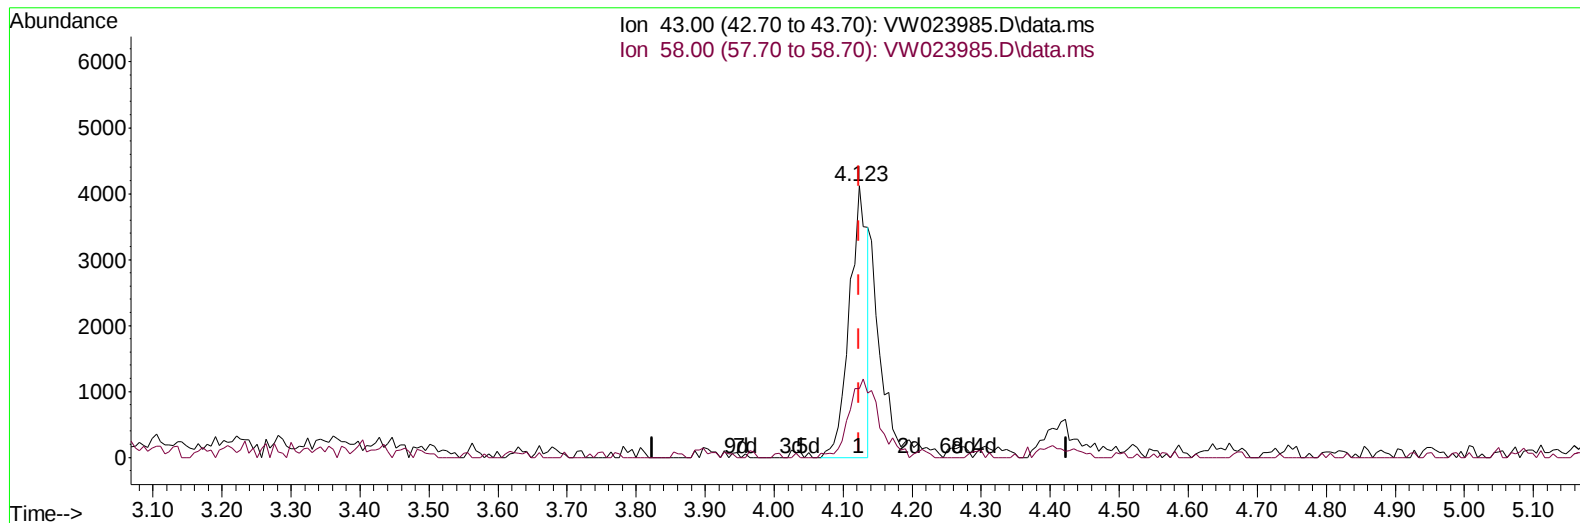

TIC: VW023985.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 43.00 ug/L

response 7359

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	46.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
 Data File : VW023985.D
 Acq On : 21 Jul 2022 16:28
 Operator : SY/VA
 Sample : N3721-20RE
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C62RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:32:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 01:28:21 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
 Supervised By :Semsettin Yesilyurt 07/22/2022

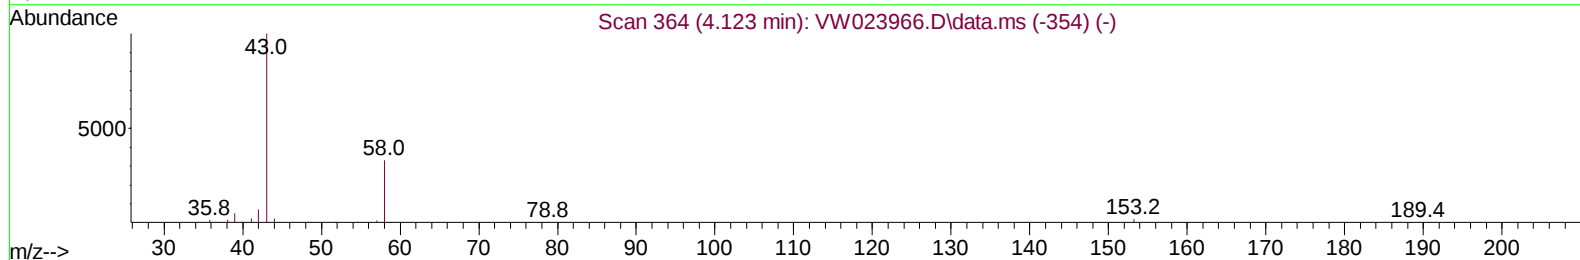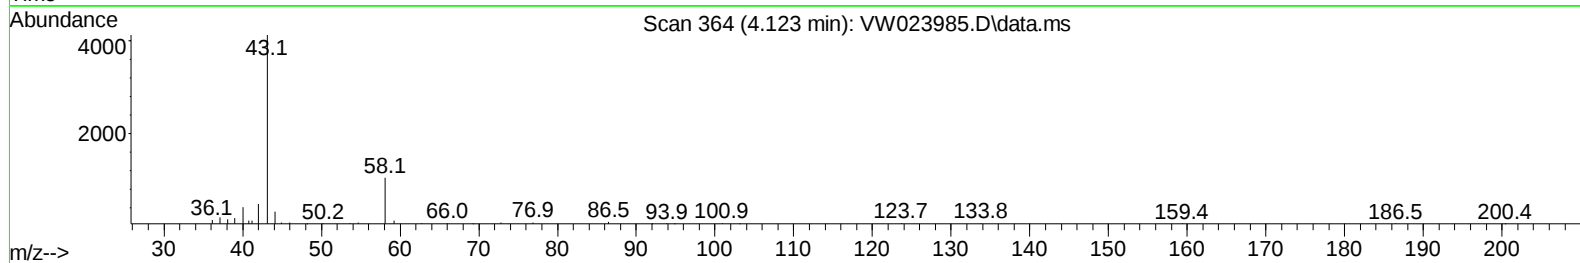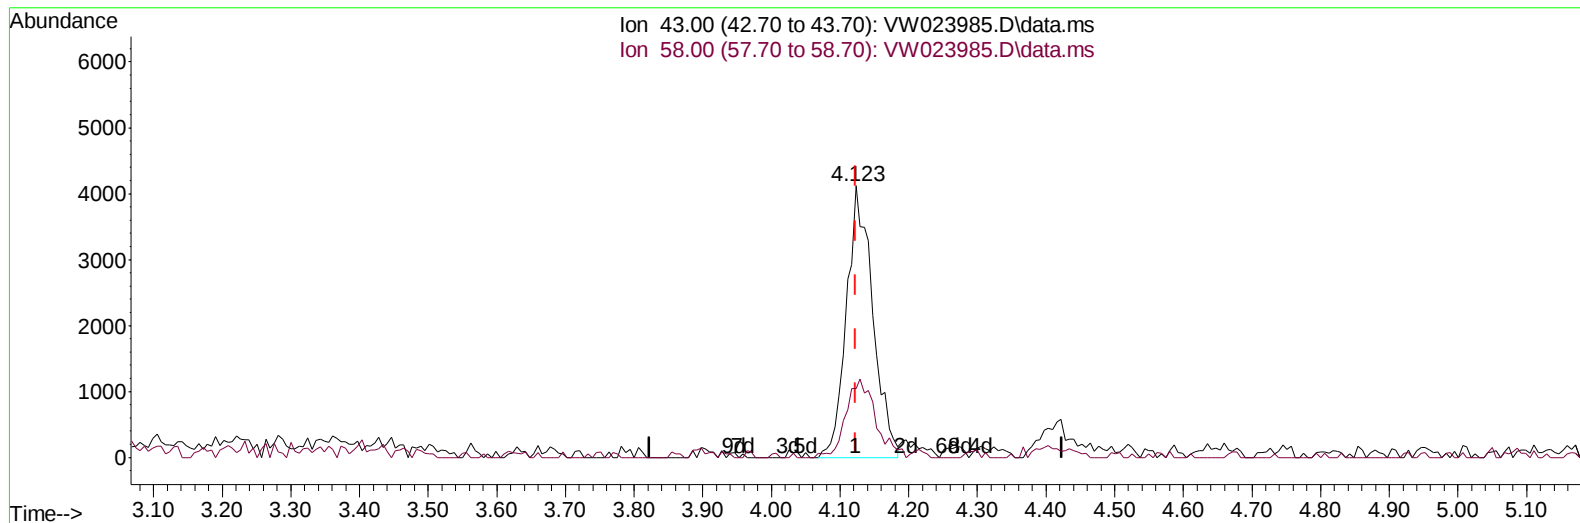

TIC: VW023985.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 63.94 ug/L m

response 10943

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	31.27
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
 Data File : VW023985.D
 Acq On : 21 Jul 2022 16:28
 Operator : SY/VA
 Sample : N3721-20RE
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C62RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:32:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 01:28:21 2022
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
 Supervised By :Semsettin Yesilyurt 07/22/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		61100	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		56751	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		21111	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.337	65		32538	20.850	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	83.400%	
7) Chloroethane-d5	2.873	69		21556	20.706	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	82.840%	
11) 1,1-Dichloroethene-d2	4.001	63		26451	20.815	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	83.280%	
21) 2-Butanone-d5	7.086	46		14981	61.890	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	123.780%	
24) Chloroform-d	7.647	84		46294	26.024	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	104.080%	
26) 1,2-Dichloroethane-d4	8.305	65		26202	24.083	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	96.320%	
32) Benzene-d6	8.275	84		76569	25.955	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	103.800%	
36) 1,2-Dichloropropane-d6	9.274	67		25605	28.814	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	115.240%	
41) Toluene-d8	10.323	98		58826	19.659	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	78.640%	
43) trans-1,3-Dichloroprop...	10.579	79		8374	20.104	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	80.400%	
47) 2-Hexanone-d5	10.927	63		8786	47.019	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	94.040%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		26403	26.886	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	107.560%	
66) 1,2-Dichlorobenzene-d4	13.853	152		19042	25.267	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	101.080%	
Target Compounds							
13) Acetone	4.123	43		10943m	63.943	ug/L	
16) Methylene chloride	4.903	84		6846	7.165	ug/L	88
20) cis-1,2-Dichloroethene	7.171	96		7654	8.792	ug/L #	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
Data File : VW023985.D
Acq On : 21 Jul 2022 16:28
Operator : SY/VA
Sample : N3721-20RE
Misc : 5.58g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F5C62RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 01:32:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 22 01:28:21 2022
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022
Supervised By :Semsettin Yesilyurt 07/22/2022

