

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
 Data File : VW023972.D
 Acq On : 21 Jul 2022 11:08
 Operator : SY/VA
 Sample : N3658-04
 Misc : 5.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Jul 22 01:30:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 01:28:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	264529	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	256966	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	115185	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	136327	20.178	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.720%		
7) Chloroethane-d5	2.879	69	96322	21.370	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.480%		
11) 1,1-Dichloroethene-d2	4.013	63	104271	18.953	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	75.800%		
21) 2-Butanone-d5	7.080	46	58590	55.908	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	111.820%		
24) Chloroform-d	7.647	84	192788	25.032	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	100.120%		
26) 1,2-Dichloroethane-d4	8.305	65	113347	24.063	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	96.240%		
32) Benzene-d6	8.275	84	354906	26.569	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	106.280%		
36) 1,2-Dichloropropane-d6	9.274	67	109610	27.241	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	108.960%		
41) Toluene-d8	10.323	98	325202	24.001	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	96.000%		
43) trans-1,3-Dichloroprop...	10.579	79	45932	24.354	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	97.400%		
47) 2-Hexanone-d5	10.927	63	47819	56.518	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	113.040%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	111390	25.050	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	100.200%		
66) 1,2-Dichlorobenzene-d4	13.847	152	118412	28.798	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	115.200%		
Target Compounds						Qvalue
16) Methylene chloride	4.909	84	16229	3.923	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072122\
Data File : VW023972.D
Acq On : 21 Jul 2022 11:08
Operator : SY/VA
Sample : N3658-04
Misc : 5.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001


Quant Time: Jul 22 01:30:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 22 01:28:21 2022
Response via : Initial Calibration

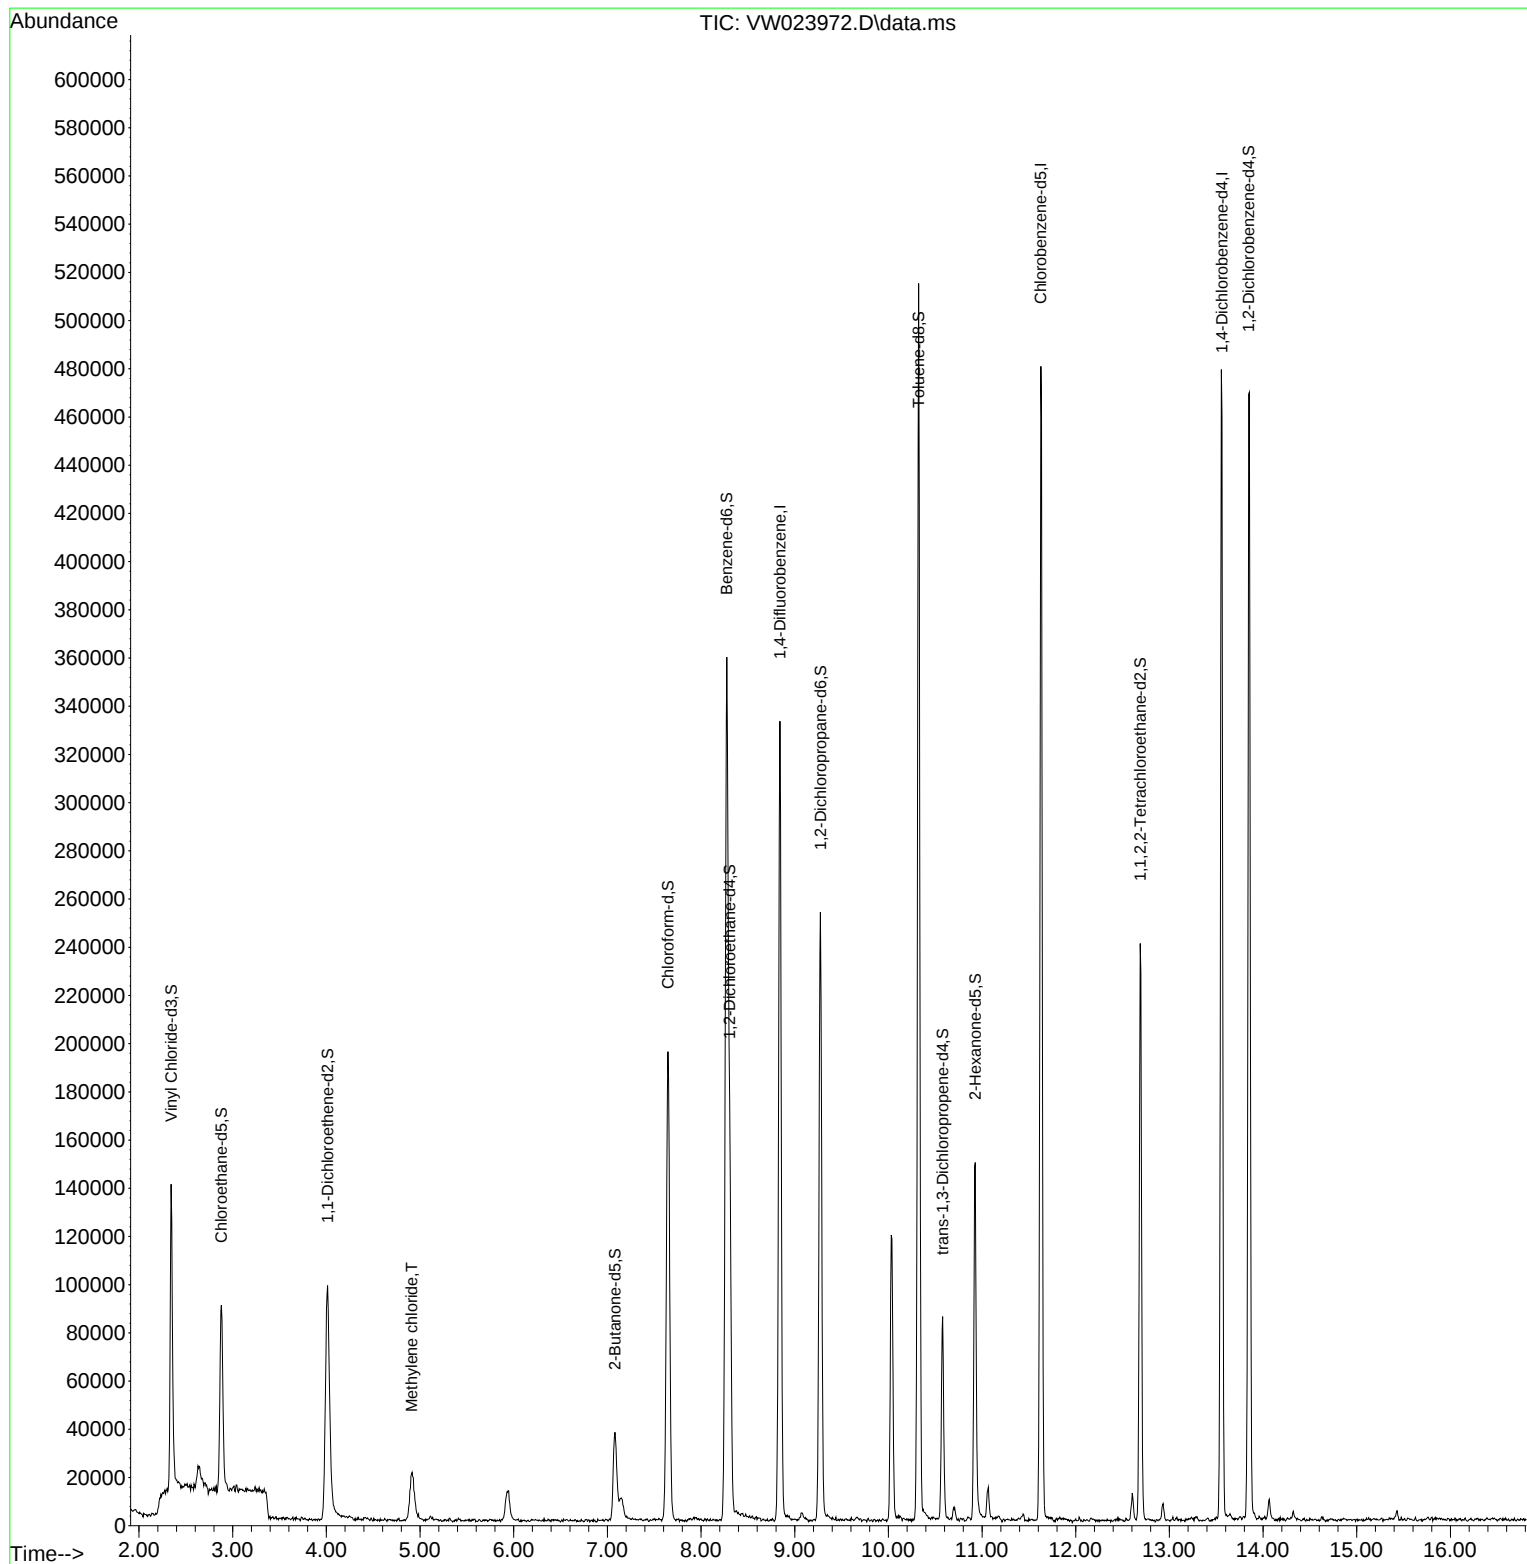

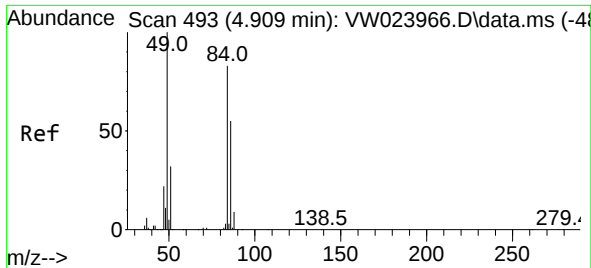

#16
Methylene chloride
Concen: 3.923 ug/L
RT: 4.909 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW023972.D
Acq: 21 Jul 2022 11:08

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

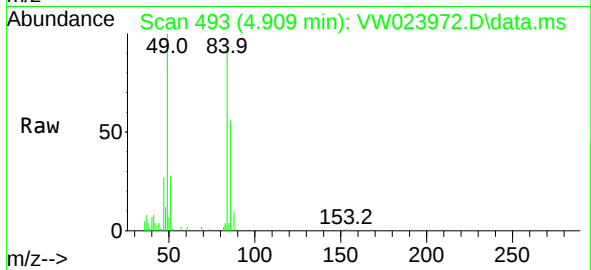

Tgt Ion:	84	Resp:	16229
Ion	Ratio	Lower	Upper
84	100		
86	61.0	42.8	79.6
49	108.2	85.4	158.6

