

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024039.D
 Acq On : 23 Jul 2022 08:15
 Operator : SY/VA
 Sample : N3790-08
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 24 00:40:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 06:00:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	242612	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	229812	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	88087	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	101448	16.372	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.480%
7) Chloroethane-d5	2.873	69	76601	18.530	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.120%
11) 1,1-Dichloroethene-d2	4.007	63	70384	13.949	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.800%
21) 2-Butanone-d5	7.080	46	43484	45.242	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.480%
24) Chloroform-d	7.647	84	156237	22.119	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.480%
26) 1,2-Dichloroethane-d4	8.305	65	91599	21.203	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.800%
32) Benzene-d6	8.275	84	267705	22.409	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.640%
36) 1,2-Dichloropropane-d6	9.274	67	86988	24.174	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.680%
41) Toluene-d8	10.323	98	239496	19.765	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.040%
43) trans-1,3-Dichloroprop...	10.573	79	33415	19.810	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.240%
47) 2-Hexanone-d5	10.927	63	35869	47.403	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.800%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	85755	21.564	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	77882	24.768	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.080%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	3218	0.652	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024039.D
Acq On : 23 Jul 2022 08:15
Operator : SY/VA
Sample : N3790-08
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jul 24 00:40:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 06:00:17 2022
Response via : Initial Calibration

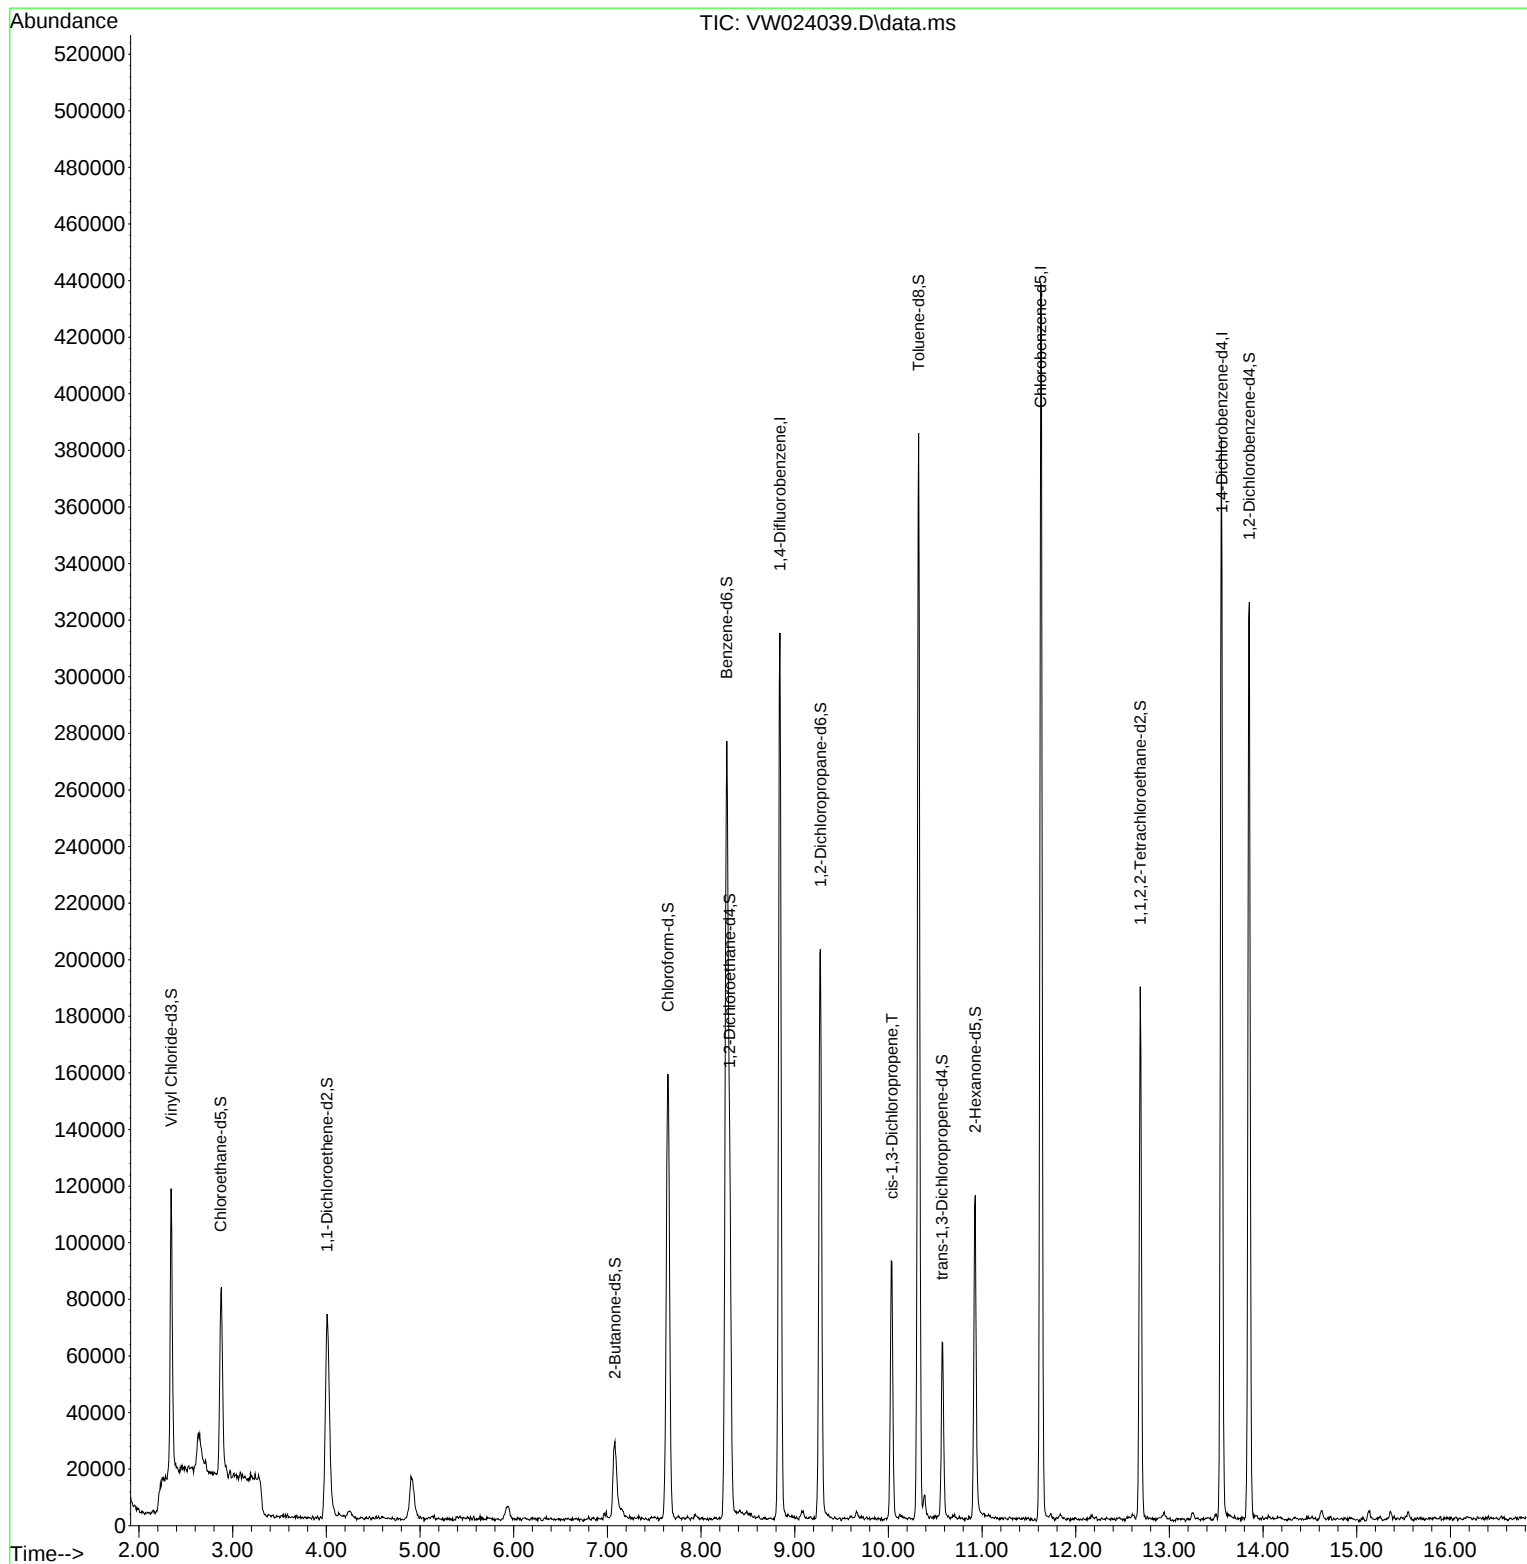

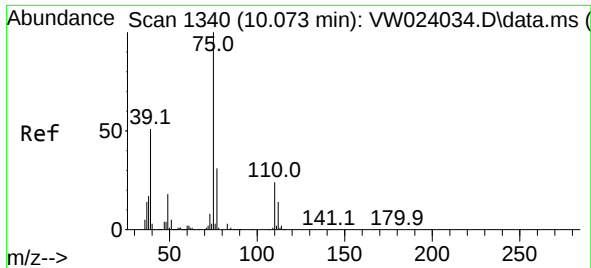

#39
 cis-1,3-Dichloropropene
 Concen: 0.652 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW024039.D
 Acq: 23 Jul 2022 08:15

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3218
 Ion Ratio Lower Upper
 75 100
 77 41.6 22.5 41.9

