

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024051.D
 Acq On : 23 Jul 2022 13:08
 Operator : SY/VA
 Sample : N3790-20
 Misc : 6.31g/10mL/MSVOA_W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 24 00:42:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 06:00:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	255410	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	249093	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	109062	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	106183	16.277	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.120%
7) Chloroethane-d5	2.873	69	81404	18.706	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.840%
11) 1,1-Dichloroethene-d2	4.007	63	66460	12.511	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.040%
21) 2-Butanone-d5	7.074	46	54010	53.378	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.760%
24) Chloroform-d	7.647	84	159611	21.464	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.840%
26) 1,2-Dichloroethane-d4	8.305	65	97638	21.468	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.880%
32) Benzene-d6	8.275	84	271037	20.932	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.720%
36) 1,2-Dichloropropane-d6	9.268	67	92271	23.657	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.640%
41) Toluene-d8	10.323	98	244810	18.639	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.560%
43) trans-1,3-Dichloroprop...	10.579	79	32320	17.678	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.720%
47) 2-Hexanone-d5	10.927	63	39764	48.483	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.960%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	106936	24.809	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.240%
66) 1,2-Dichlorobenzene-d4	13.847	152	96146	24.695	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.800%
Target Compounds						
39) cis-1,3-Dichloropropene	10.024	75	2695	0.504	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024051.D
Acq On : 23 Jul 2022 13:08
Operator : SY/VA
Sample : N3790-20
Misc : 6.31g/10mL/MSVOA_W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jul 24 00:42:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 06:00:17 2022
Response via : Initial Calibration

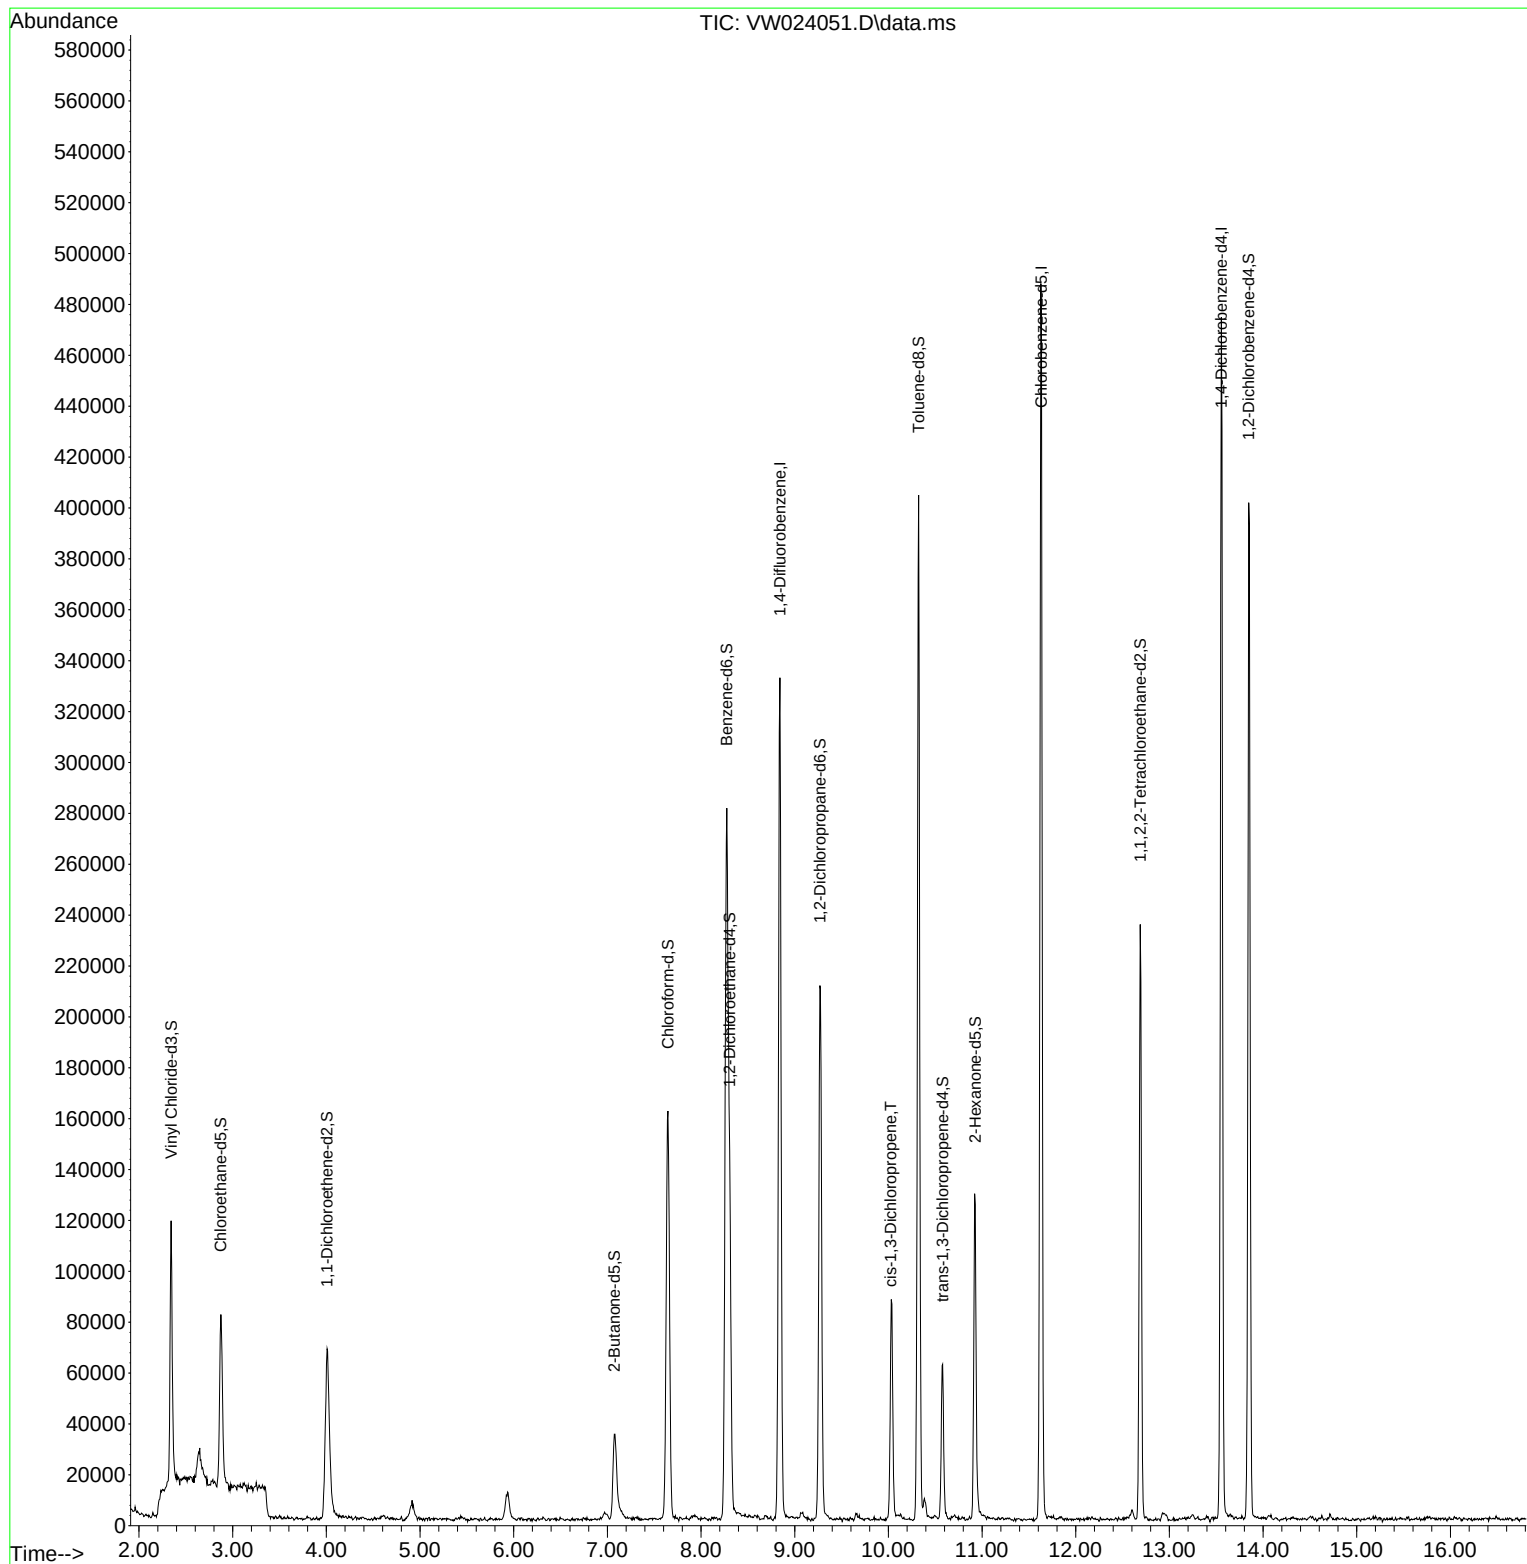

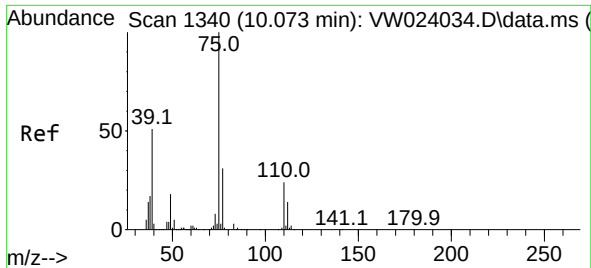

#39
 cis-1,3-Dichloropropene
 Concen: 0.504 ug/L
 RT: 10.024 min Scan# 11
 Delta R.T. -0.049 min
 Lab File: VW024051.D
 Acq: 23 Jul 2022 13:08

Instrument :
 MSVOA_W
 ClientSampleId :

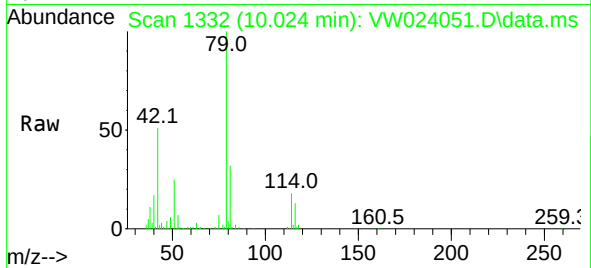

Tgt Ion: 75 Resp: 2695
 Ion Ratio Lower Upper
 75 100
 77 30.9 22.5 41.9

