

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024054.D
 Acq On : 23 Jul 2022 14:22
 Operator : SY/VA
 Sample : N3790-19
 Misc : 6.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 24 00:42:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 06:00:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	201088	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	209502	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	90165	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	92227	17.957	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.840%
7) Chloroethane-d5	2.873	69	72060	21.031	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.120%
11) 1,1-Dichloroethene-d2	4.013	63	55770	13.335	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.360%
21) 2-Butanone-d5	7.080	46	44328	55.644	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.280%
24) Chloroform-d	7.647	84	140081	23.927	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.720%
26) 1,2-Dichloroethane-d4	8.305	65	83820	23.409	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.640%
32) Benzene-d6	8.269	84	240517	22.085	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.320%
36) 1,2-Dichloropropane-d6	9.274	67	78602	23.961	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.840%
41) Toluene-d8	10.323	98	216700	19.617	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.480%
43) trans-1,3-Dichloroprop...	10.573	79	29577	19.235	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.920%
47) 2-Hexanone-d5	10.920	63	34835	50.499	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.000%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	85905	23.696	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.800%
66) 1,2-Dichlorobenzene-d4	13.853	152	83564	25.962	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.840%
Target Compounds					Qvalue	
13) Acetone	4.129	43	2885	5.122	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024054.D
Acq On : 23 Jul 2022 14:22
Operator : SY/VA
Sample : N3790-19
Misc : 6.02g/10mL/MSVOA_W/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jul 24 00:42:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 06:00:17 2022
Response via : Initial Calibration

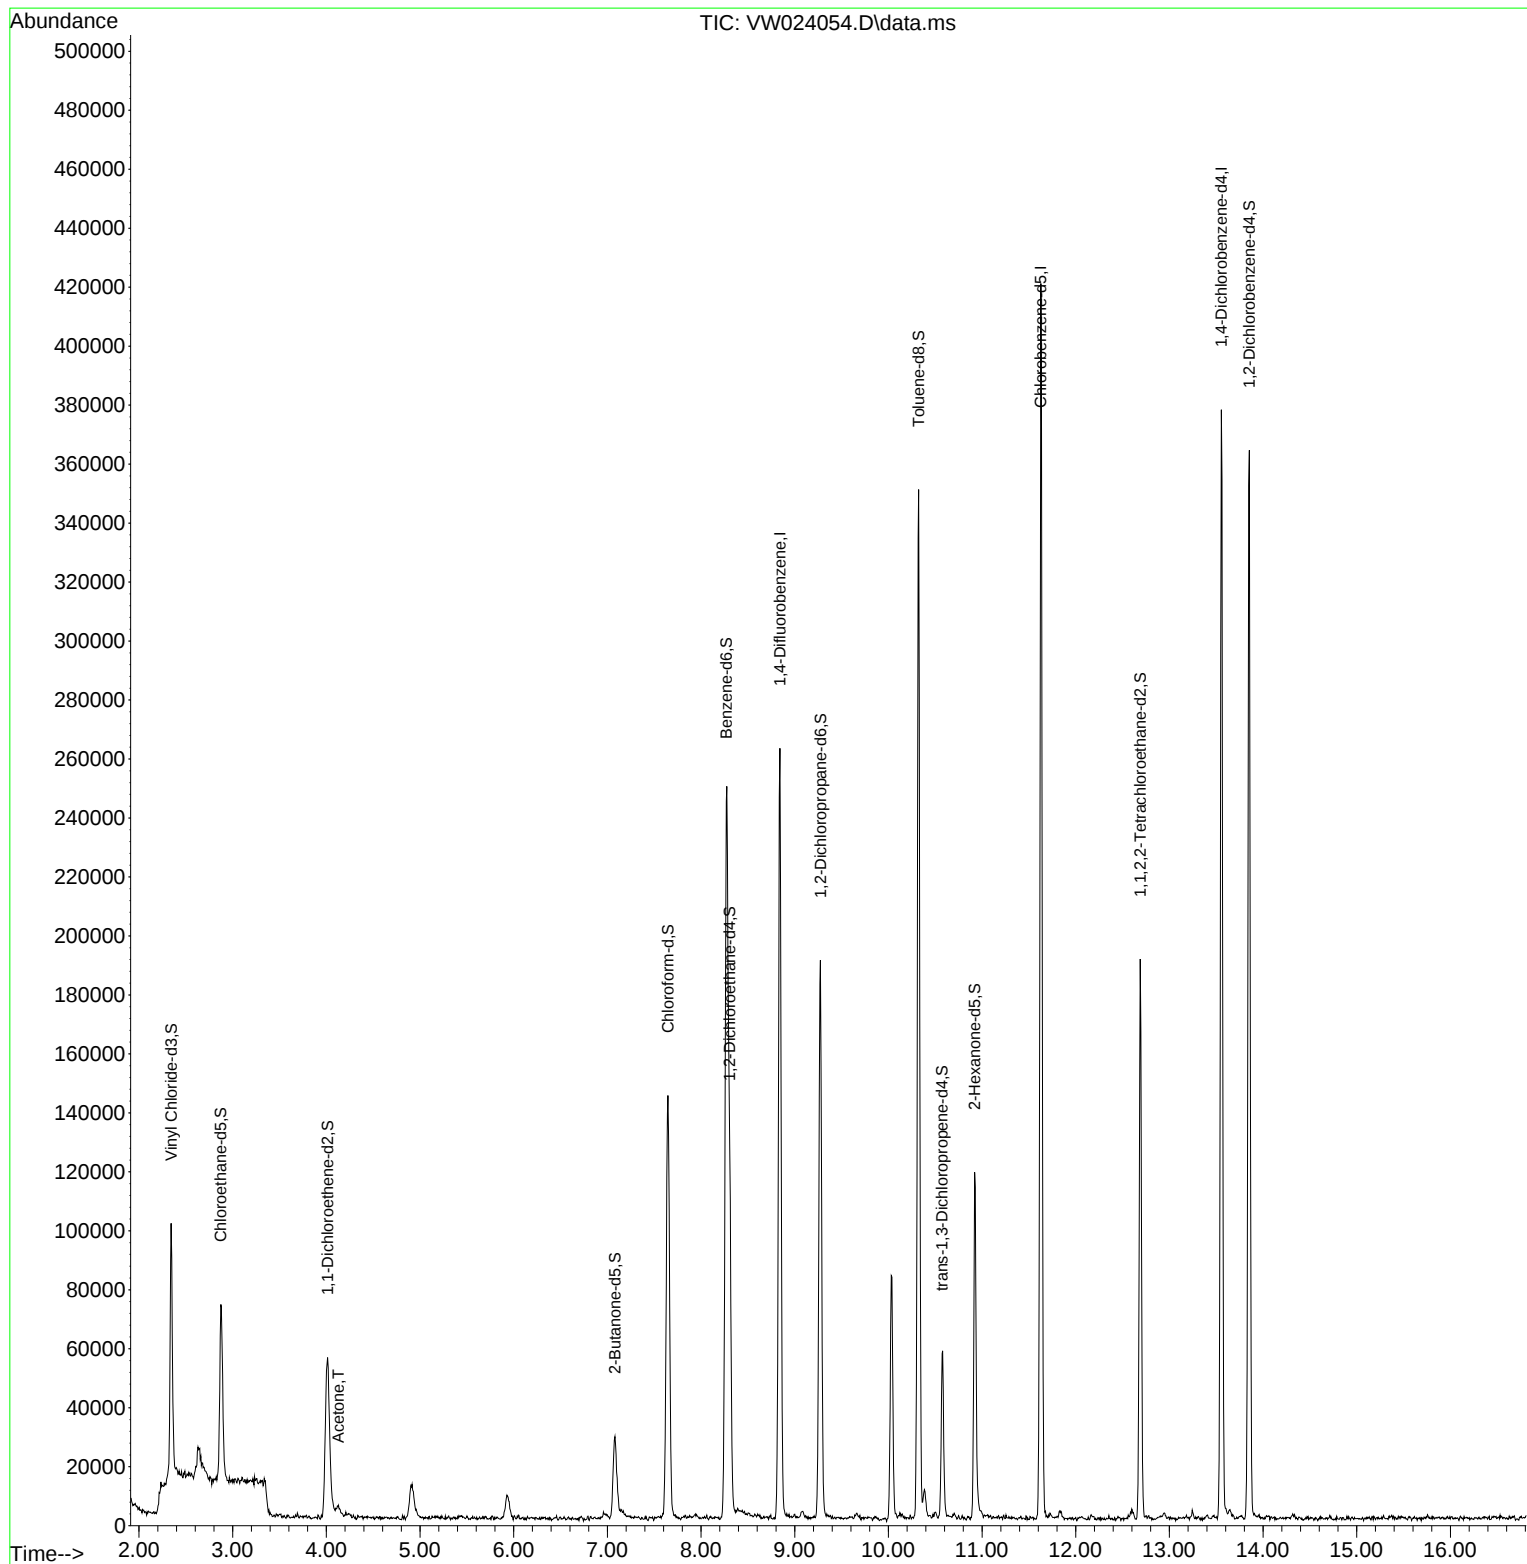

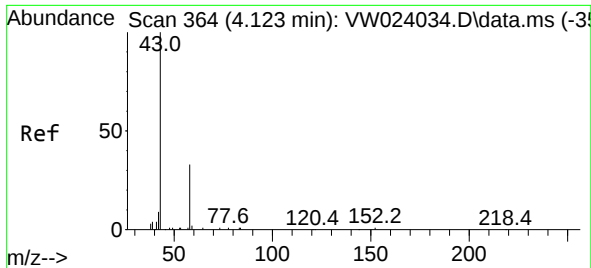

#13
 Acetone
 Concen: 5.122 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW024054.D
 Acq: 23 Jul 2022 14:22

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 43 Resp: 2885
 Ion Ratio Lower Upper
 43 100
 58 42.6 0.0 64.2

