




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW023998.D
 Acq On : 22 Jul 2022 11:29
 Operator : SY/VA
 Sample : N3738-03RE
 Misc : 5.49g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZC5RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 23:11:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 23:08:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/24/2022
 Supervised By :Mahesh Dadoda 07/24/2022

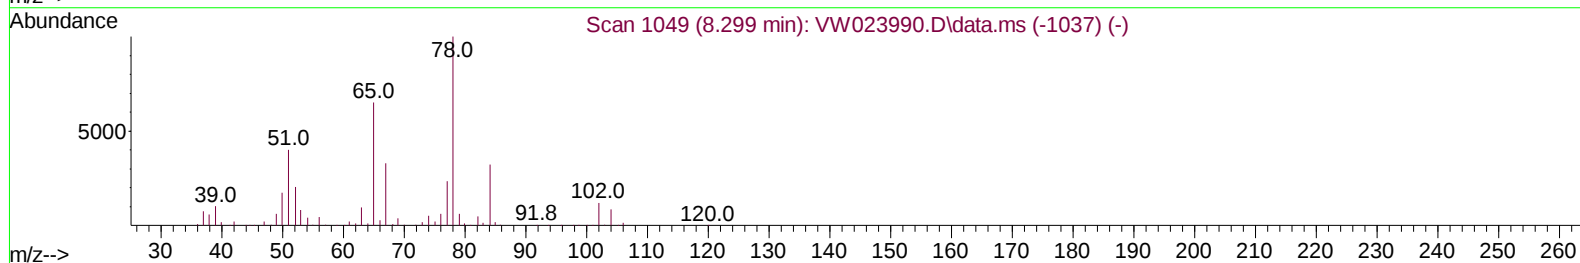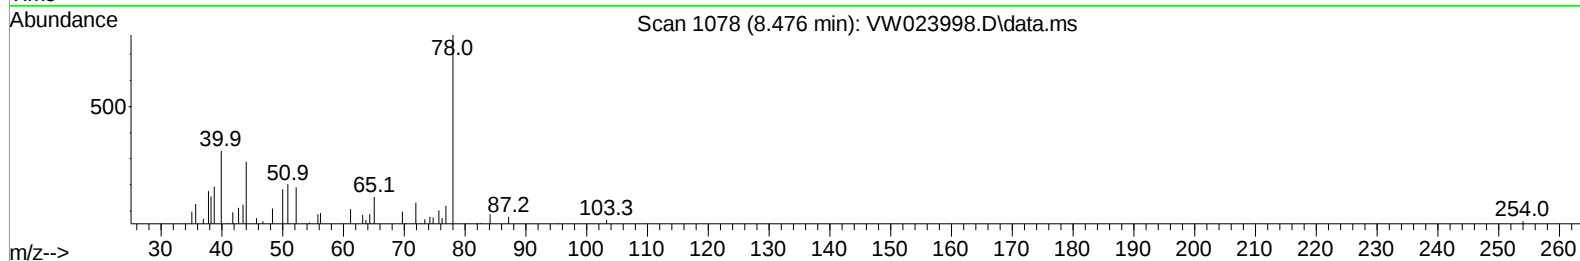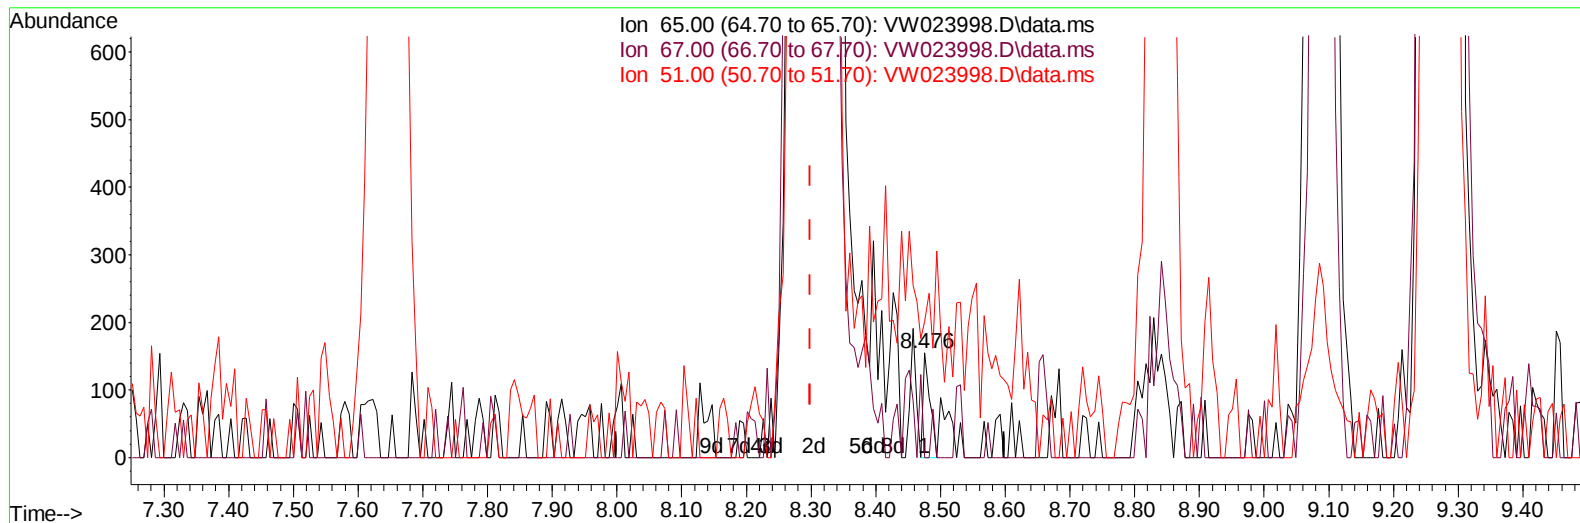

TIC: VW023998.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.476min (+ 0.177) 0.03 ug/L

response 111

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	40.54
51.00	92.20	73.87
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW023998.D
Acq On : 22 Jul 2022 11:29
Operator : SY/VA
Sample : N3738-03RE
Misc : 5.49g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZC5RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 23:11:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 22 23:08:43 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/24/2022
Supervised By :Mahesh Dadoda 07/24/2022

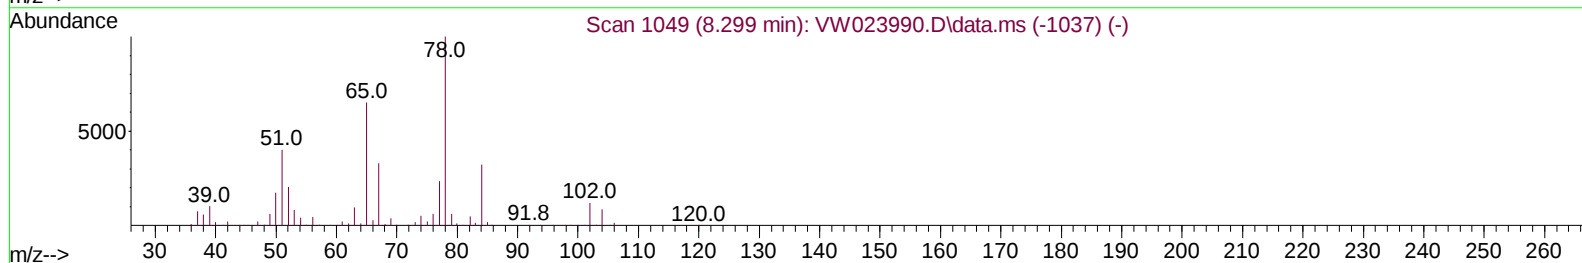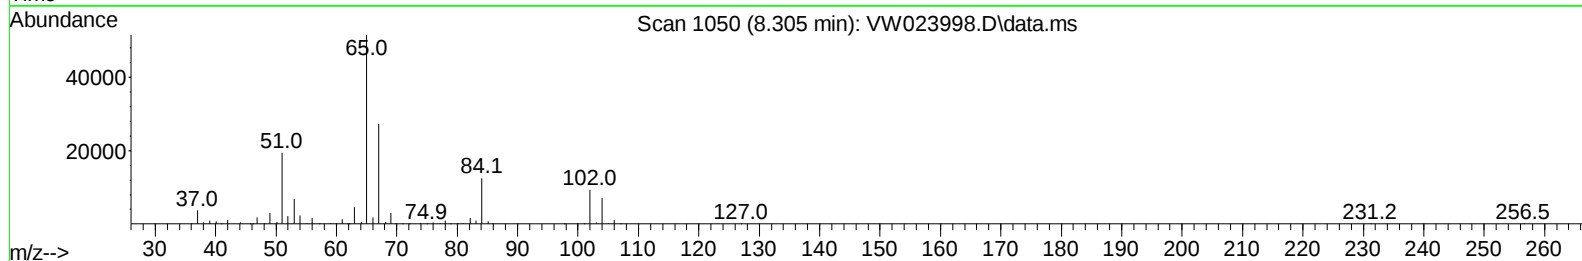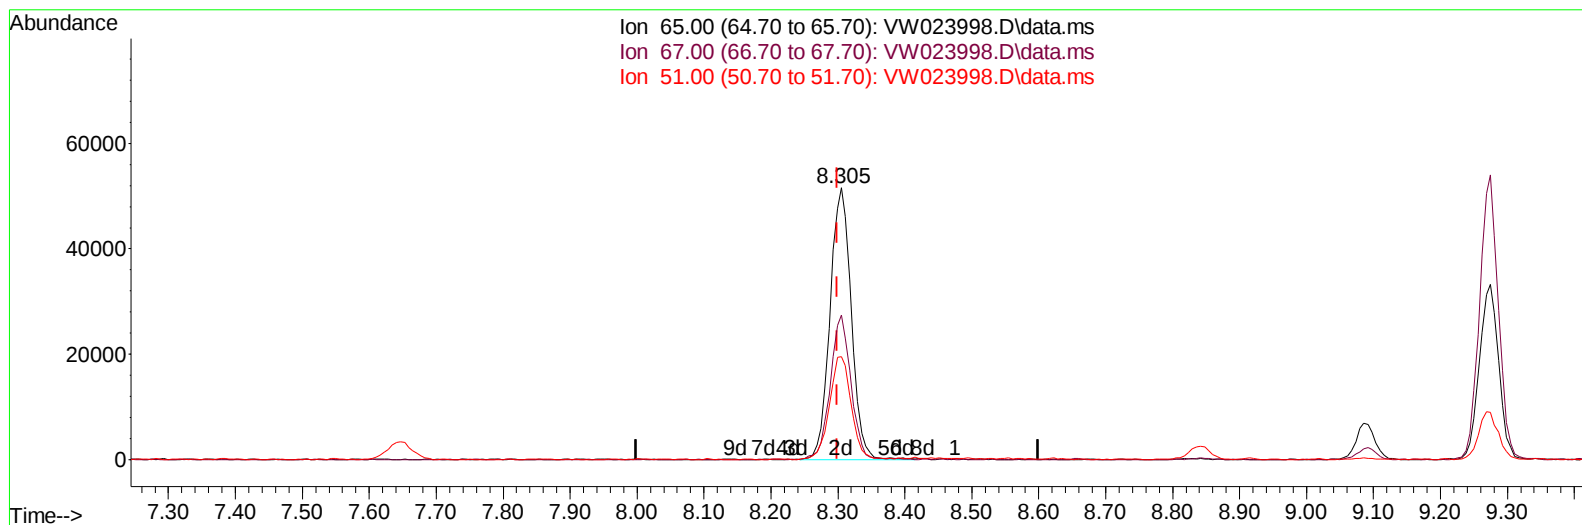

TIC: VW023998.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.006) 26.43 ug/L m

response 113572

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.04#
51.00	92.20	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW023998.D
 Acq On : 22 Jul 2022 11:29
 Operator : SY/VA
 Sample : N3738-03RE
 Misc : 5.49g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZC5RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 23:11:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 23:08:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/24/2022
 Supervised By :Mahesh Dadoda 07/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	241340	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	190478	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	53978	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	135534	21.988	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	87.960%	
7) Chloroethane-d5	2.873	69	98796	24.025	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	96.120%	
11) 1,1-Dichloroethene-d2	4.013	63	86232	17.180	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	68.720%	
21) 2-Butanone-d5	7.080	46	53294	55.741	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	111.480%	
24) Chloroform-d	7.641	84	180969	25.755	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	103.040%	
26) 1,2-Dichloroethane-d4	8.305	65	113572m	26.428	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	105.720%	
32) Benzene-d6	8.269	84	318486	32.165	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	128.640%	
36) 1,2-Dichloropropane-d6	9.274	67	105374	35.330	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	141.320%#	
41) Toluene-d8	10.323	98	255028	25.392	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	101.560%	
43) trans-1,3-Dichloroprop...	10.579	79	29616	21.184	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	84.720%	
47) 2-Hexanone-d5	10.921	63	49053	78.213	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	156.420%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	115155	34.937	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	139.760%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	58954	30.595	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	122.400%#	
Target Compounds						
						Qvalue
16) Methylene chloride	4.903	84	28734	7.614	ug/L	95
17) trans-1,2-Dichloroethene	5.428	96	2810	0.905	ug/L	85
20) cis-1,2-Dichloroethene	7.165	96	52844	15.367	ug/L #	94
34) Trichloroethene	9.092	95	851891	298.035	ug/L	90
46) Tetrachloroethene	10.860	164	173553	78.525	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW023998.D
Acq On : 22 Jul 2022 11:29
Operator : SY/VA
Sample : N3738-03RE
Misc : 5.49g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZC5RE

Manual IntegrationsAPPROVED

Quant Time: Jul 22 23:11:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 22 23:08:43 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/24/2022
Supervised By :Mahesh Dadoda 07/24/2022

