




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024021.D
 Acq On : 22 Jul 2022 22:10
 Operator : SY/VA
 Sample : N3741-07RE
 Misc : 5.13g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B15RE

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:41:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/23/2022
 Supervised By :Mahesh Dadoda 07/24/2022

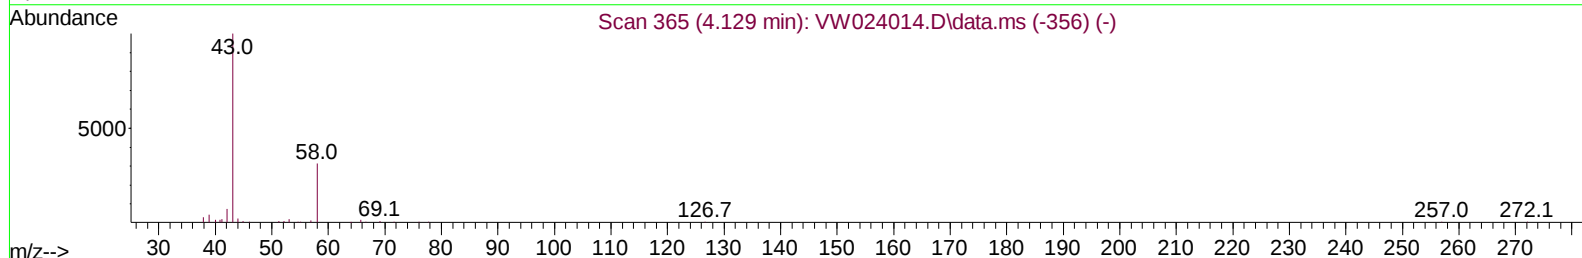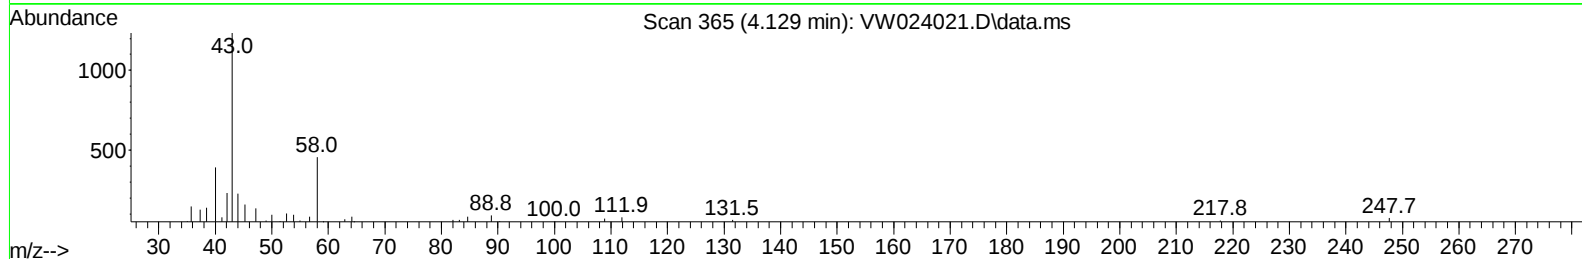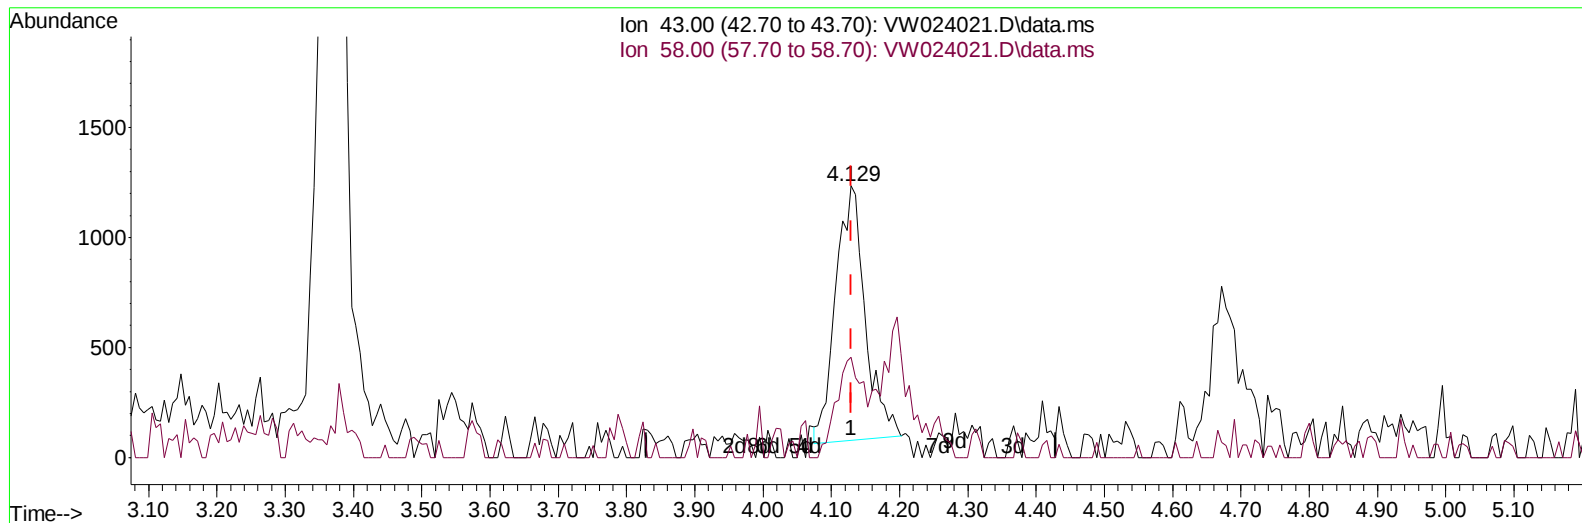

TIC: VW024021.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 8.61 ug/L

response 3491

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	29.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024021.D
 Acq On : 22 Jul 2022 22:10
 Operator : SY/VA
 Sample : N3741-07RE
 Misc : 5.13g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B15RE

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:41:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/23/2022
 Supervised By :Mahesh Dadoda 07/24/2022

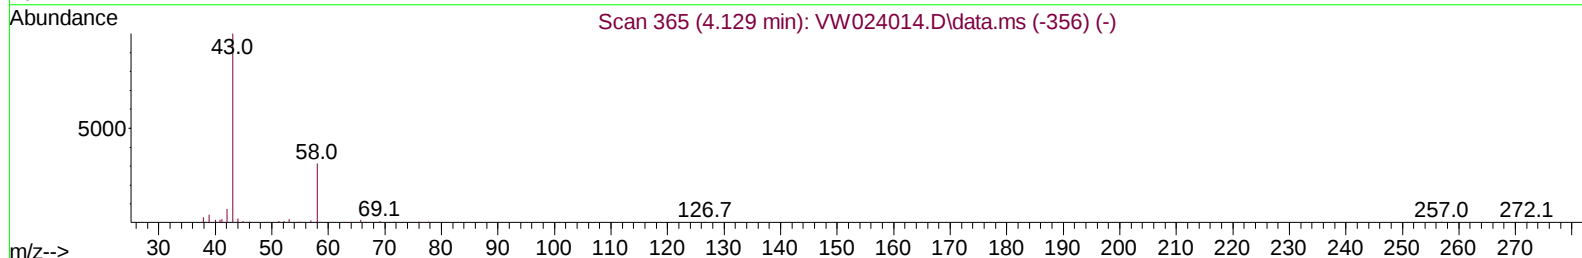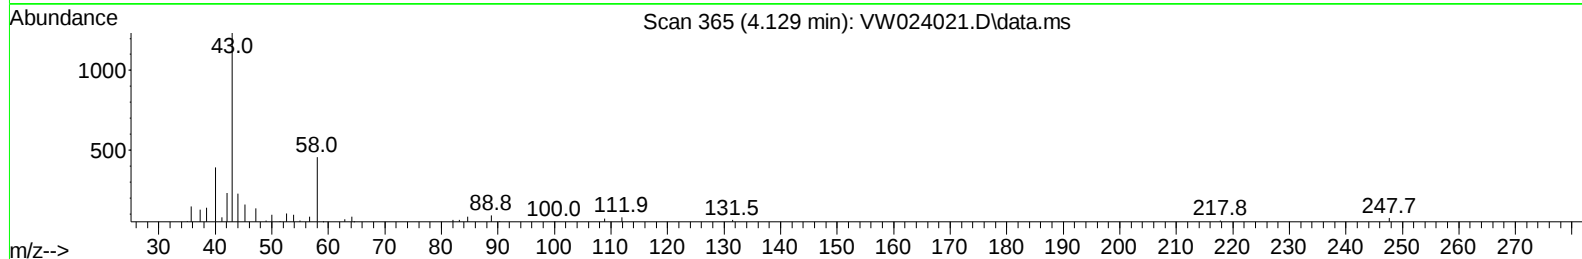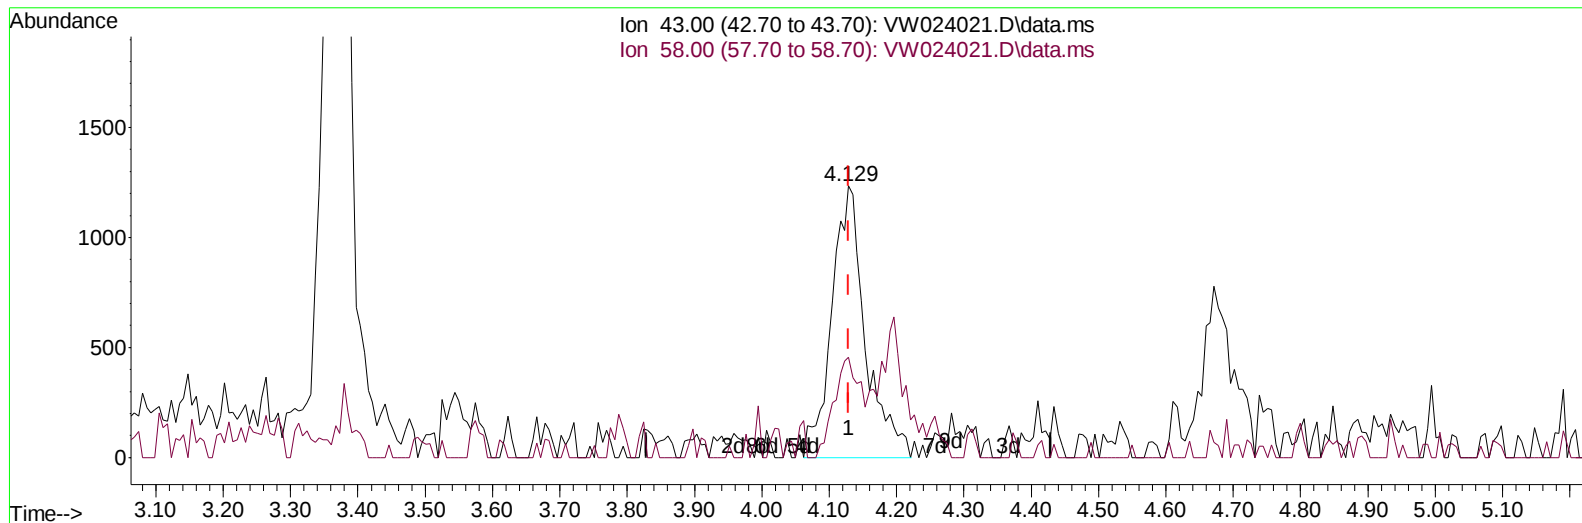

TIC: VW024021.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 10.55 ug/L m

response 4280

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	23.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024021.D
 Acq On : 22 Jul 2022 22:10
 Operator : SY/VA
 Sample : N3741-07RE
 Misc : 5.13g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0B15RE

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:41:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/23/2022
 Supervised By :Mahesh Dadoda 07/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	144781	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	123433	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	35490	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	45432	12.286	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	49.160%		
7) Chloroethane-d5	2.873	69	37866	15.350	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	61.400%		
11) 1,1-Dichloroethene-d2	4.001	63	28768	9.554	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery =	38.200%#		
21) 2-Butanone-d5	7.086	46	6922	12.068	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	24.140%		
24) Chloroform-d	7.647	84	104367	24.759	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	99.040%		
26) 1,2-Dichloroethane-d4	8.305	65	79563	30.861	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	123.440%		
32) Benzene-d6	8.275	84	152715	23.801	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	95.200%		
36) 1,2-Dichloropropane-d6	9.274	67	69775	36.101	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	144.400%#		
41) Toluene-d8	10.323	98	114200	17.547	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	70.200%		
43) trans-1,3-Dichloroprop...	10.579	79	9229	10.187	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	40.760%		
47) 2-Hexanone-d5	10.927	63	3655	8.993	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	17.980%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	67345	31.530	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	126.120%#		
66) 1,2-Dichlorobenzene-d4	13.853	152	35460	27.989	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	111.960%		
Target Compounds						
13) Acetone	4.129	43	4280m	10.554	ug/L	
16) Methylene chloride	4.909	84	18809	8.308	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024021.D
Acq On : 22 Jul 2022 22:10
Operator : SY/VA
Sample : N3741-07RE
Misc : 5.13g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
H0B15RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/23/2022
Supervised By :Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 04:41:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 03:31:10 2022
Response via : Initial Calibration

