




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024030.D
Acq On : 23 Jul 2022 01:51
Operator : SY/VA
Sample : N3790-12
Misc : 4.82g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/23/2022
Supervised By :Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 04:43:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 03:31:10 2022
Response via : Initial Calibration

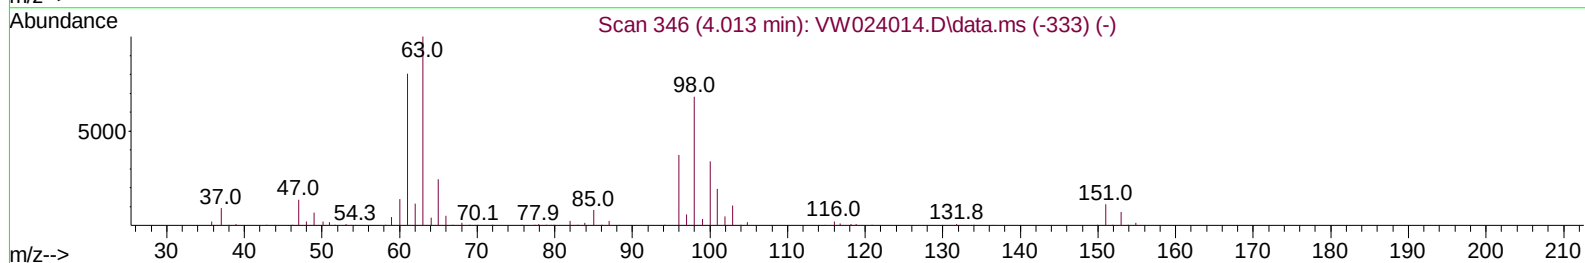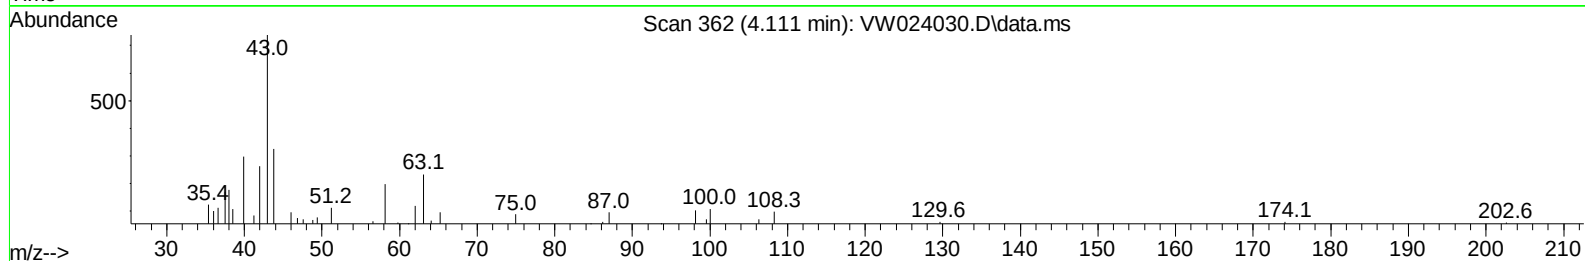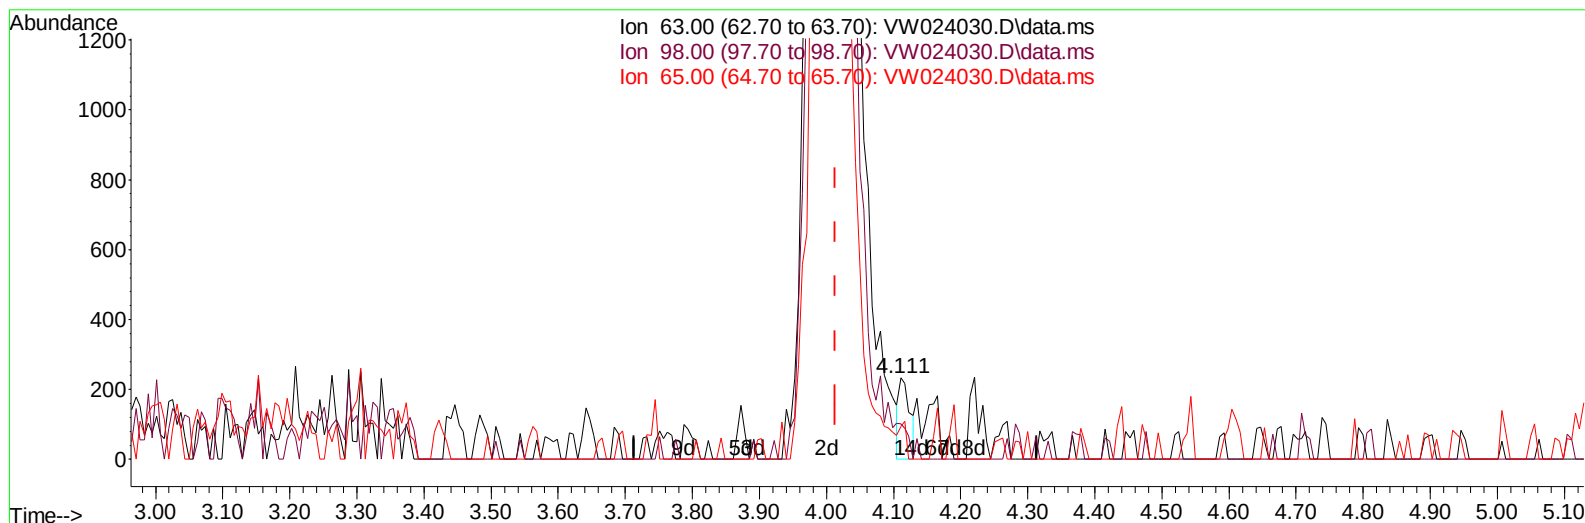

TIC: VW024030.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.111min (+ 0.097) 0.08 ug/L

response 260

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.20	50.77
65.00	24.10	28.46
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024030.D
Acq On : 23 Jul 2022 01:51
Operator : SY/VA
Sample : N3790-12
Misc : 4.82g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/23/2022
Supervised By :Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 04:43:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 03:31:10 2022
Response via : Initial Calibration

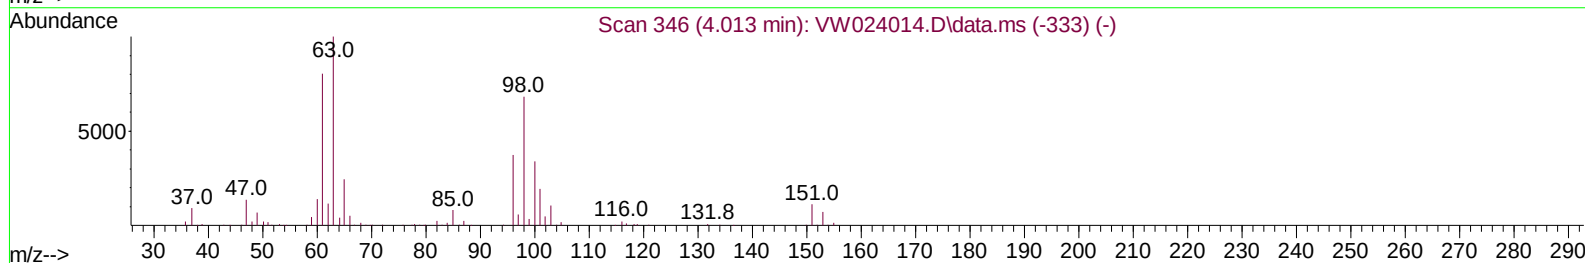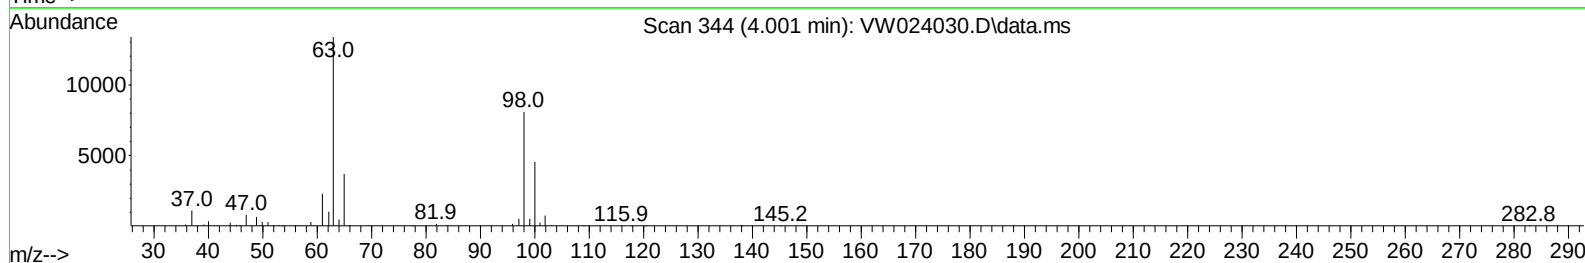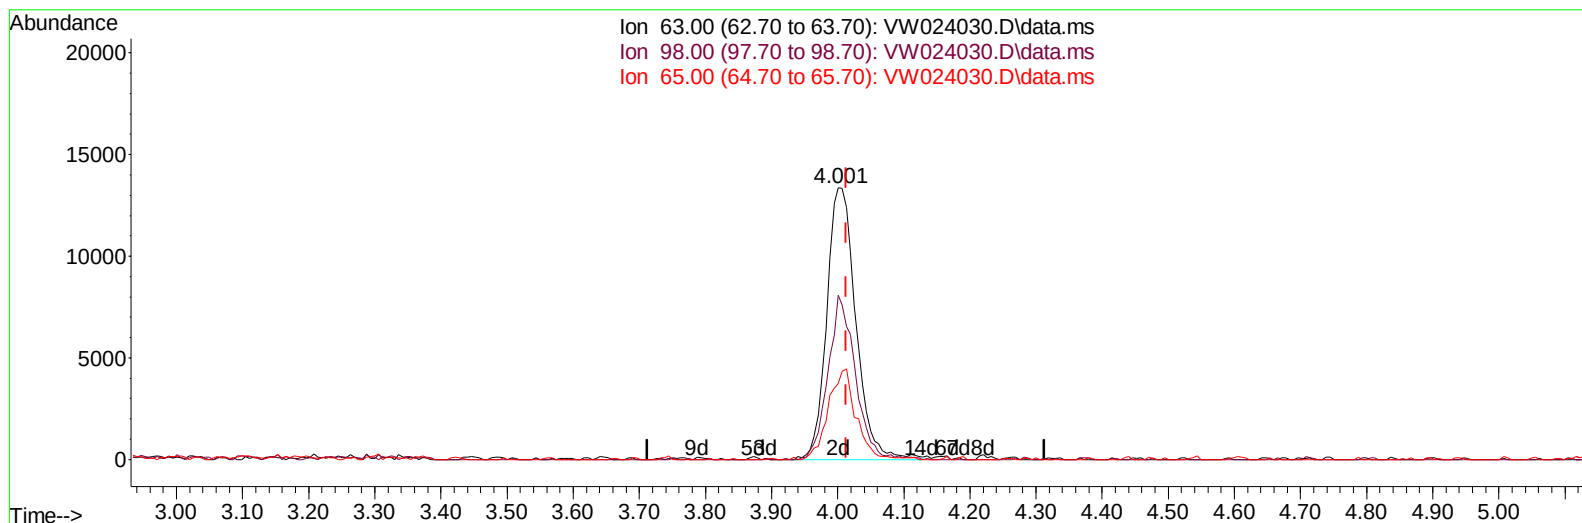

TIC: VW024030.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.001min (-0.012) 11.83 ug/L m

response 40749

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	68.20	0.32#
65.00	24.10	0.18#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024030.D
 Acq On : 23 Jul 2022 01:51
 Operator : SY/VA
 Sample : N3790-12
 Misc : 4.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK6

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:43:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/23/2022
 Supervised By :Mahesh Dadoda 07/24/2022

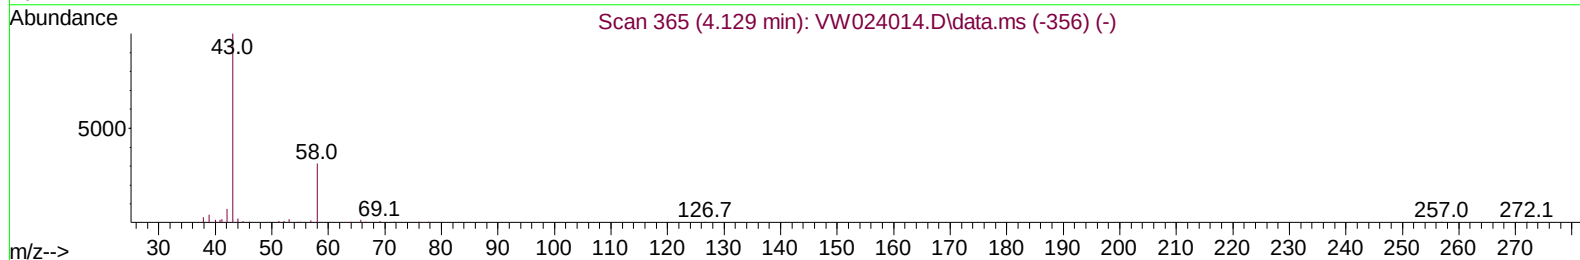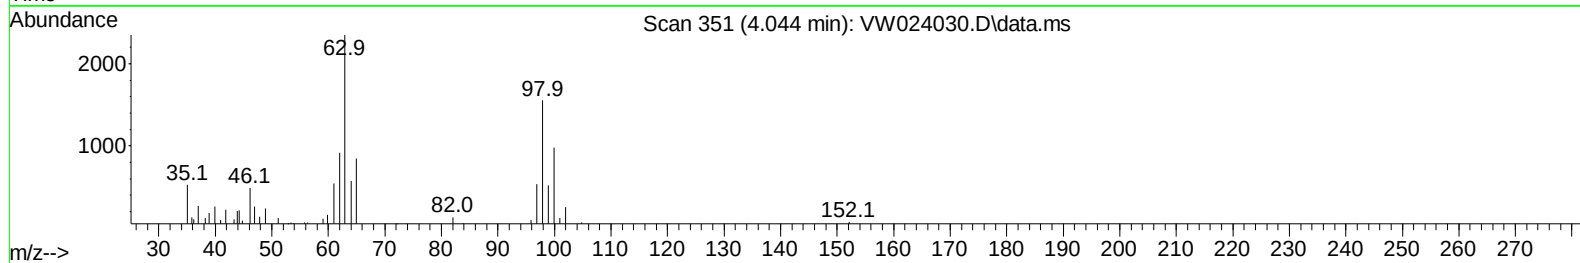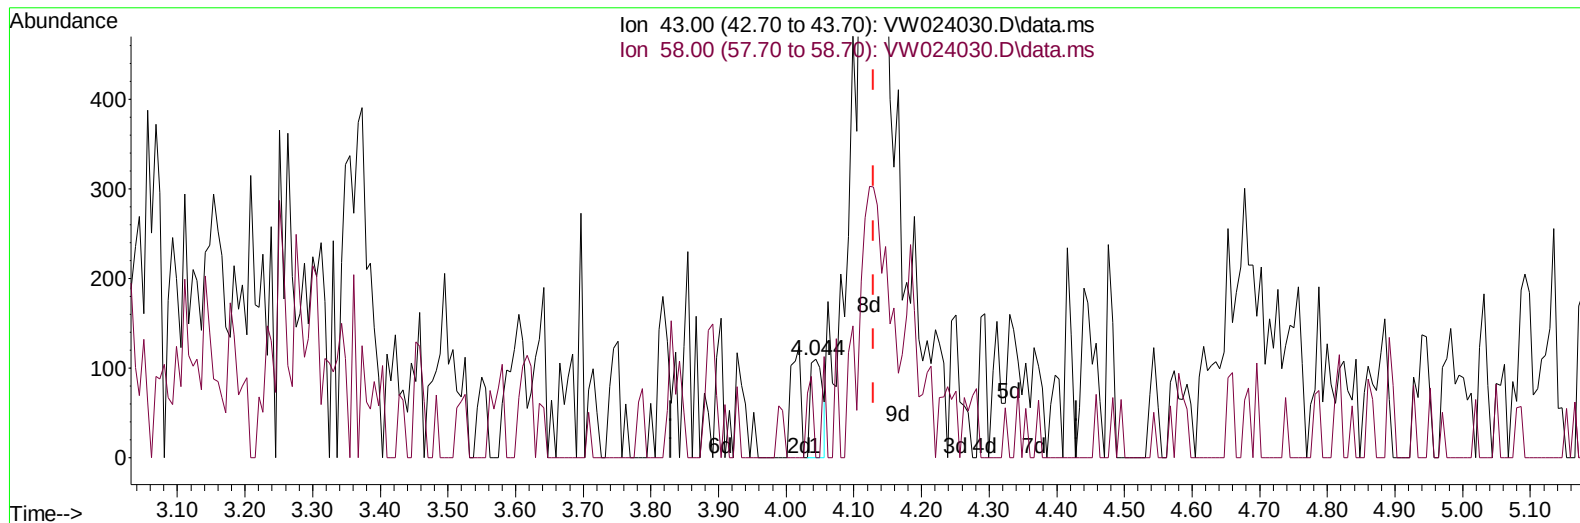

TIC: VW024030.D\data.ms

(13) Acetone (T)

4.044min (-0.086) 0.30 ug/L

response 139

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	43.17
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024030.D
 Acq On : 23 Jul 2022 01:51
 Operator : SY/VA
 Sample : N3790-12
 Misc : 4.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK6

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:43:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/23/2022
 Supervised By :Mahesh Dadoda 07/24/2022

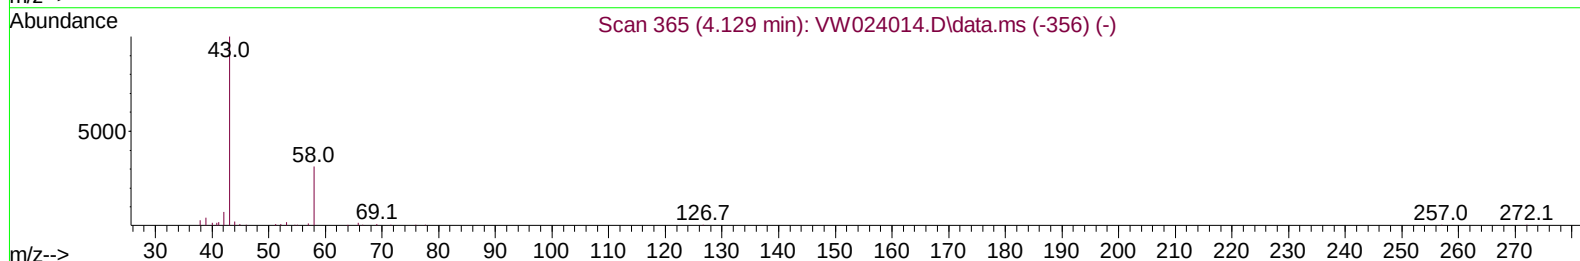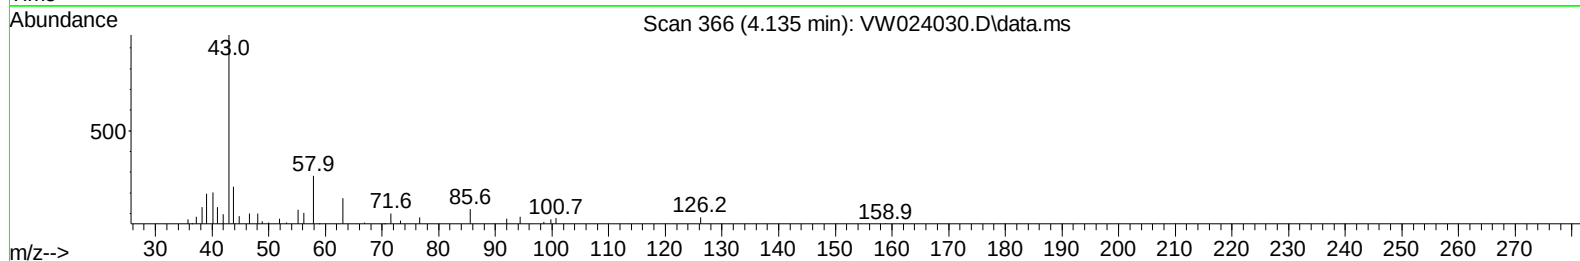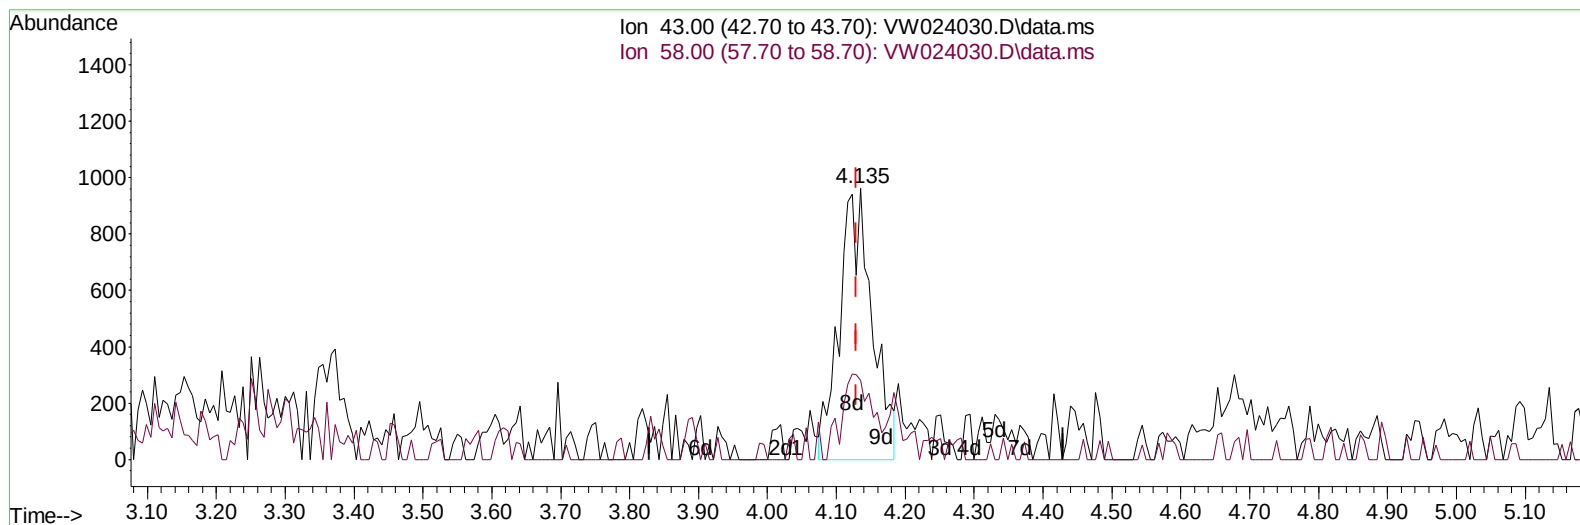

TIC: VW024030.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 6.82 ug/L m

response 3165

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	1.90
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024030.D
Acq On : 23 Jul 2022 01:51
Operator : SY/VA
Sample : N3790-12
Misc : 4.82g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/23/2022
Supervised By :Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 04:43:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 03:31:10 2022
Response via : Initial Calibration

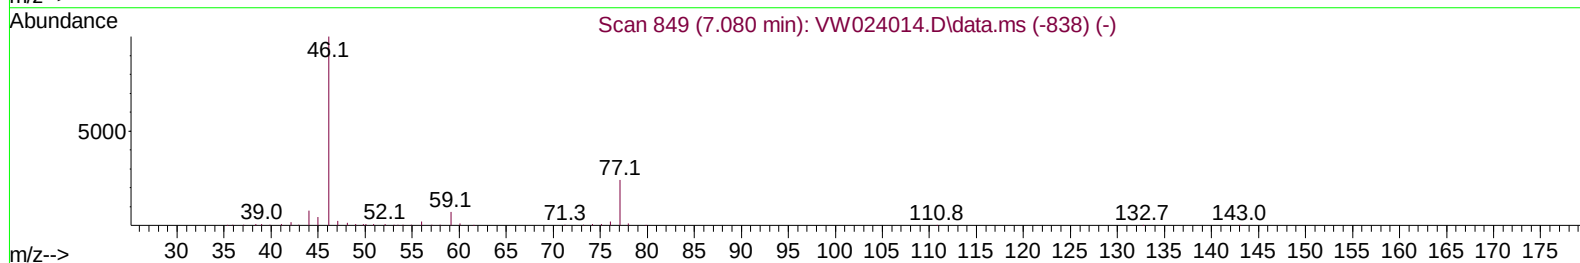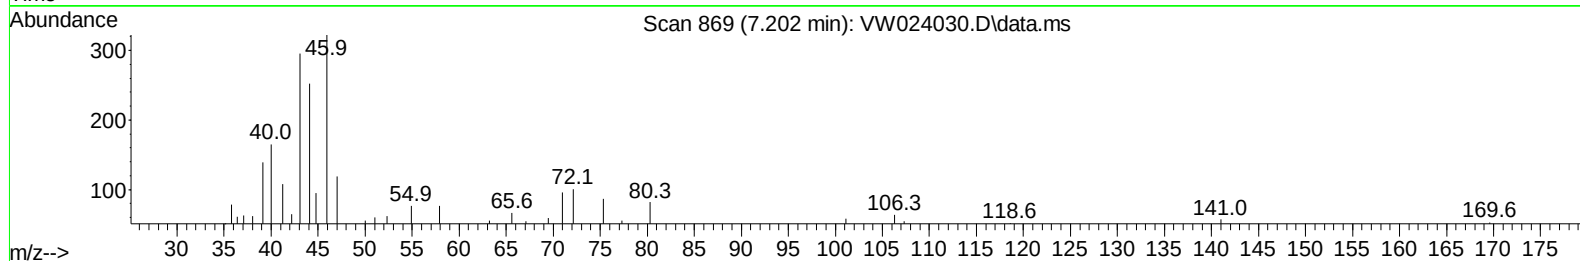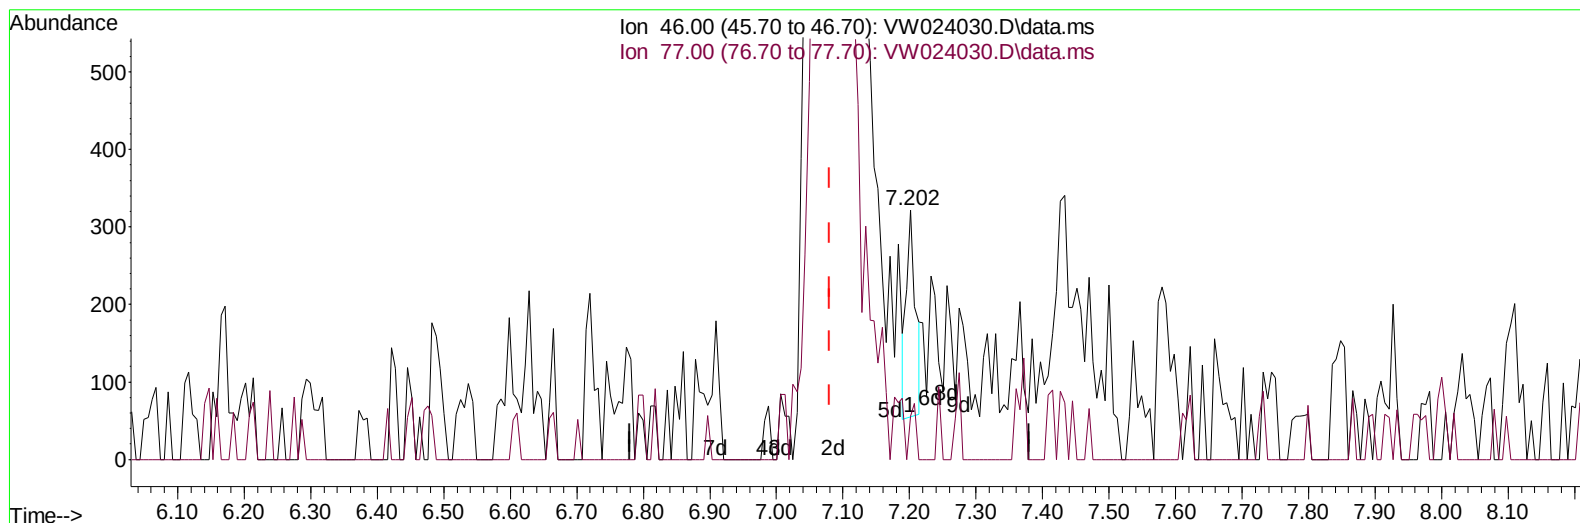

TIC: VW024030.D\data.ms

(21) 2-Butanone-d5 (S)

7.202min (+ 0.122) 0.39 ug/L

response 254

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	18.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024030.D
 Acq On : 23 Jul 2022 01:51
 Operator : SY/VA
 Sample : N3790-12
 Misc : 4.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK6

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:43:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/23/2022
 Supervised By :Mahesh Dadoda 07/24/2022

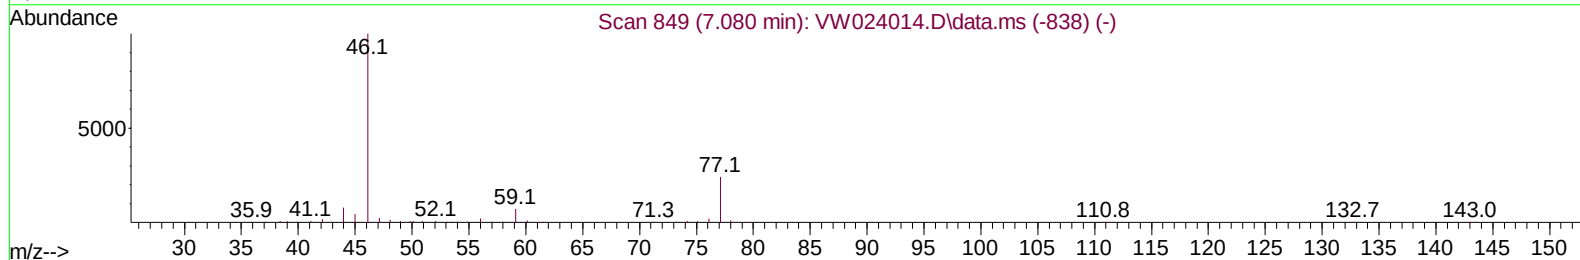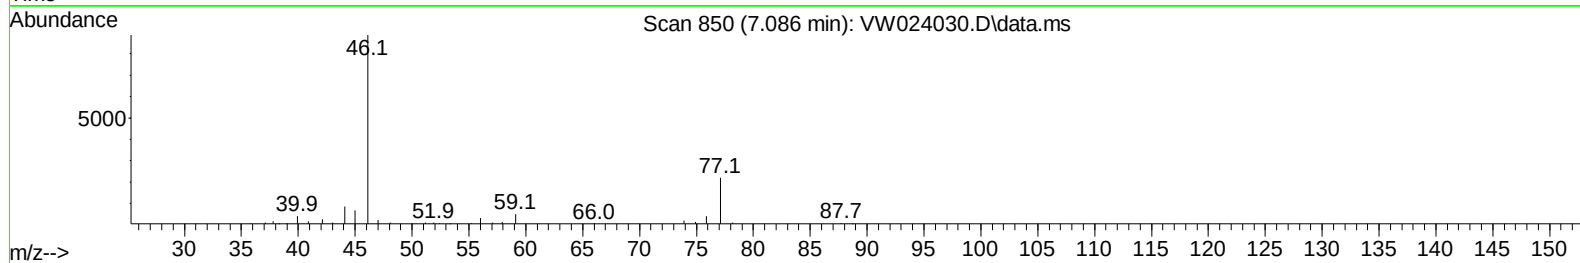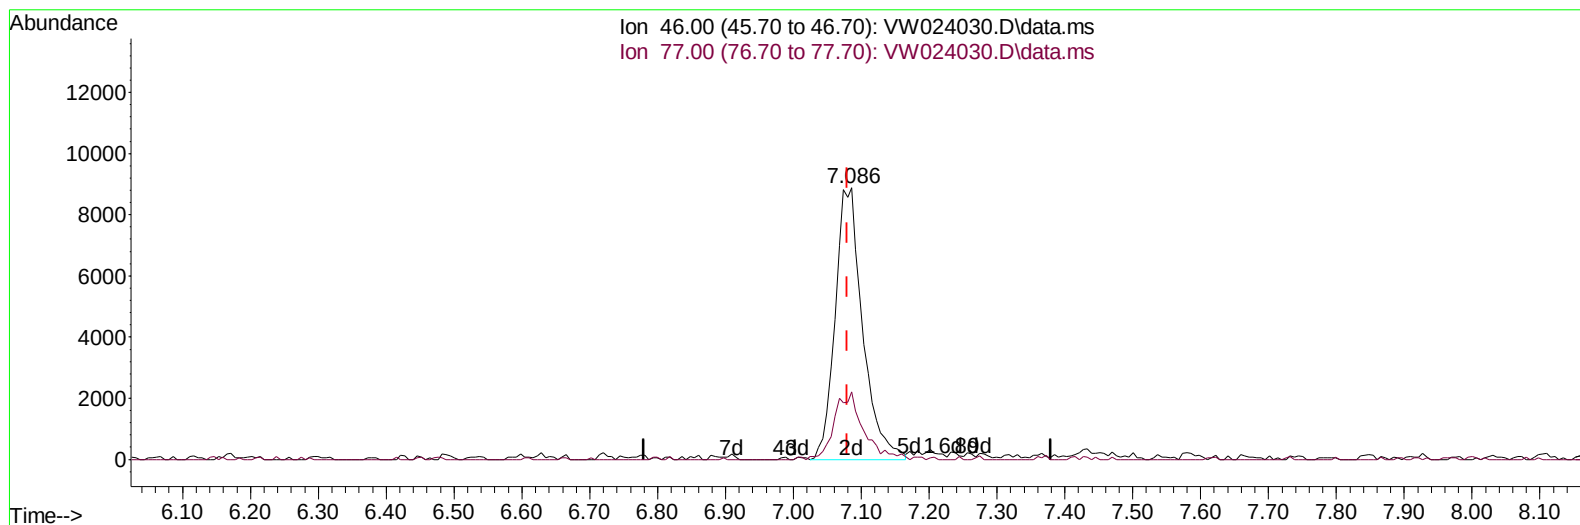

TIC: VW024030.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (+ 0.006) 38.17 ug/L m

response 25053

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	0.19#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024030.D
 Acq On : 23 Jul 2022 01:51
 Operator : SY/VA
 Sample : N3790-12
 Misc : 4.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK6

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:43:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/23/2022
 Supervised By :Mahesh Dadoda 07/24/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	165680	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	134894	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	39310	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	70048	16.554	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	66.200%	
7) Chloroethane-d5	2.873	69	47542	16.841	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.360%	
11) 1,1-Dichloroethene-d2	4.001	63	40749m	11.826	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	47.320%	
21) 2-Butanone-d5	7.086	46	25053m	38.169	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	76.340%	
24) Chloroform-d	7.647	84	120358	24.951	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	99.800%	
26) 1,2-Dichloroethane-d4	8.299	65	76390	25.893	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.560%	
32) Benzene-d6	8.275	84	157793	22.503	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	90.000%	
36) 1,2-Dichloropropane-d6	9.274	67	68489	32.425	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	129.720%#	
41) Toluene-d8	10.323	98	124227	17.466	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	69.880%	
43) trans-1,3-Dichloroprop...	10.579	79	11979	12.099	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	48.400%	
47) 2-Hexanone-d5	10.920	63	8159	18.370	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	36.740%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	67588	28.955	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	115.800%	
66) 1,2-Dichlorobenzene-d4	13.853	152	35875	25.565	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	102.280%	
Target Compounds						
13) Acetone	4.135	43	3165m	6.820	ug/L	
16) Methylene chloride	4.909	84	15146	5.846	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024030.D
Acq On : 23 Jul 2022 01:51
Operator : SY/VA
Sample : N3790-12
Misc : 4.82g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/23/2022
Supervised By :Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 04:43:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 03:31:10 2022
Response via : Initial Calibration

