




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024031.D
 Acq On : 23 Jul 2022 02:16
 Operator : SY/VA
 Sample : N3790-13
 Misc : 2.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/24/2022
 Supervised By :Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 04:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

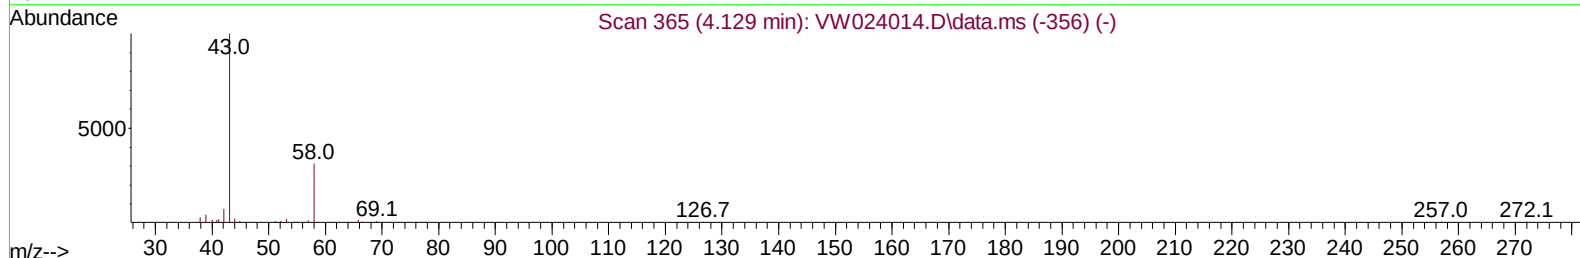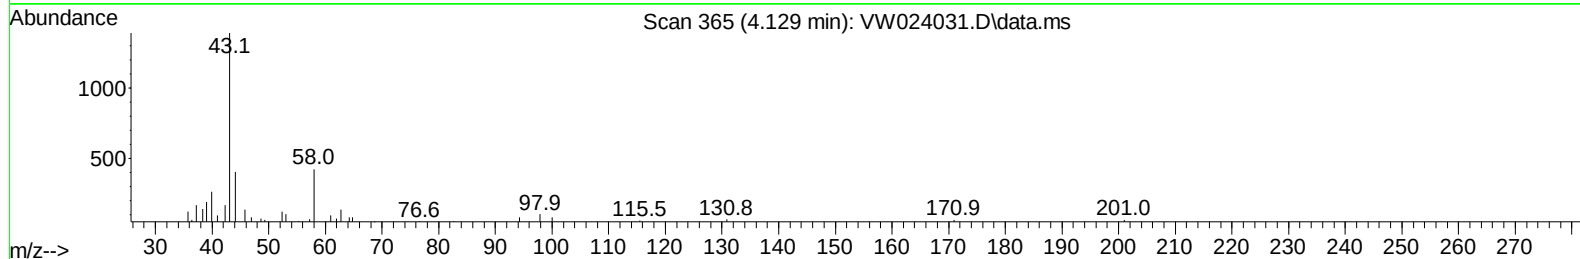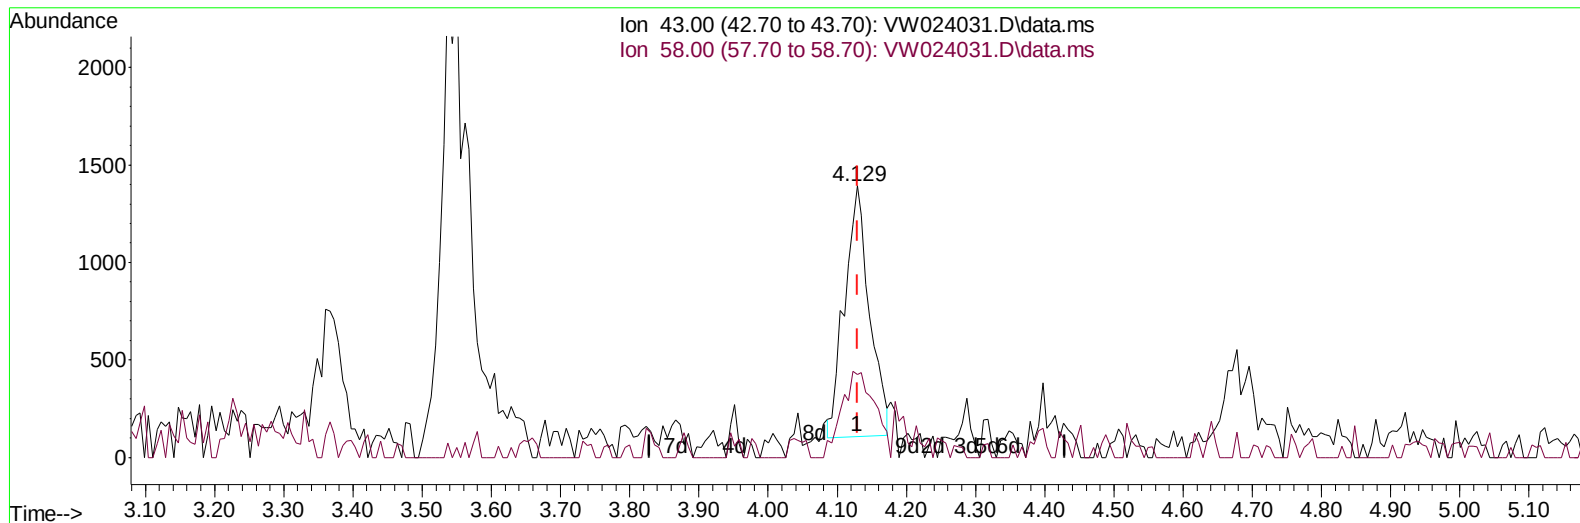

TIC: VW024031.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 7.53 ug/L

response 3192

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	45.39
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024031.D
Acq On : 23 Jul 2022 02:16
Operator : SY/VA
Sample : N3790-13
Misc : 2.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/24/2022
Supervised By :Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 04:43:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 03:31:10 2022
Response via : Initial Calibration

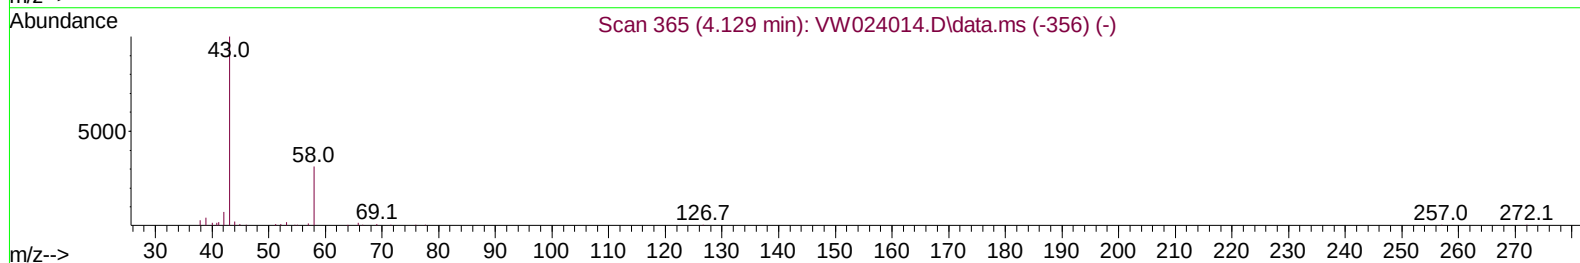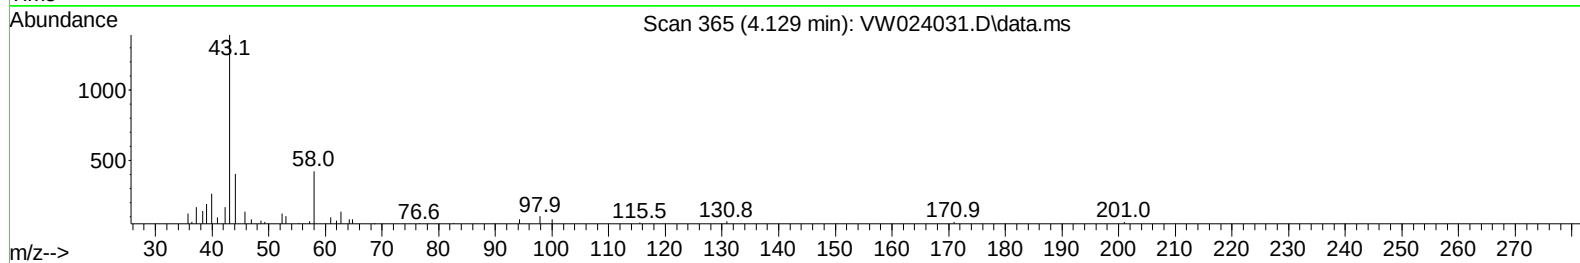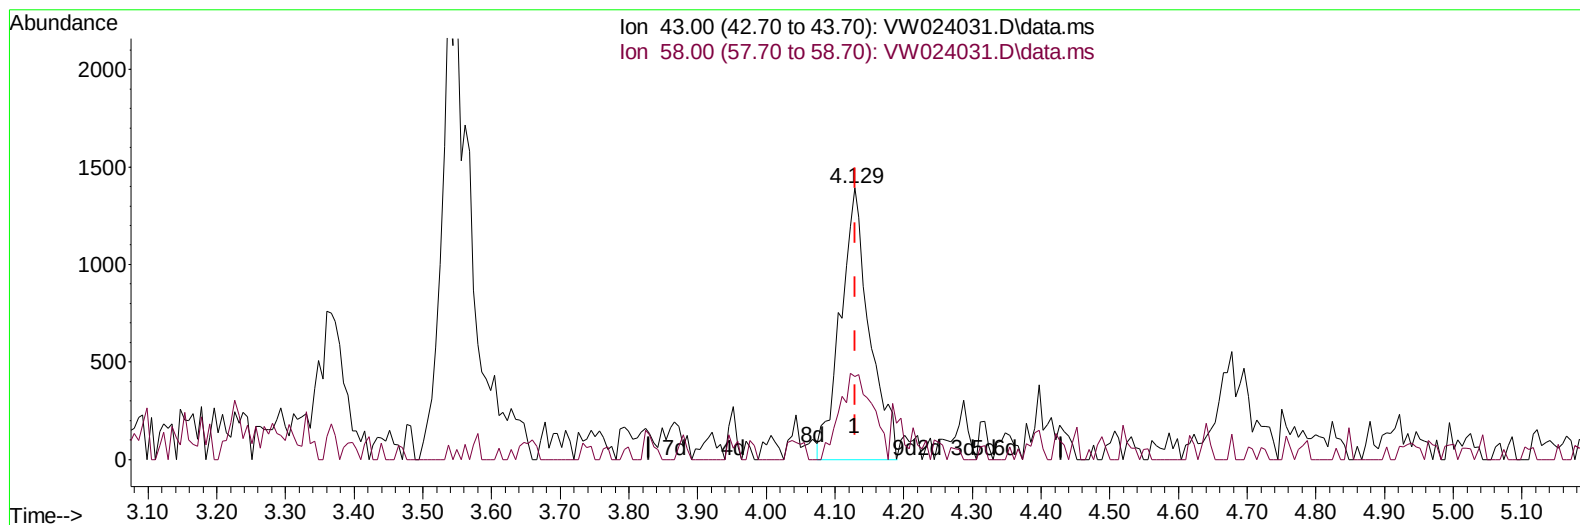

TIC: VW024031.D\data.ms

(13) Acetone (T)

4.129min (-0.000) 9.60 ug/L m

response 4068

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	35.62
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024031.D
Acq On : 23 Jul 2022 02:16
Operator : SY/VA
Sample : N3790-13
Misc : 2.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/24/2022
Supervised By :Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 04:43:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 03:31:10 2022
Response via : Initial Calibration

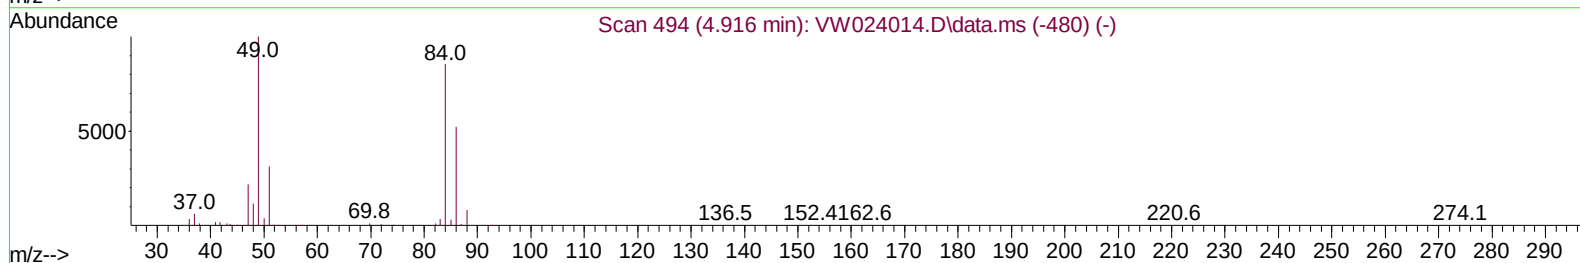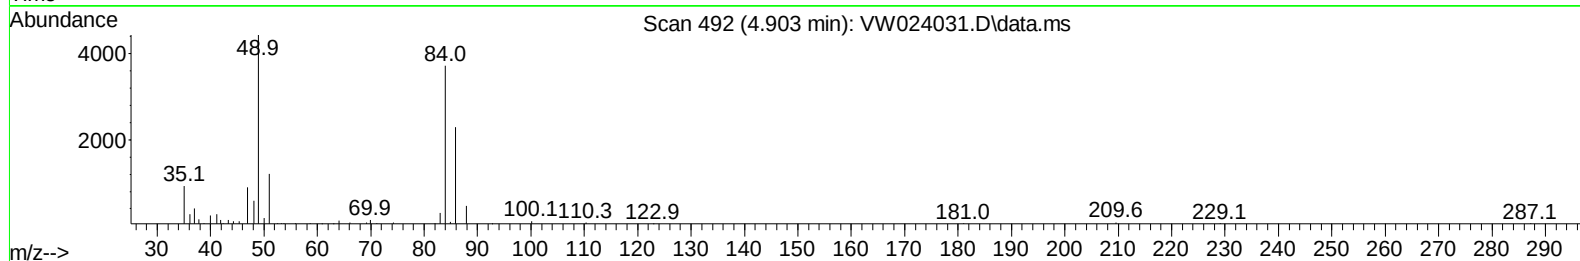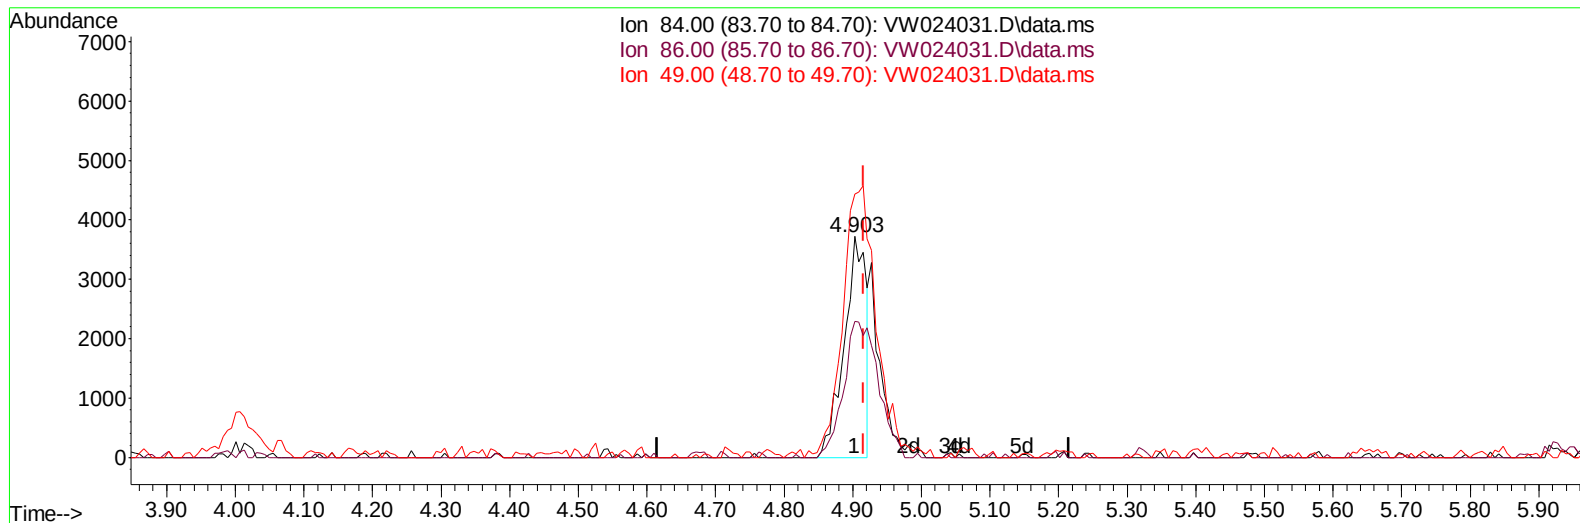

TIC: VW024031.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.013) 3.52 ug/L

response 8324

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	61.71
49.00	122.00	119.14
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024031.D
 Acq On : 23 Jul 2022 02:16
 Operator : SY/VA
 Sample : N3790-13
 Misc : 2.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK7

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/24/2022
 Supervised By :Mahesh Dadoda 07/24/2022

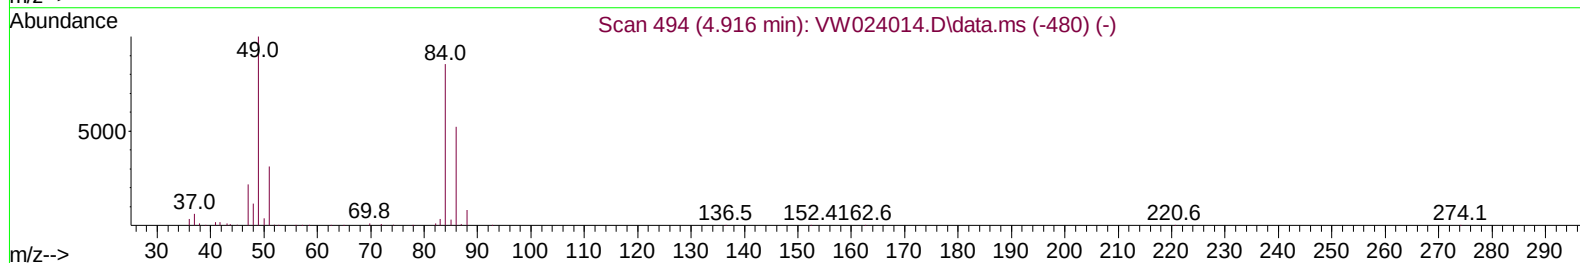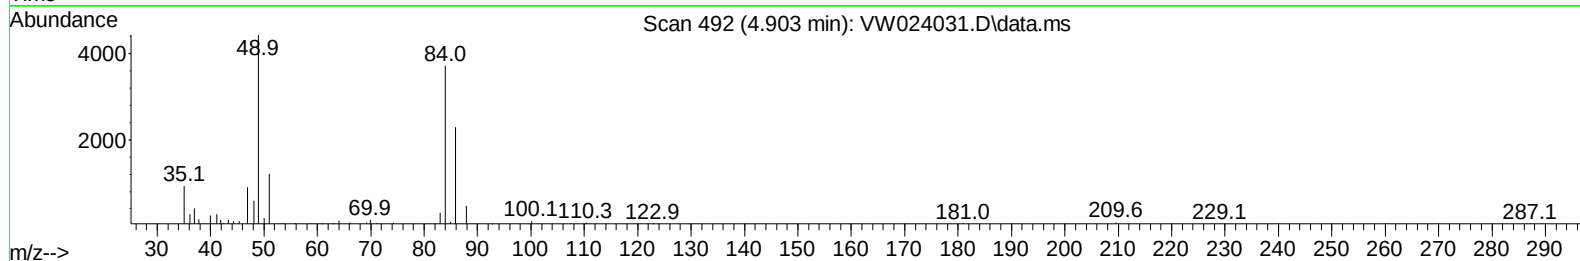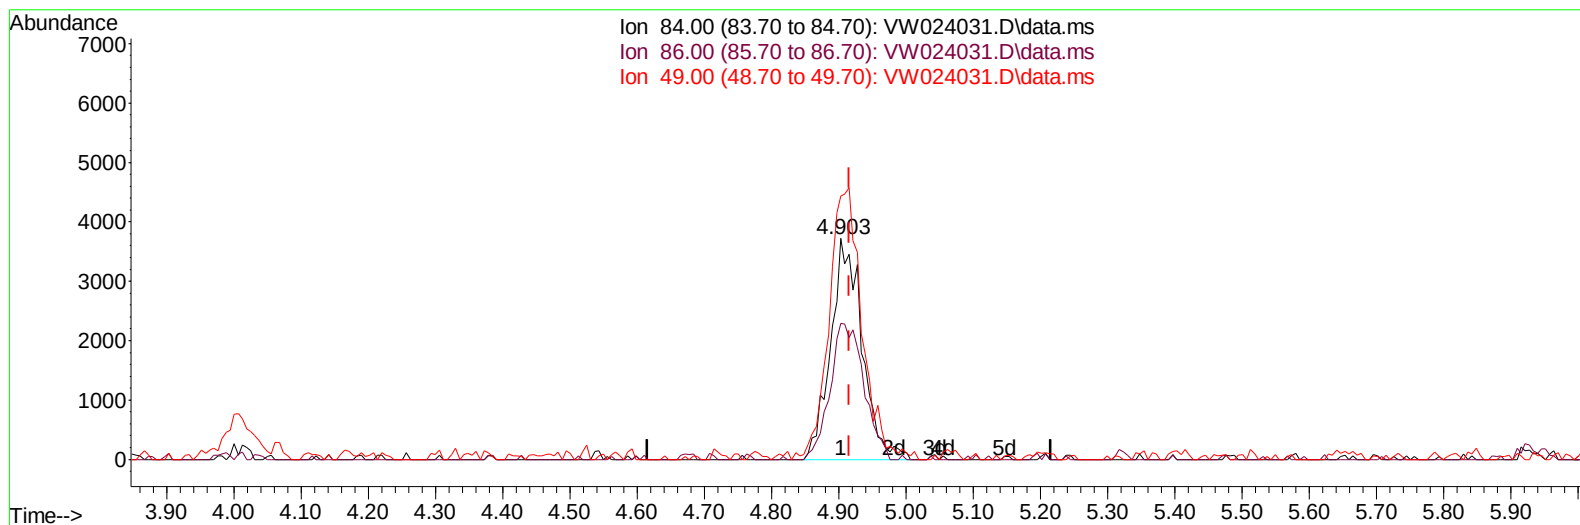

TIC: VW024031.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.013) 5.11 ug/L m

response 12086

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.20	61.71
49.00	122.00	119.14
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024031.D
 Acq On : 23 Jul 2022 02:16
 Operator : SY/VA
 Sample : N3790-13
 Misc : 2.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK7

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/24/2022
 Supervised By :Mahesh Dadoda 07/24/2022

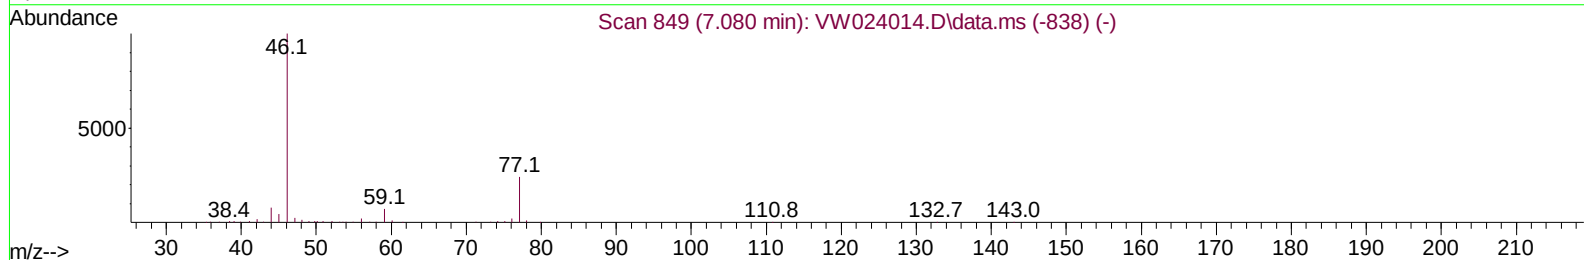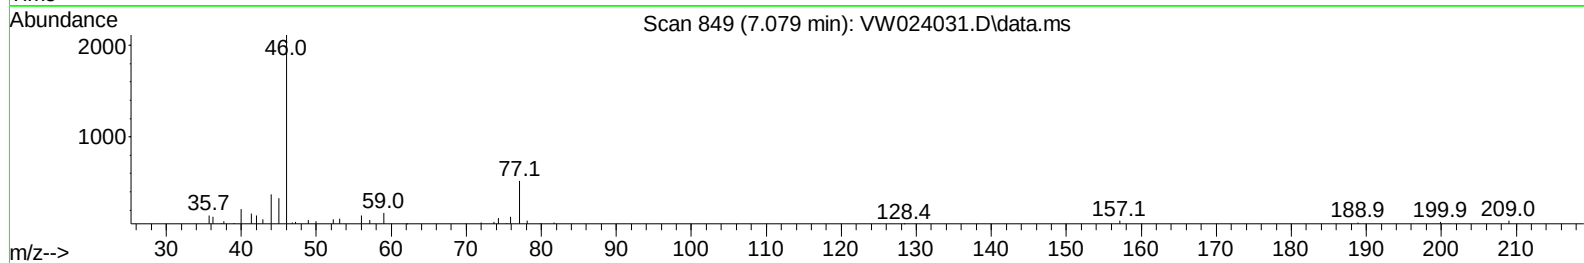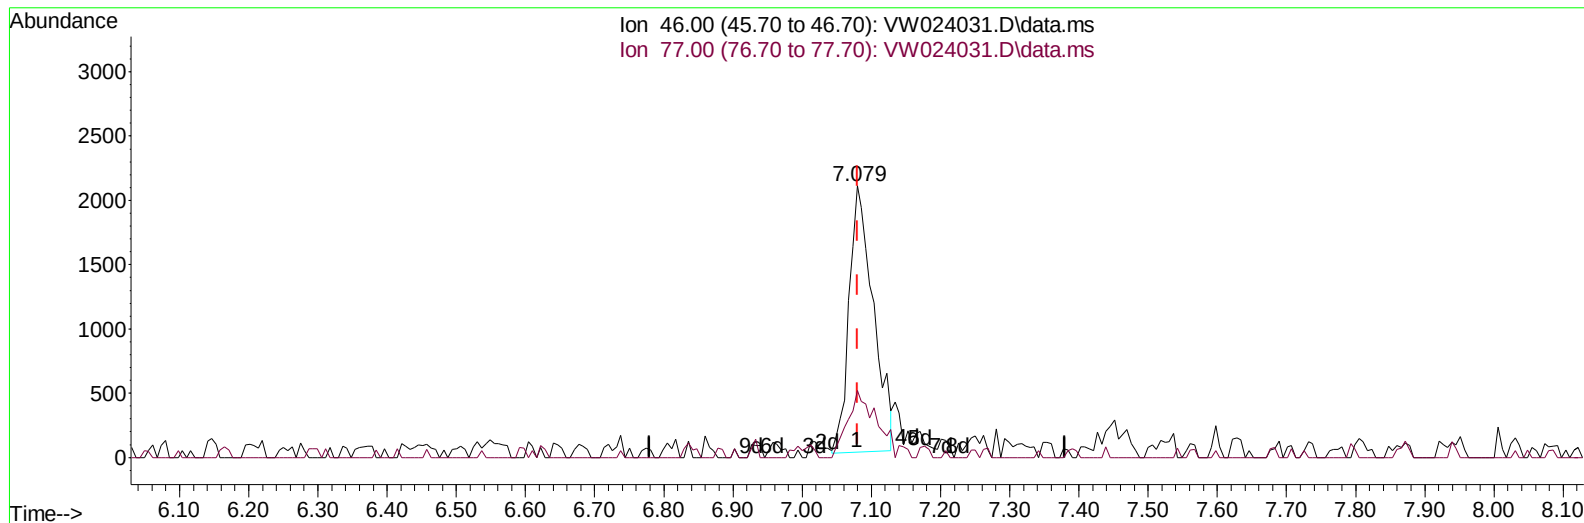

TIC: VW024031.D\data.ms

(21) 2-Butanone-d5 (S)

7.079min (-0.000) 8.37 ug/L

response 5019

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	27.77
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024031.D
 Acq On : 23 Jul 2022 02:16
 Operator : SY/VA
 Sample : N3790-13
 Misc : 2.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK7

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/24/2022
 Supervised By :Mahesh Dadoda 07/24/2022

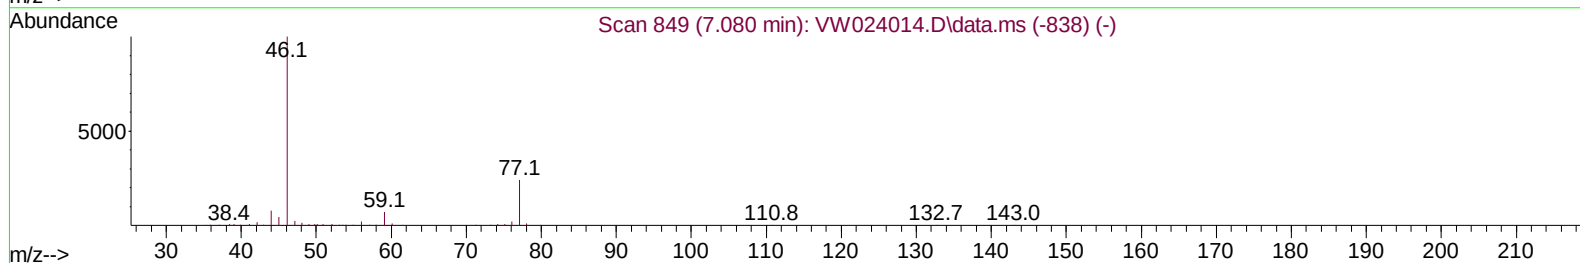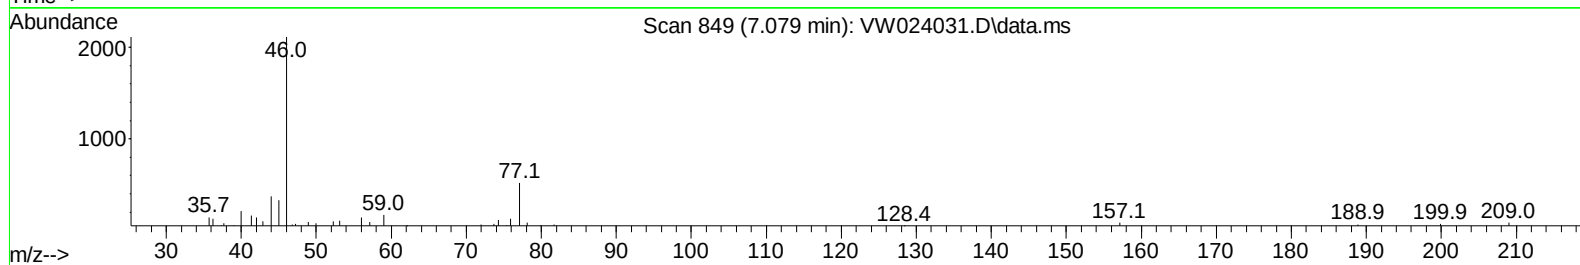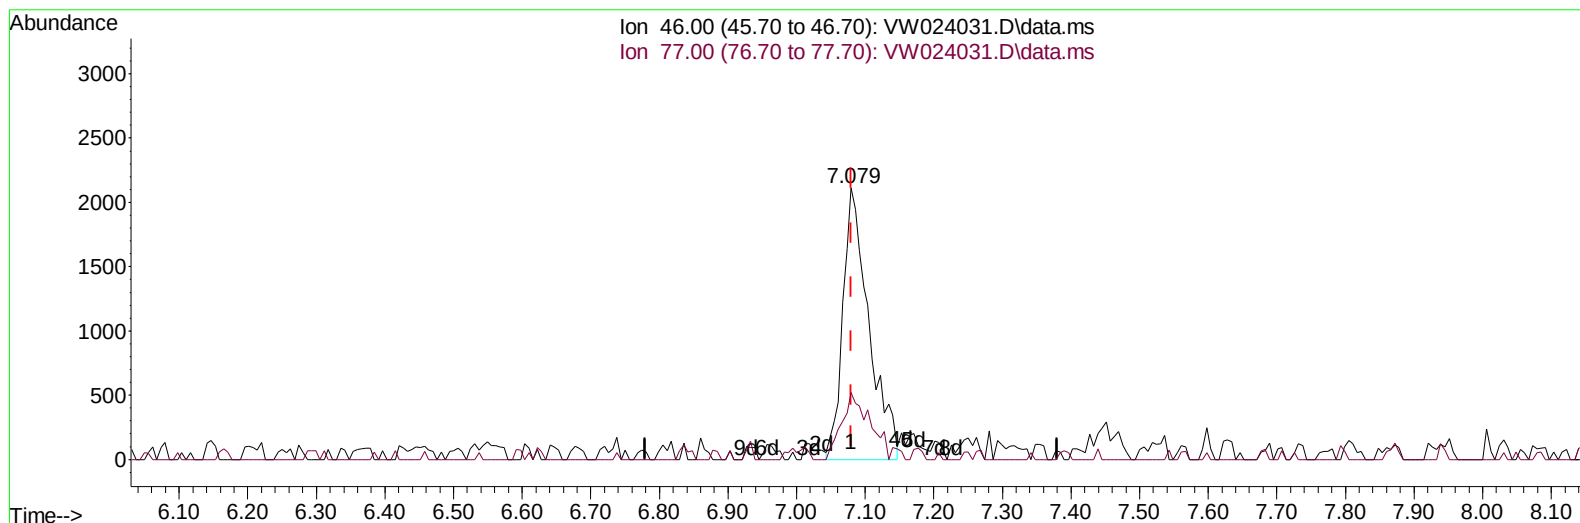

TIC: VW024031.D\data.ms

(21) 2-Butanone-d5 (S)

7.079min (-0.000) 9.29 ug/L m

response 5565

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.70	25.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024031.D
 Acq On : 23 Jul 2022 02:16
 Operator : SY/VA
 Sample : N3790-13
 Misc : 2.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK7

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/24/2022
 Supervised By :Mahesh Dadoda 07/24/2022

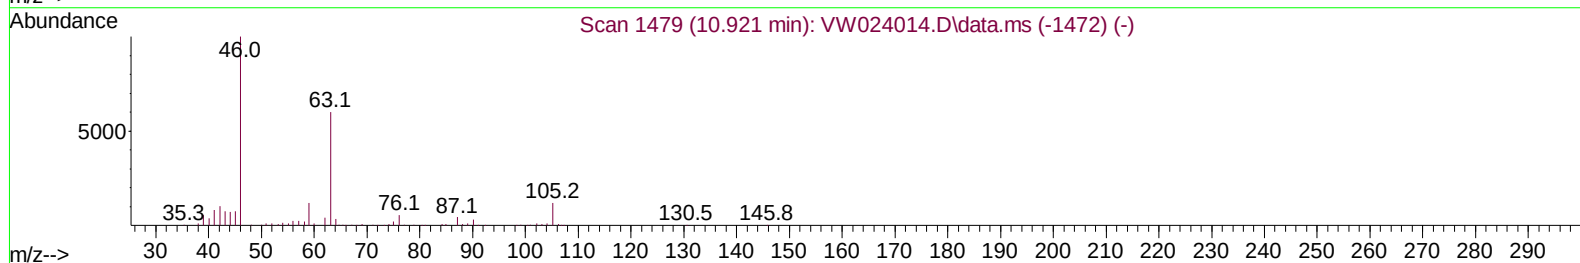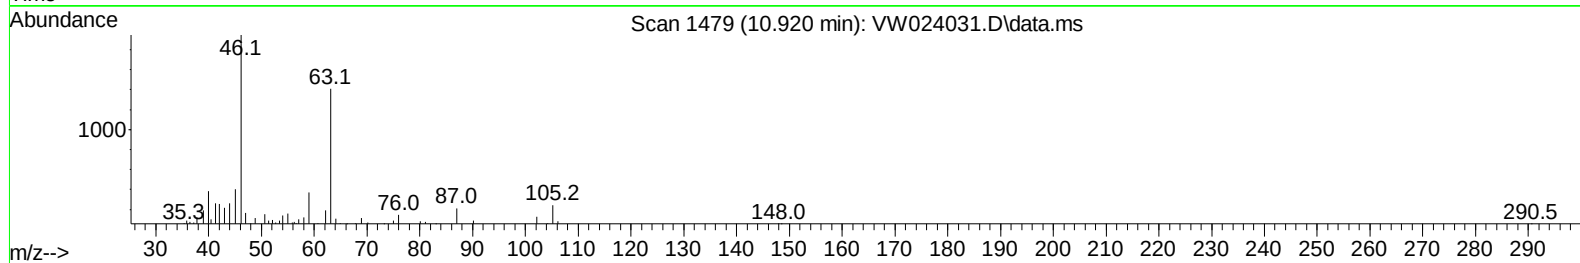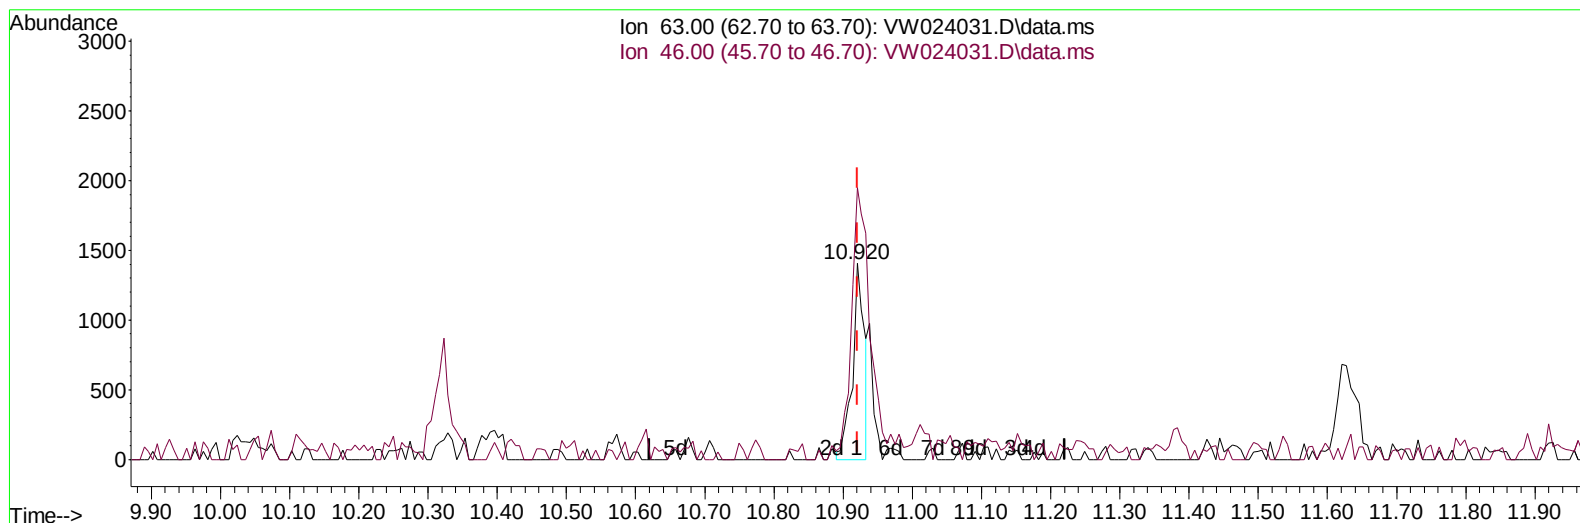

TIC: VW024031.D\data.ms

(47) 2-Hexanone-d5 (S)

10.920min (-0.000) 5.30 ug/L

response 1663

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	183.00	214.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024031.D
 Acq On : 23 Jul 2022 02:16
 Operator : SY/VA
 Sample : N3790-13
 Misc : 2.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK7

Manual IntegrationsAPPROVED

Quant Time: Jul 23 04:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/24/2022
 Supervised By :Mahesh Dadoda 07/24/2022

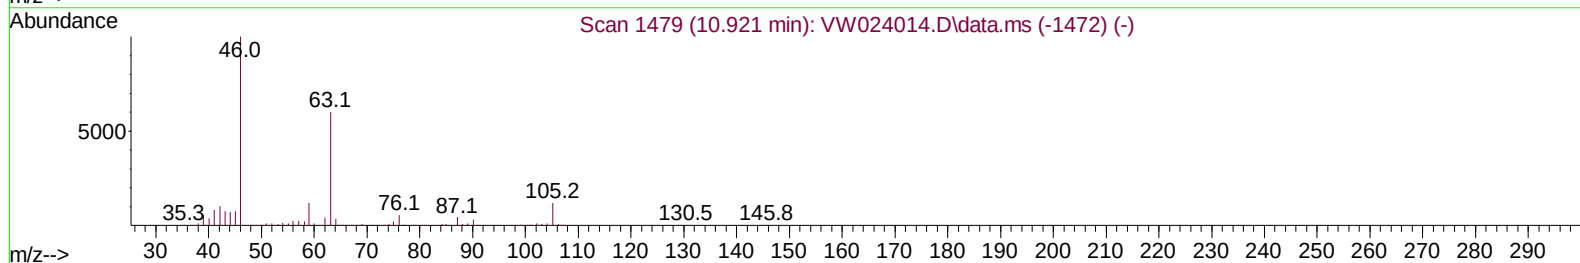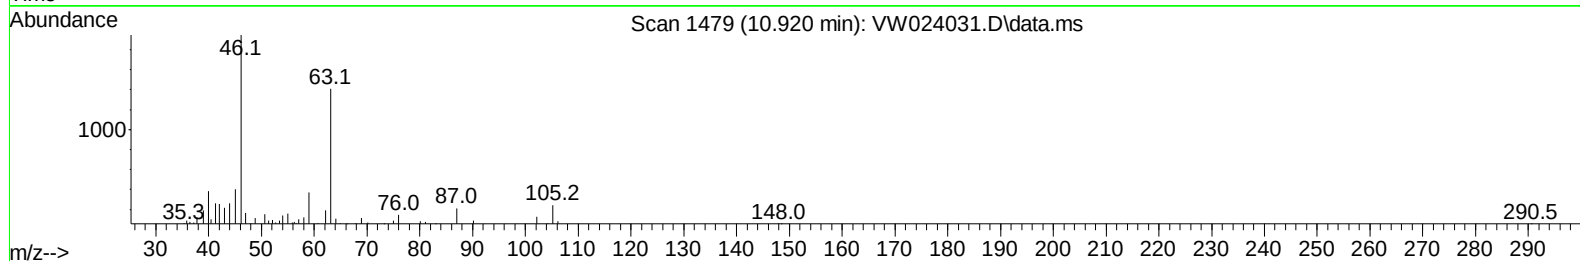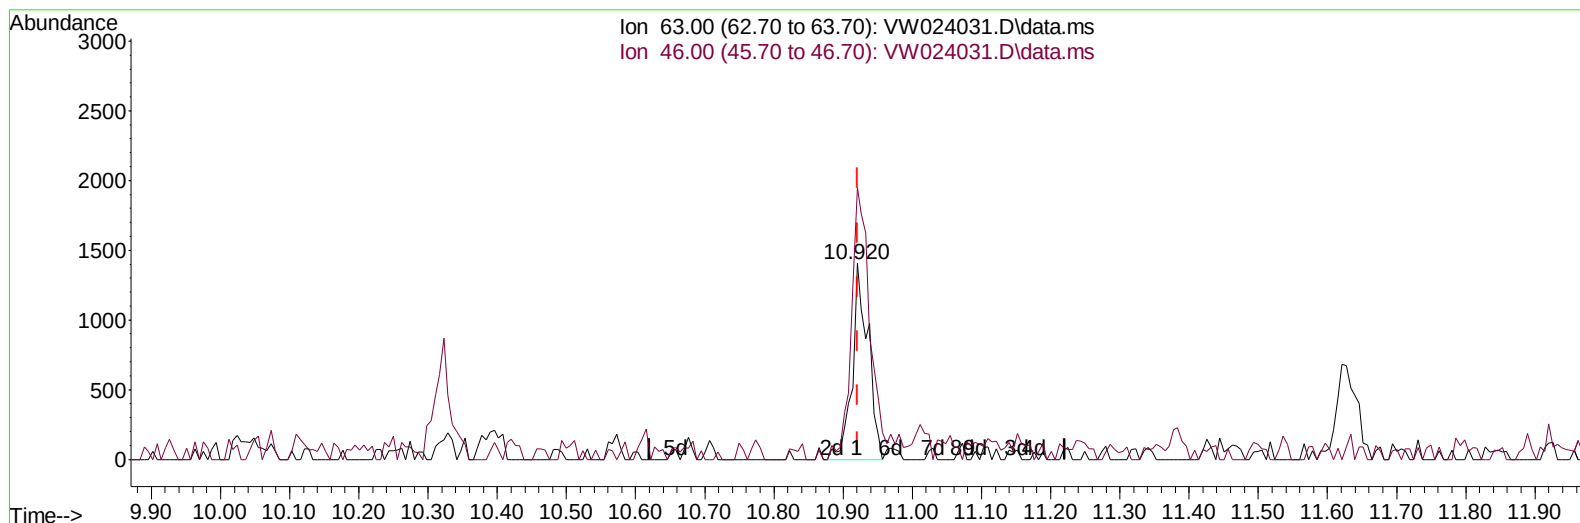

TIC: VW024031.D\data.ms

(47) 2-Hexanone-d5 (S)

10.920min (-0.000) 7.16 ug/L m

response 2246

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	183.00	158.73
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024031.D
 Acq On : 23 Jul 2022 02:16
 Operator : SY/VA
 Sample : N3790-13
 Misc : 2.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUK7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/24/2022
 Supervised By :Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 04:43:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	151287	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	95241	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	17549	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.342	65	75254	19.476	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	77.920%	
7) Chloroethane-d5	2.873	69	53392	20.713	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	82.840%	
11) 1,1-Dichloroethene-d2	4.001	63	38439	12.217	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	48.880%	
21) 2-Butanone-d5	7.079	46	5565m	9.285	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	18.580%#	
24) Chloroform-d	7.646	84	112797	25.608	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	102.440%	
26) 1,2-Dichloroethane-d4	8.305	65	68813	25.544	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	102.160%	
32) Benzene-d6	8.274	84	154068	31.119	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	124.480%	
36) 1,2-Dichloropropane-d6	9.274	67	61356	41.142	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	164.560%#	
41) Toluene-d8	10.323	98	108660	21.637	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	86.560%	
43) trans-1,3-Dichloroprop...	10.573	79	6479	9.268	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	37.080%	
47) 2-Hexanone-d5	10.920	63	2246m	7.162	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	14.320%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	40294	24.449	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	97.800%	
66) 1,2-Dichlorobenzene-d4	13.853	152	14822	23.660	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	94.640%	
Target Compounds						Qvalue
13) Acetone	4.129	43	4068m	9.600	ug/L	
16) Methylene chloride	4.903	84	12086m	5.109	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024031.D
Acq On : 23 Jul 2022 02:16
Operator : SY/VA
Sample : N3790-13
Misc : 2.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUK7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/24/2022
Supervised By :Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 04:43:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 03:31:10 2022
Response via : Initial Calibration

