




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024054.D
 Acq On : 23 Jul 2022 14:22
 Operator : SY/VA
 Sample : N3790-19
 Misc : 6.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUL5

Manual IntegrationsAPPROVED

Quant Time: Jul 24 00:42:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 06:00:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

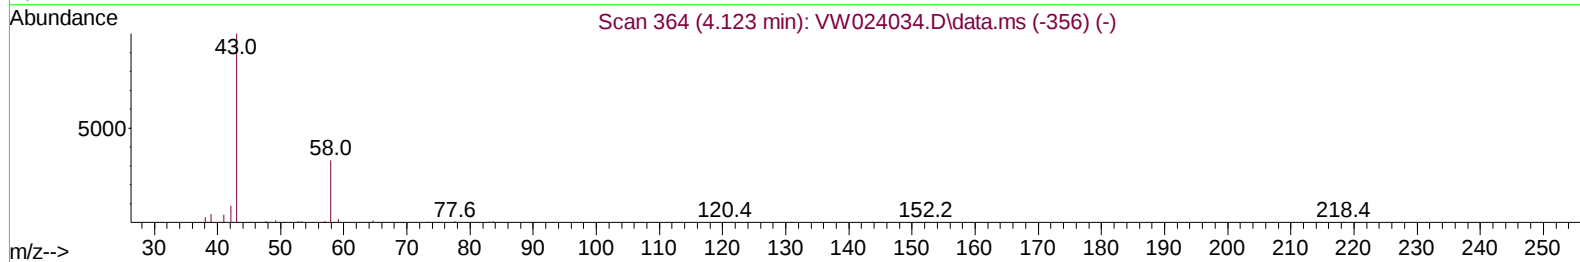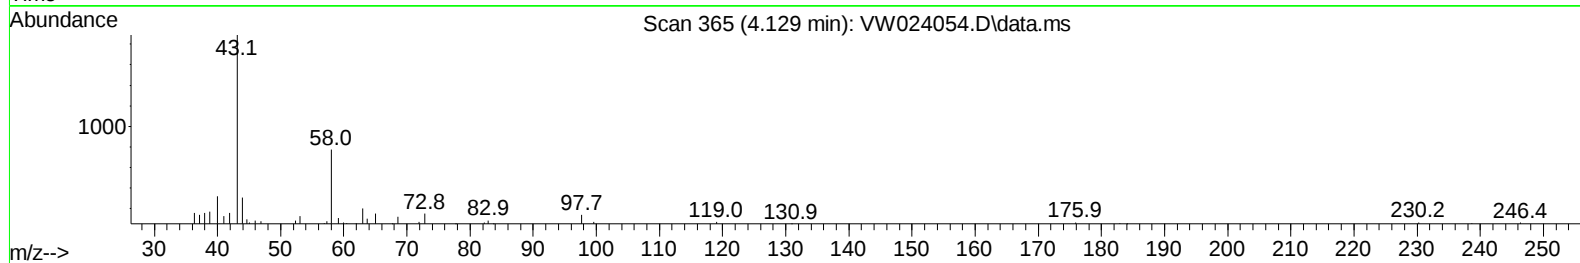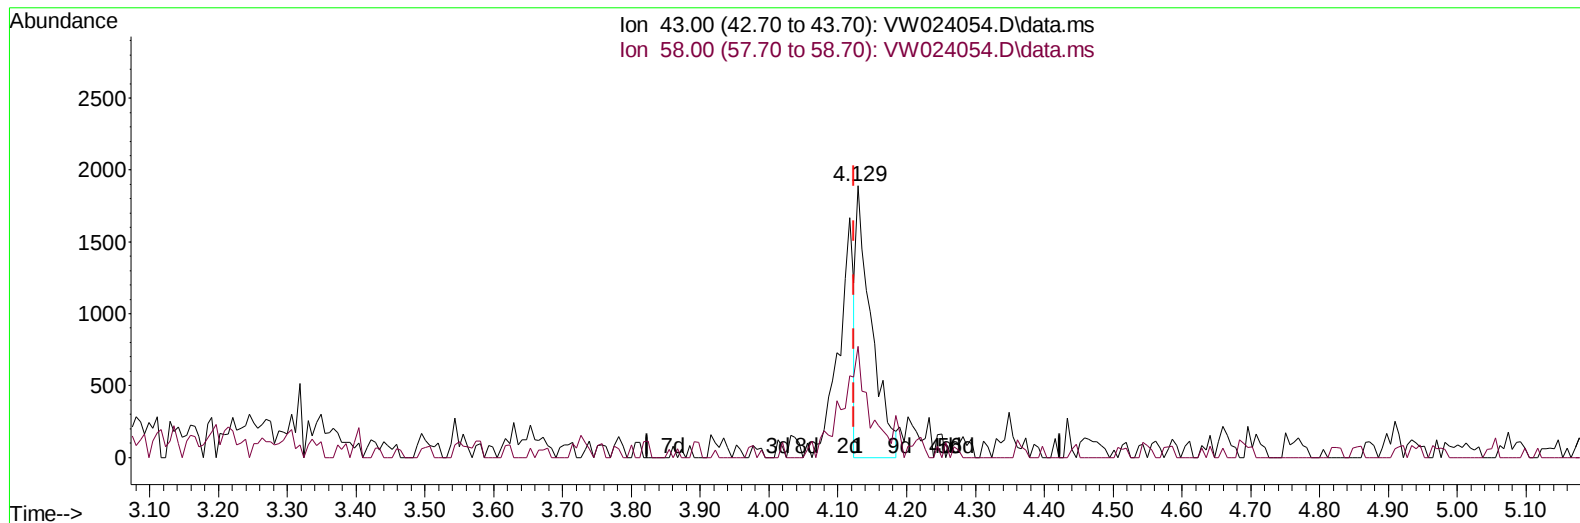

TIC: VW024054.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 5.12 ug/L

response 2885

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	42.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024054.D
 Acq On : 23 Jul 2022 14:22
 Operator : SY/VA
 Sample : N3790-19
 Misc : 6.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUL5

Manual IntegrationsAPPROVED

Quant Time: Jul 24 00:42:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 06:00:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

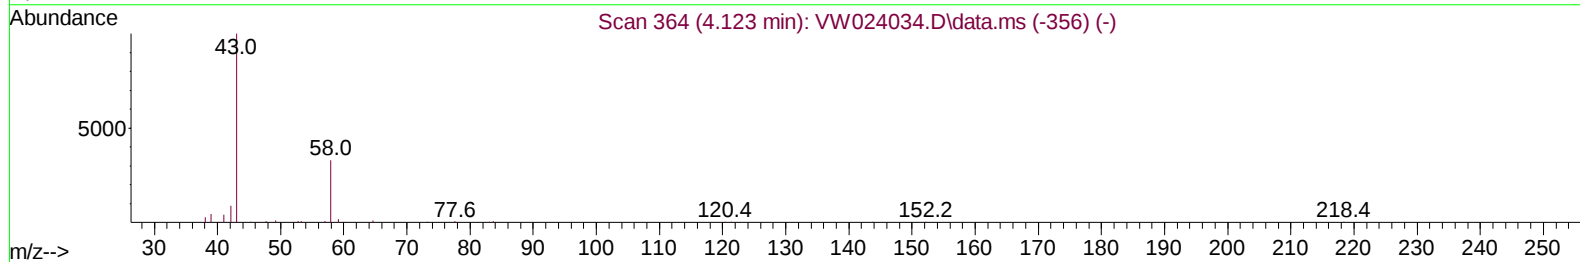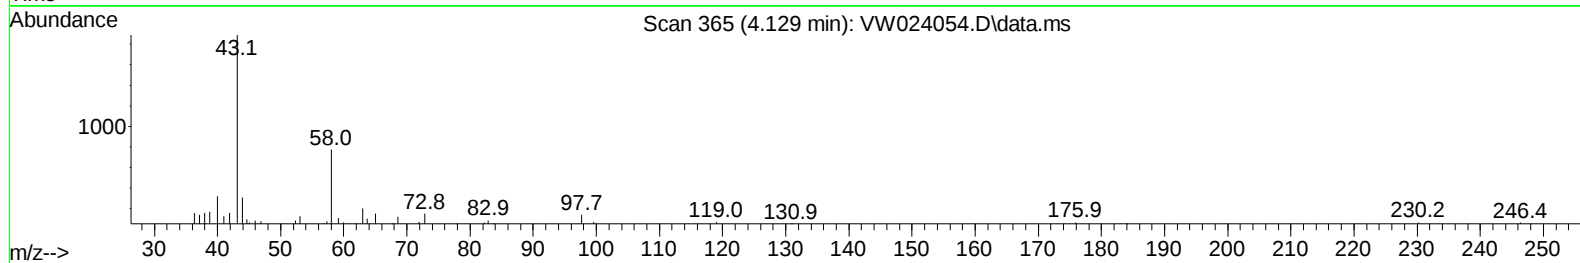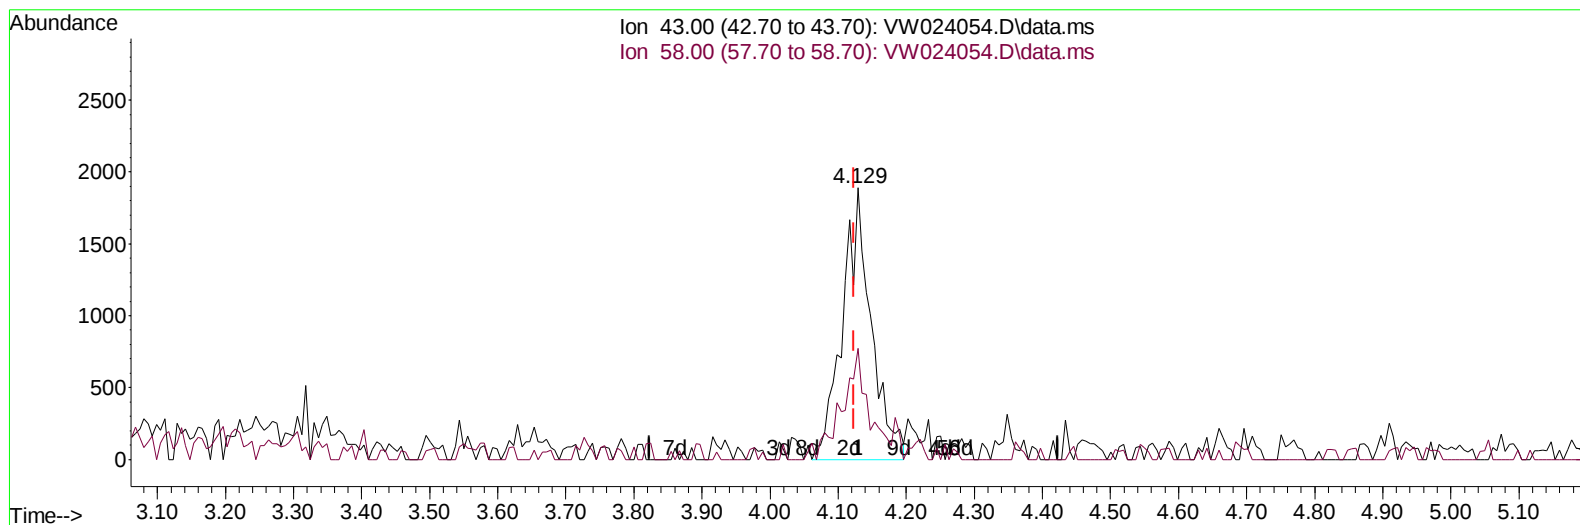

TIC: VW024054.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 9.81 ug/L m

response 5528

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.10	22.21
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024054.D
 Acq On : 23 Jul 2022 14:22
 Operator : SY/VA
 Sample : N3790-19
 Misc : 6.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUL5

Manual IntegrationsAPPROVED

Quant Time: Jul 24 00:42:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 06:00:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		201088	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		209502	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		90165	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.343	65		92227	17.957	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	71.840%		
7) Chloroethane-d5	2.873	69		72060	21.031	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	84.120%		
11) 1,1-Dichloroethene-d2	4.013	63		55770	13.335	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	53.360%		
21) 2-Butanone-d5	7.080	46		44328	55.644	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	111.280%		
24) Chloroform-d	7.647	84		140081	23.927	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	95.720%		
26) 1,2-Dichloroethane-d4	8.305	65		83820	23.409	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	93.640%		
32) Benzene-d6	8.269	84		240517	22.085	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	88.320%		
36) 1,2-Dichloropropane-d6	9.274	67		78602	23.961	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	95.840%		
41) Toluene-d8	10.323	98		216700	19.617	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	78.480%		
43) trans-1,3-Dichloroprop...	10.573	79		29577	19.235	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	76.920%		
47) 2-Hexanone-d5	10.920	63		34835	50.499	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	101.000%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		85905	23.696	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	94.800%		
66) 1,2-Dichlorobenzene-d4	13.853	152		83564	25.962	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	103.840%		
Target Compounds							
13) Acetone	4.129	43		5528m	9.815	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024054.D
Acq On : 23 Jul 2022 14:22
Operator : SY/VA
Sample : N3790-19
Misc : 6.02g/10mL/MSVOA_W/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUL5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

Quant Time: Jul 24 00:42:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 06:00:17 2022
Response via : Initial Calibration

