

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024007.D
 Acq On : 22 Jul 2022 15:10
 Operator : SY/VA
 Sample : N3743-04
 Misc : 6.29g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F5C90

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 07/23/2022
 Supervised By : Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 03:03:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 22 23:08:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	301023	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	272225	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	88032	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	136418	17.743	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	70.960%	
7) Chloroethane-d5	2.873	69	101252	19.741	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	78.960%	
11) 1,1-Dichloroethene-d2	4.001	63	81020	12.941	ug/L	-0.02
Spiked Amount	25.000	Range 45 - 110	Recovery	=	51.760%	
21) 2-Butanone-d5	7.074	46	80361	67.386	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	134.780%	
24) Chloroform-d	7.647	84	190937	21.786	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	87.160%	
26) 1,2-Dichloroethane-d4	8.305	65	130820	24.406	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	97.640%	
32) Benzene-d6	8.269	84	343550	24.277	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	97.120%	
36) 1,2-Dichloropropane-d6	9.274	67	115124	27.008	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	108.040%	
41) Toluene-d8	10.323	98	294174	20.494	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	81.960%	
43) trans-1,3-Dichloroprop...	10.573	79	38623	19.330	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	77.320%	
47) 2-Hexanone-d5	10.921	63	64083	71.495	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	142.980%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	126715	26.900	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	107.600%	
66) 1,2-Dichlorobenzene-d4	13.853	152	79140	25.183	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	100.720%	
Target Compounds						
13) Acetone	4.117	43	22887	27.145	ug/L	96
16) Methylene chloride	4.909	84	32010m	6.800	ug/L	
25) Chloroform	7.671	83	5942	0.722	ug/L	88
34) Trichloroethene	9.092	95	4394	1.076	ug/L	91
46) Tetrachloroethene	10.860	164	28592	9.052	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024007.D
Acq On : 22 Jul 2022 15:10
Operator : SY/VA
Sample : N3743-04
Misc : 6.29g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F5C90

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 07/23/2022
Supervised By : Mahesh Dadoda 07/24/2022

Quant Time: Jul 23 03:03:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 22 23:08:43 2022
Response via : Initial Calibration

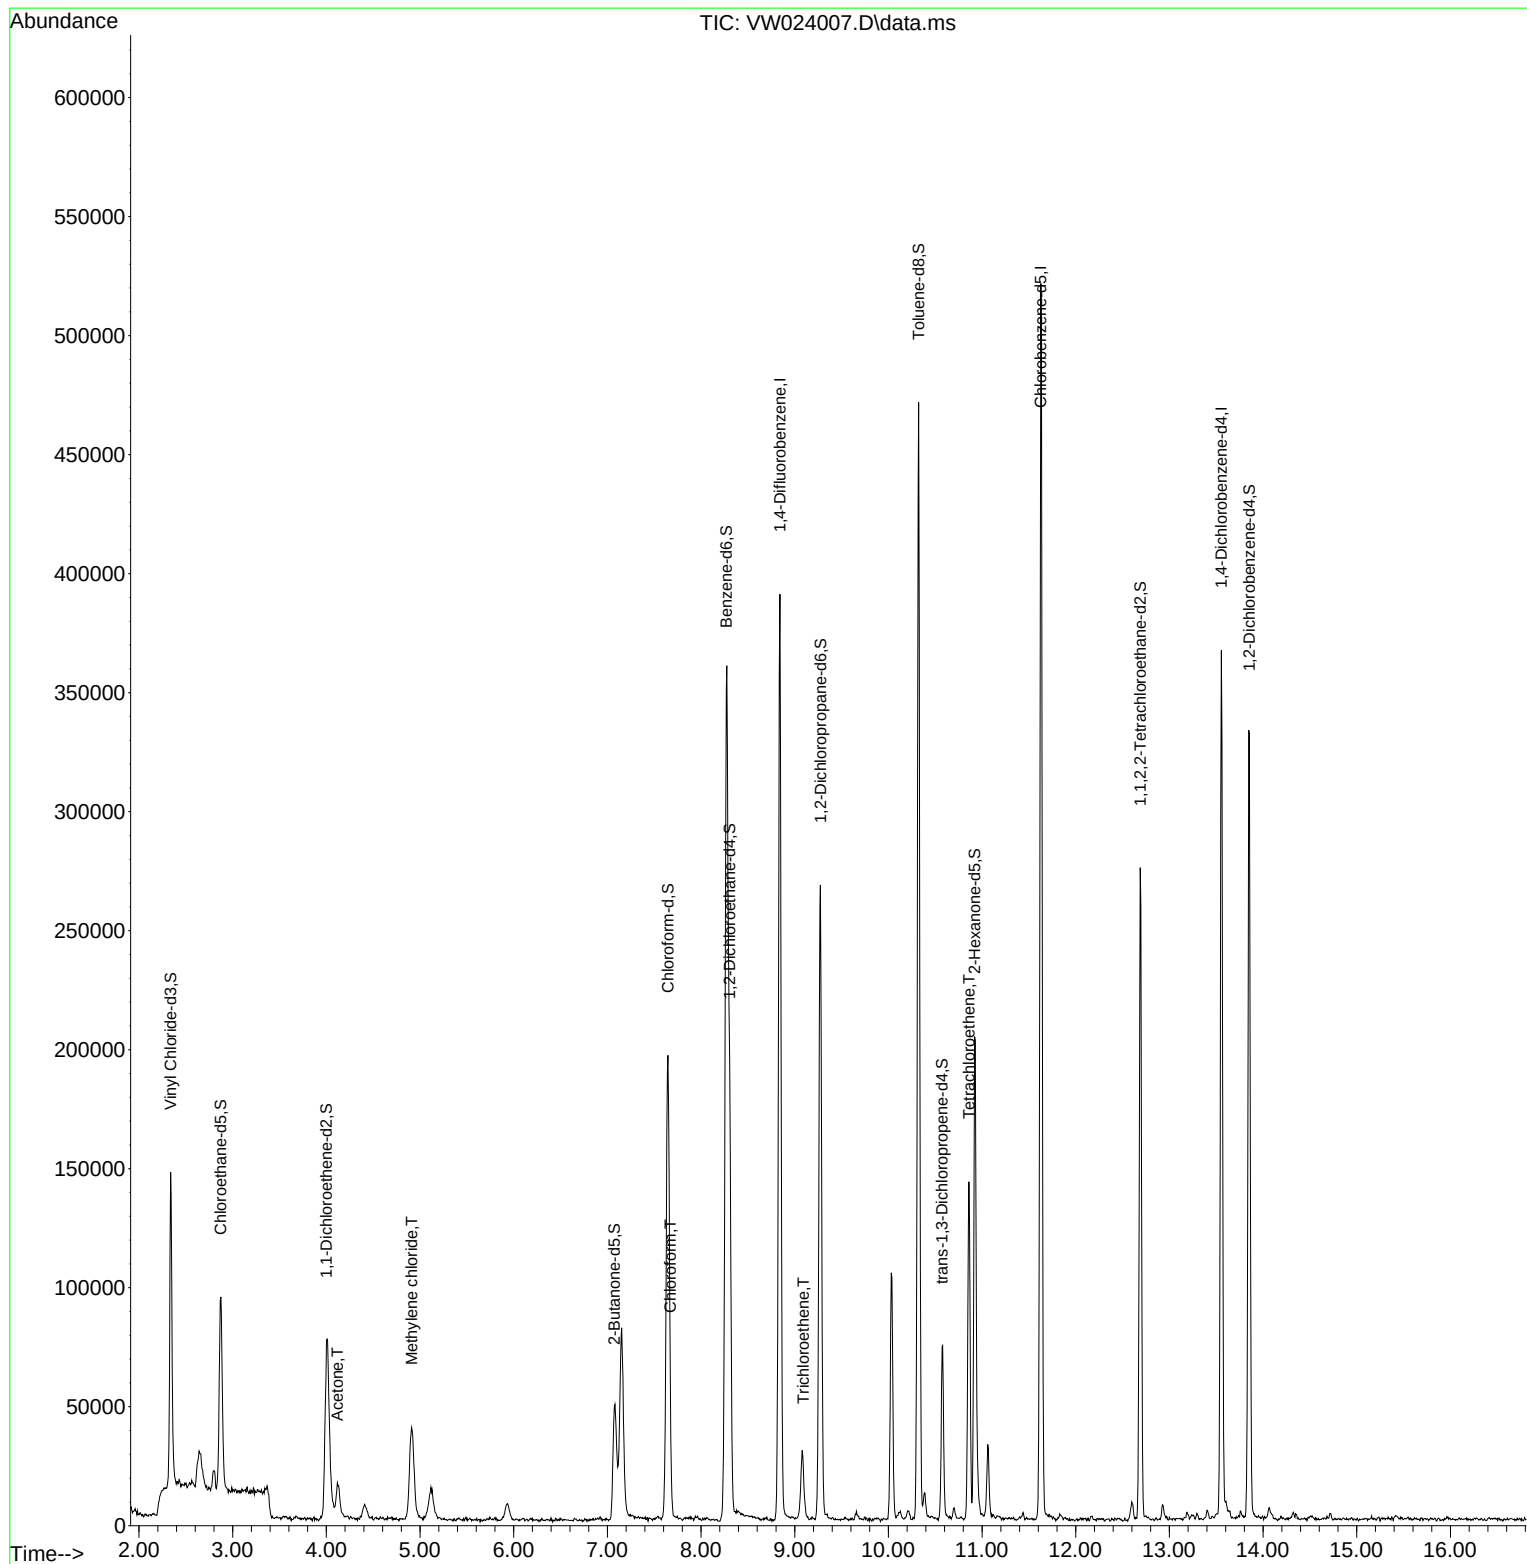

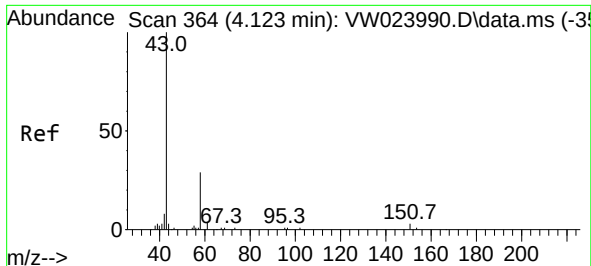





#13
Acetone
Concen: 27.145 ug/L
RT: 4.117 min Scan# 30
Delta R.T. -0.006 min
Lab File: VW024007.D
Acq: 22 Jul 2022 15:10

Instrument :
MSVOA_W
ClientSampleId :
F5C90

Tgt Ion: 43 Resp: 2288
Ion Ratio Lower Upper
43 100
58 29.6 0.0 64.2




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/23/2022
Supervised By :Mahesh Dadoda 07/24/2022

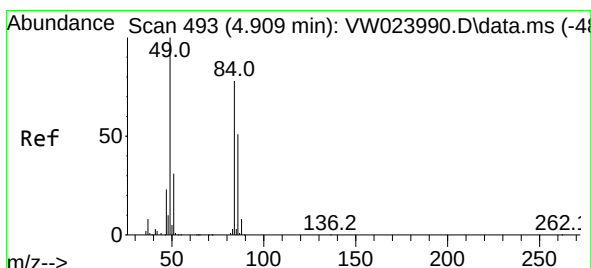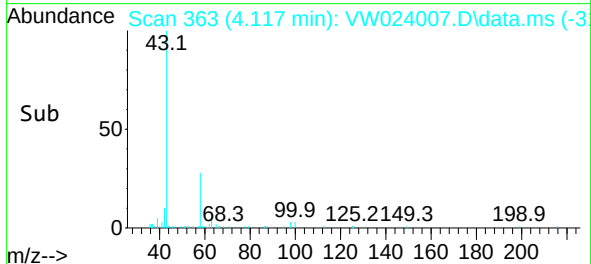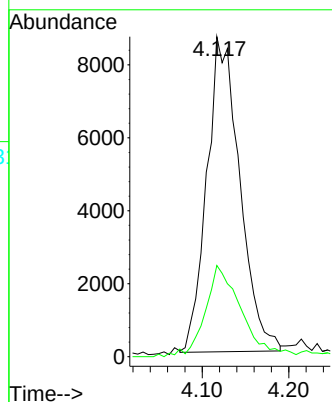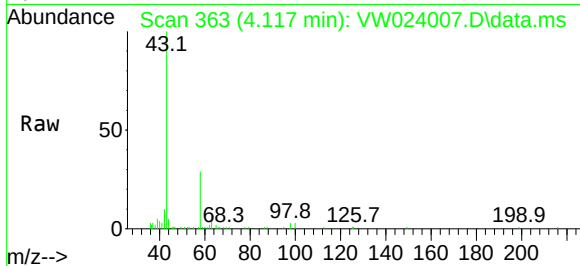

#16
Methylene chloride
Concen: 6.800 ug/L m
RT: 4.909 min Scan# 493
Delta R.T. 0.000 min
Lab File: VW024007.D
Acq: 22 Jul 2022 15:10


Tgt Ion: 84 Resp: 32010
Ion Ratio Lower Upper
84 100
86 70.9 42.8 79.6
49 130.9 85.4 158.6

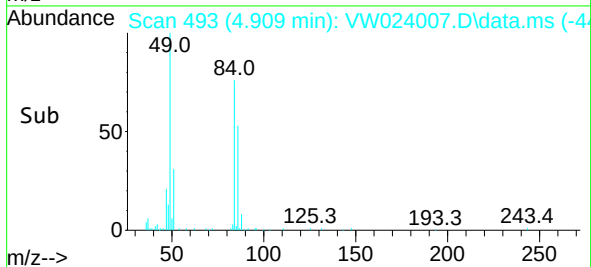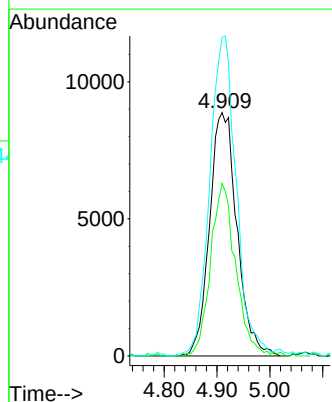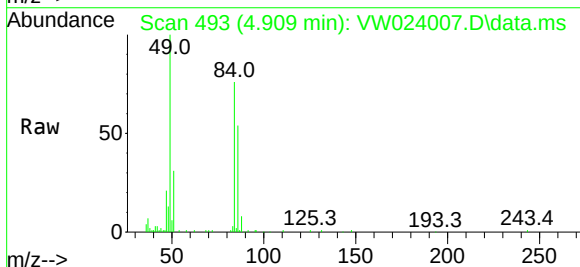

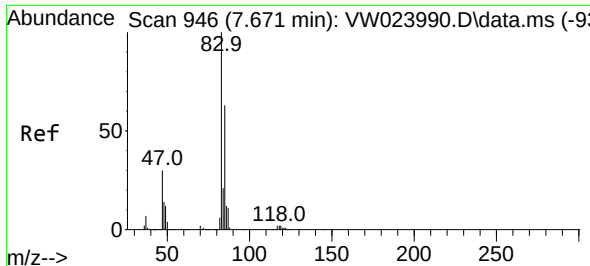

#25
Chloroform
Concen: 0.722 ug/L
RT: 7.671 min Scan# 946
Delta R.T. 0.000 min
Lab File: VW024007.D
Acq: 22 Jul 2022 15:10




Instrument :
MSVOA_W
ClientSampleId :
F5C90

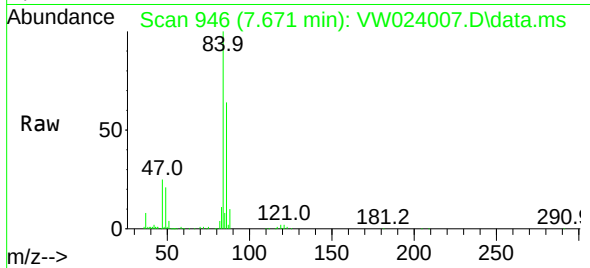

Tgt Ion: 83 Resp: 594
Ion Ratio Lower Upper
83 100
85 69.0 41.9 77.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/23/2022
Supervised By :Mahesh Dadoda 07/24/2022

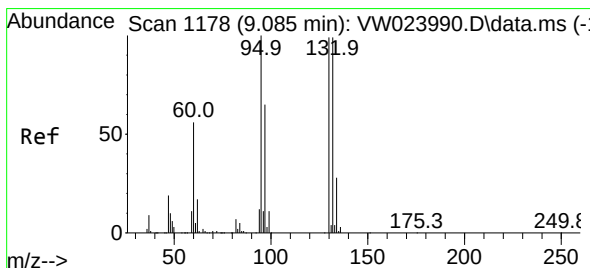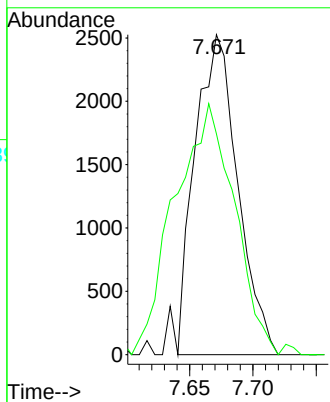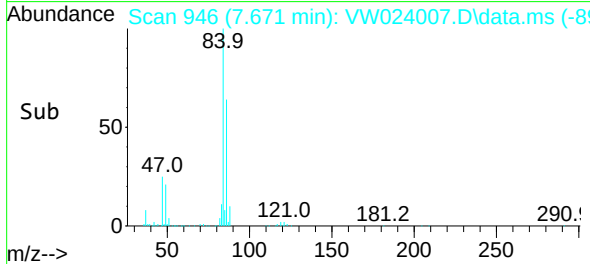

#34
Trichloroethene
Concen: 1.076 ug/L
RT: 9.092 min Scan# 1179
Delta R.T. 0.006 min
Lab File: VW024007.D
Acq: 22 Jul 2022 15:10


Tgt Ion: 95 Resp: 4394
Ion Ratio Lower Upper
95 100
97 65.1 45.6 84.8
132 82.7 69.9 129.7
130 100.9 75.4 140.0

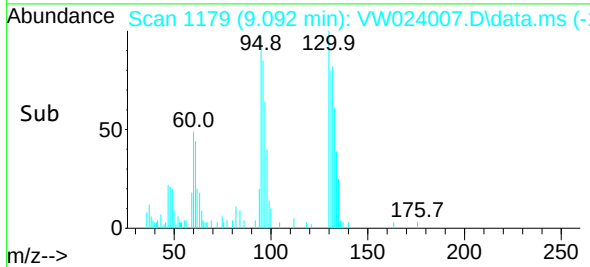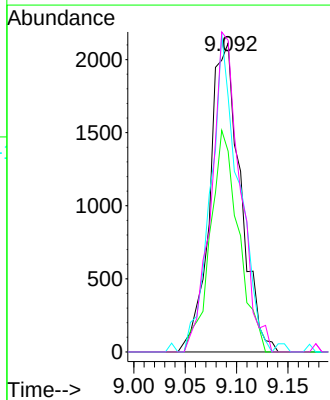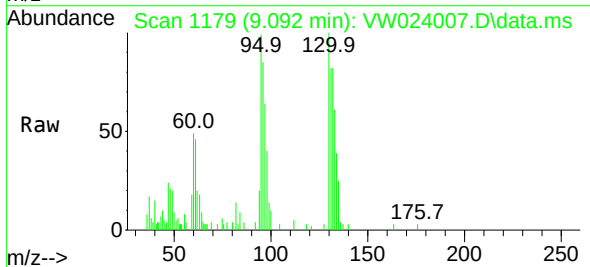

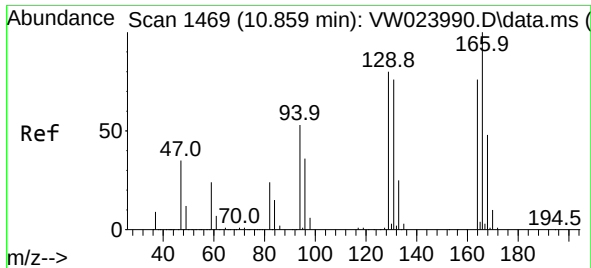

#46
Tetrachloroethene
Concen: 9.052 ug/L
RT: 10.860 min Scan# 1469
Delta R.T. 0.000 min
Lab File: VW024007.D
Acq: 22 Jul 2022 15:10

Instrument :
MSVOA_W
ClientSampleId :
F5C90

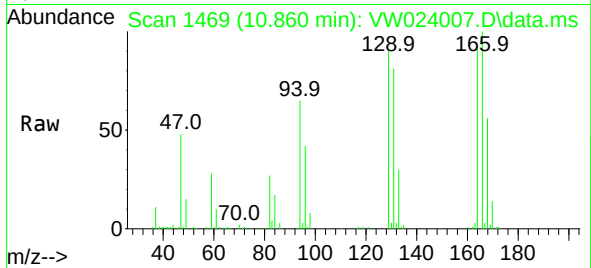

Tgt Ion:164 Resp: 28592
Ion Ratio Lower Upper
164 100
129 99.1 72.4 134.5
131 88.8 67.8 125.8
166 109.6 88.9 165.1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/23/2022
Supervised By :Mahesh Dadoda 07/24/2022

