

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024025.D
 Acq On : 22 Jul 2022 23:48
 Operator : SY/VA
 Sample : N3790-04
 Misc : 5.53g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUJ9

Quant Time: Jul 23 04:42:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 03:31:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	225154	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	191580	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	70275	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	93778	16.307	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.240%
7) Chloroethane-d5	2.879	69	65183	16.991	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.960%
11) 1,1-Dichloroethene-d2	4.007	63	56786	12.127	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.520%
21) 2-Butanone-d5	7.080	46	34584	38.772	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.540%
24) Chloroform-d	7.647	84	146186	22.300	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.200%
26) 1,2-Dichloroethane-d4	8.305	65	91096	22.721	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.880%
32) Benzene-d6	8.268	84	221404	22.232	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.920%
36) 1,2-Dichloropropane-d6	9.274	67	84901	28.302	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	113.200%
41) Toluene-d8	10.323	98	180286	17.847	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.400%
43) trans-1,3-Dichloroprop...	10.579	79	16810	11.955	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	47.800%
47) 2-Hexanone-d5	10.926	63	13659	21.653	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	43.300%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	83755	25.264	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	62280	24.826	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.320%
Target Compounds					Qvalue	
13) Acetone	4.129	43	3868	6.133	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024025.D
Acq On : 22 Jul 2022 23:48
Operator : SY/VA
Sample : N3790-04
Misc : 5.53g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUJ9

Quant Time: Jul 23 04:42:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 03:31:10 2022
Response via : Initial Calibration

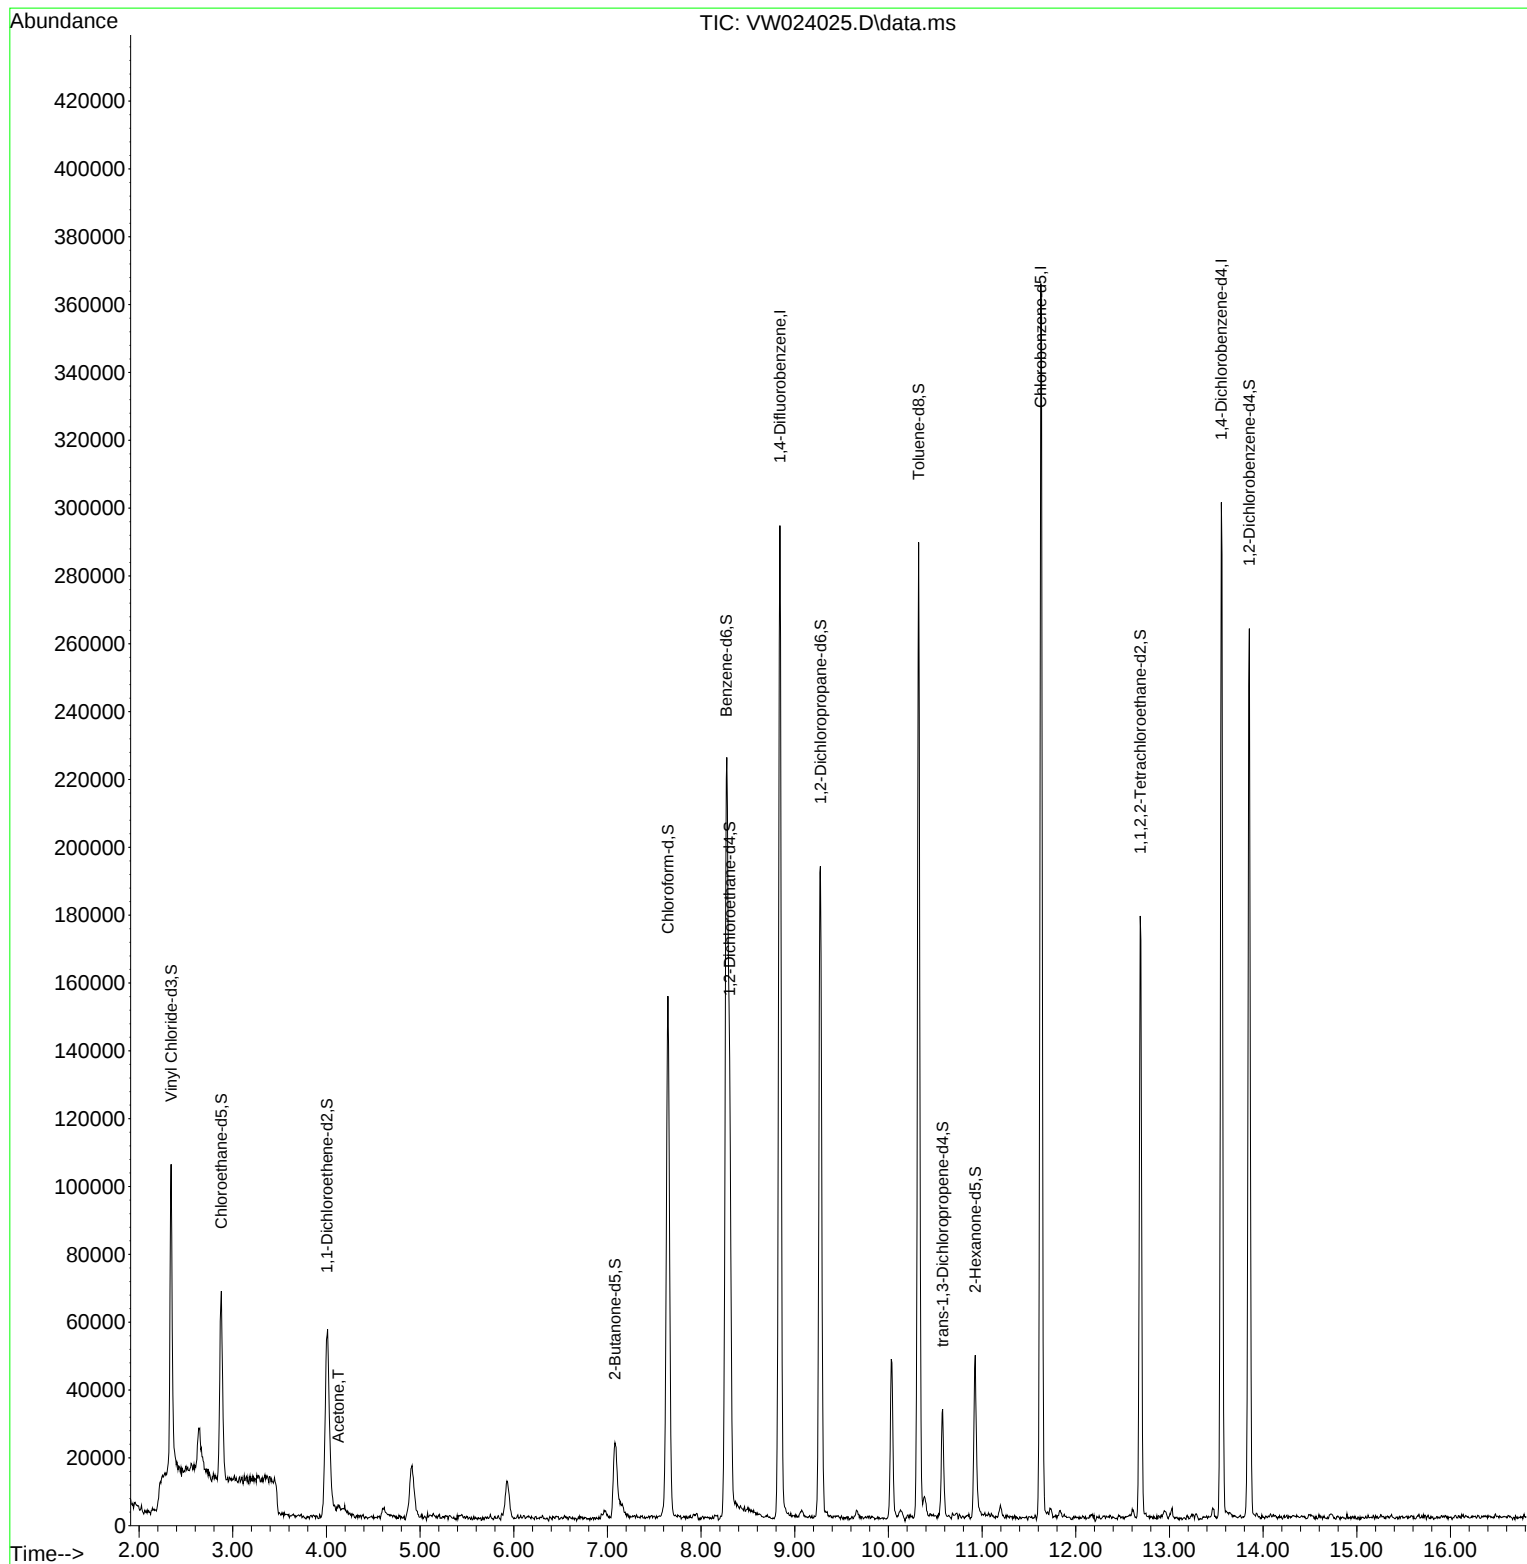

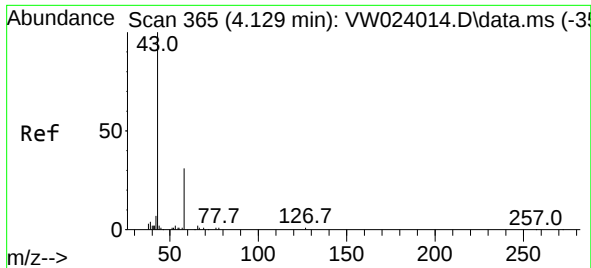

#13
 Acetone
 Concen: 6.133 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW024025.D
 Acq: 22 Jul 2022 23:48

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUJ9

Tgt Ion: 43 Resp: 3868
 Ion Ratio Lower Upper
 43 100
 58 21.0 0.0 64.2

