

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024043.D
 Acq On : 23 Jul 2022 09:52
 Operator : SY/VA
 Sample : N3795-05
 Misc : 11.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUM9

Quant Time: Jul 24 00:41:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 06:00:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	184409	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	181184	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	70455	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.337	65	72971	15.493	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.960%
7) Chloroethane-d5	2.873	69	49466	15.743	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.960%
11) 1,1-Dichloroethene-d2	4.007	63	47329	12.340	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.360%
21) 2-Butanone-d5	7.080	46	46377	63.481	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.960%
24) Chloroform-d	7.647	84	114840	21.389	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.560%
26) 1,2-Dichloroethane-d4	8.299	65	72985	22.226	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.920%
32) Benzene-d6	8.275	84	195103	20.715	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.840%
36) 1,2-Dichloropropane-d6	9.268	67	64629	22.780	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.120%
41) Toluene-d8	10.323	98	166377	17.415	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	69.680%
43) trans-1,3-Dichloroprop...	10.573	79	25992	19.545	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.200%
47) 2-Hexanone-d5	10.921	63	35207	59.016	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.040%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	79141	25.242	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.960%
66) 1,2-Dichlorobenzene-d4	13.853	152	58291	23.176	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.720%
Target Compounds					Qvalue	
13) Acetone	4.123	43	13272	25.695	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024043.D
Acq On : 23 Jul 2022 09:52
Operator : SY/VA
Sample : N3795-05
Misc : 11.38g/10mL/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBUM9

Quant Time: Jul 24 00:41:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 06:00:17 2022
Response via : Initial Calibration

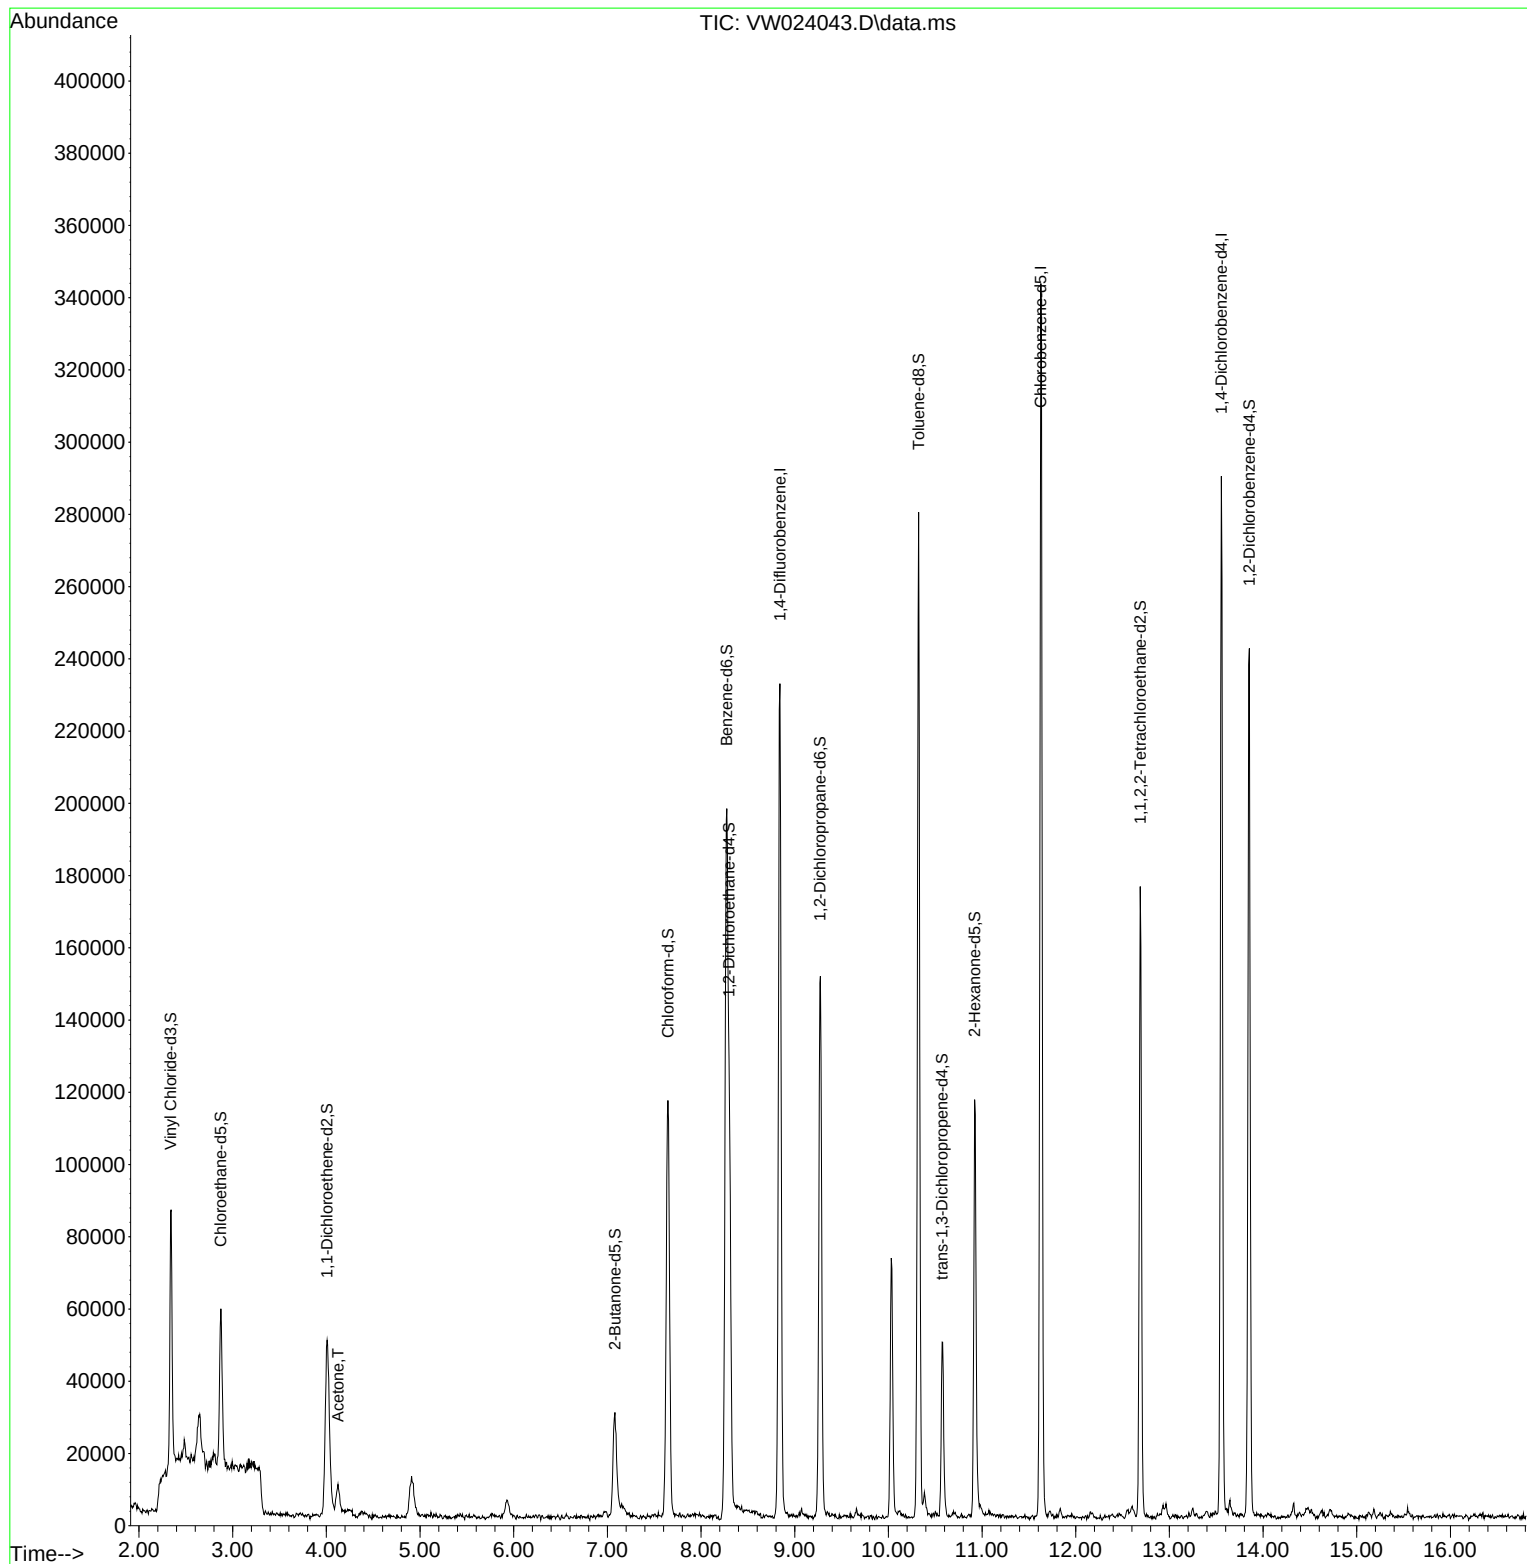

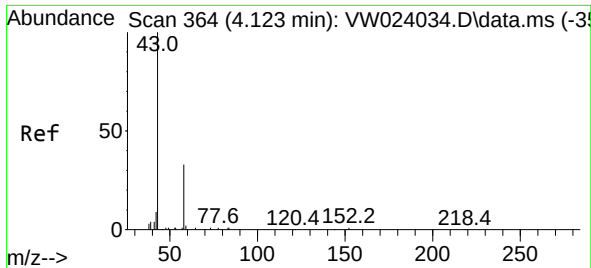

#13
 Acetone
 Concen: 25.695 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW024043.D
 Acq: 23 Jul 2022 09:52

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUM9

Tgt Ion: 43 Resp: 13272
 Ion Ratio Lower Upper
 43 100
 58 34.6 0.0 64.2

