

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024053.D
 Acq On : 23 Jul 2022 13:57
 Operator : SY/VA
 Sample : N3790-18
 Misc : 7.09g/10mL/MSVOA_W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUL4

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 07/25/2022
 Supervised By : Mahesh Dadoda 07/25/2022

Quant Time: Jul 24 00:42:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 06:00:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	204788	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	208639	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	84361	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	90419	17.287	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	69.160%		
7) Chloroethane-d5	2.873	69	69270	19.852	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.400%		
11) 1,1-Dichloroethene-d2	4.007	63	54212	12.728	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	50.920%		
21) 2-Butanone-d5	7.080	46	45564	56.162	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	112.320%		
24) Chloroform-d	7.647	84	135399	22.709	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.840%		
26) 1,2-Dichloroethane-d4	8.305	65	81885m	22.455	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	89.840%		
32) Benzene-d6	8.269	84	227704	20.995	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.960%		
36) 1,2-Dichloropropane-d6	9.274	67	75164	23.007	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	92.040%		
41) Toluene-d8	10.323	98	209316	19.027	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	76.120%		
43) trans-1,3-Dichloroprop...	10.579	79	29345	19.163	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	76.640%		
47) 2-Hexanone-d5	10.927	63	38125	55.497	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	111.000%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	86892	24.067	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	96.280%		
66) 1,2-Dichlorobenzene-d4	13.853	152	79240	26.312	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	105.240%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	13617	23.740	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024053.D
Acq On : 23 Jul 2022 13:57
Operator : SY/VA
Sample : N3790-18
Misc : 7.09g/10mL/MSVOA_W/SOIL
ALS Vial : 20 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBUL4

Quant Time: Jul 24 00:42:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 06:00:17 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

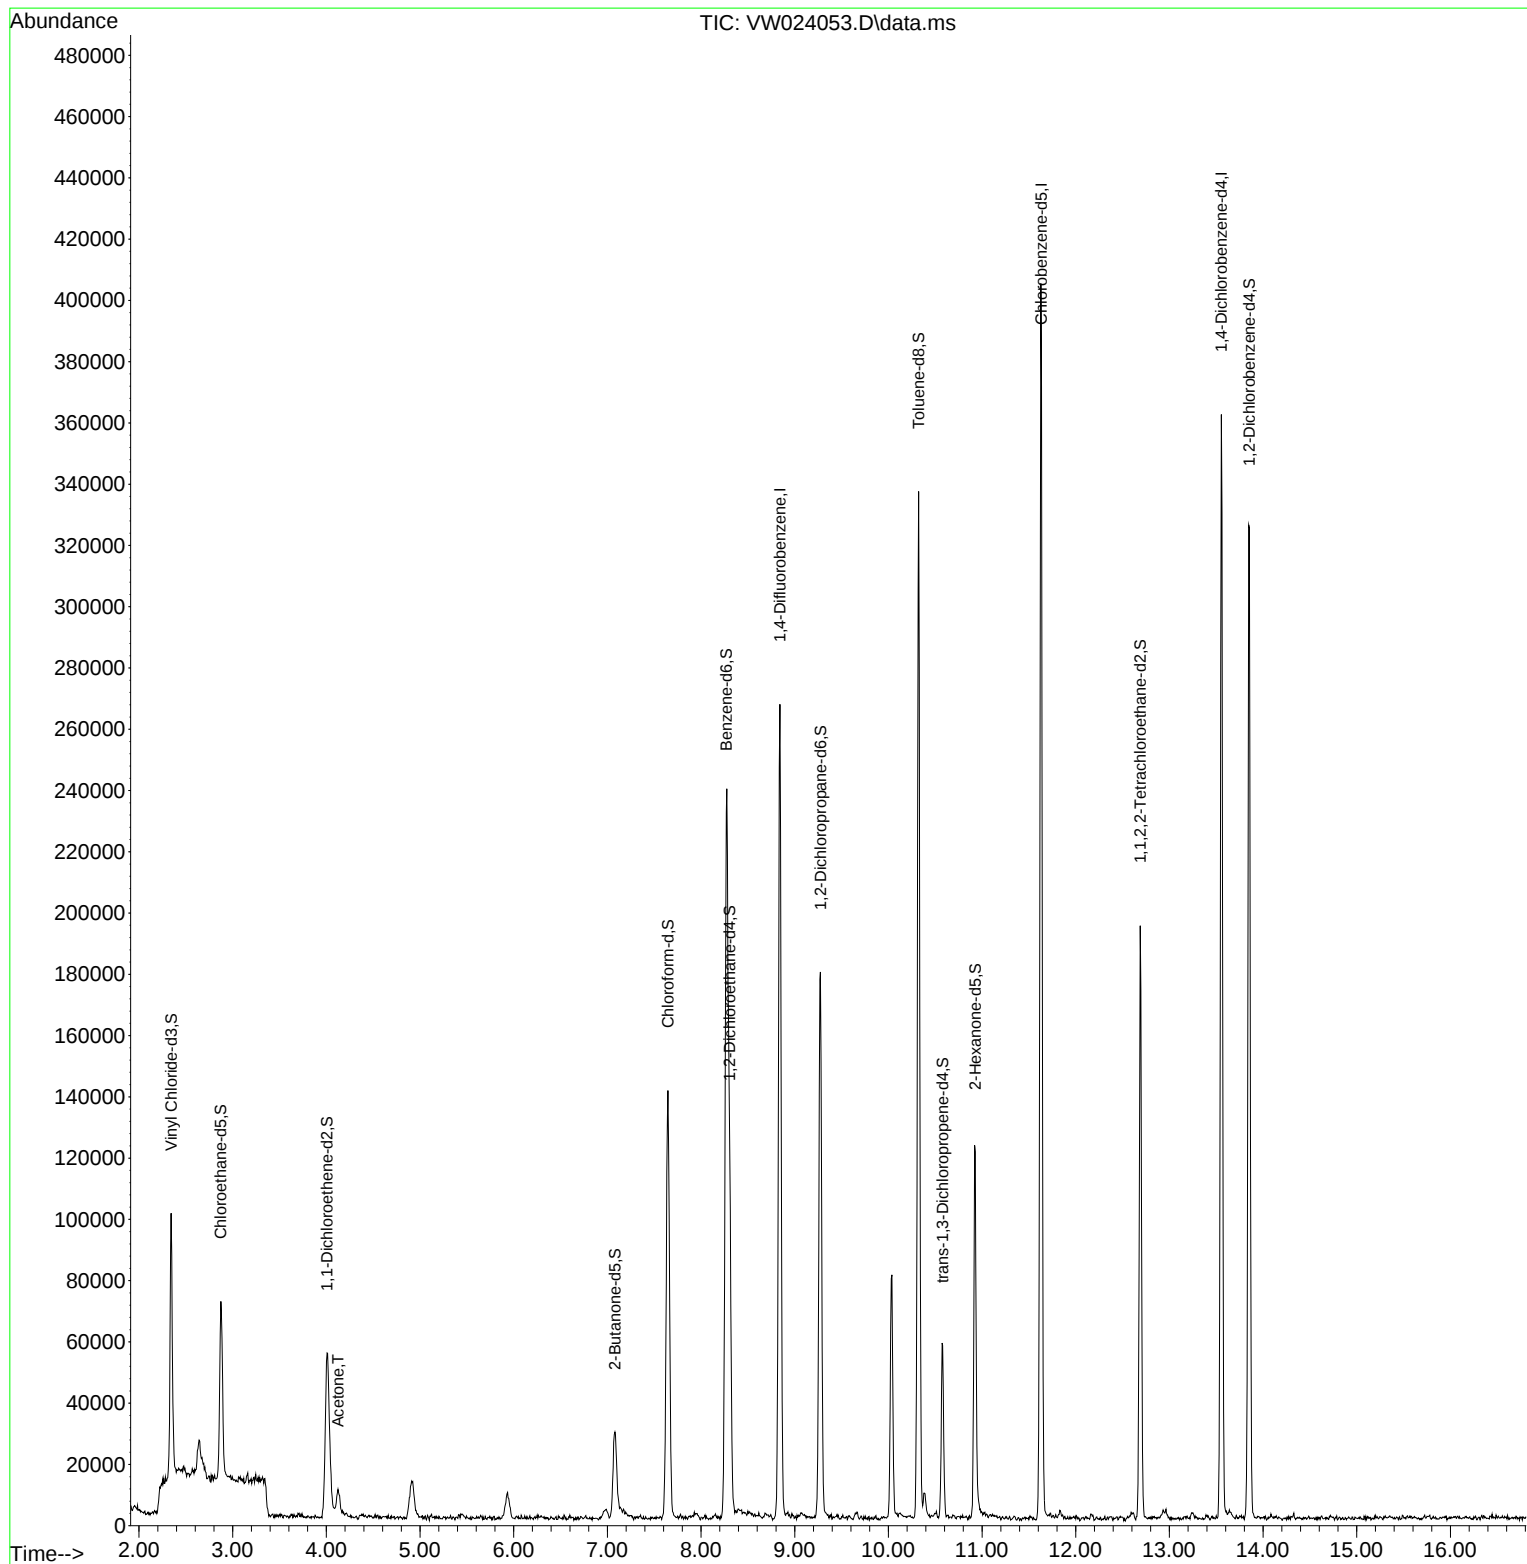

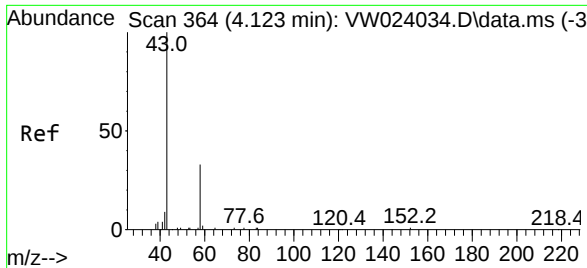

#13
Acetone
Concen: 23.740 ug/L
RT: 4.123 min Scan# 30
Delta R.T. 0.000 min
Lab File: VW024053.D
Acq: 23 Jul 2022 13:57

Instrument :
MSVOA_W
ClientSampleId :
DBUL4

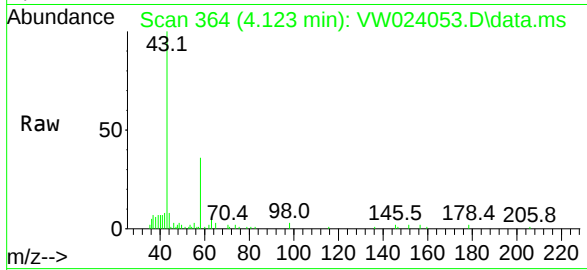

Tgt Ion: 43 Resp: 1361
Ion Ratio Lower Upper
43 100
58 28.8 0.0 64.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

