

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
 Data File : VW024054.D
 Acq On : 23 Jul 2022 14:22
 Operator : SY/VA
 Sample : N3790-19
 Misc : 6.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBUL5

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/25/2022
 Supervised By :Mahesh Dadoda 07/25/2022

Quant Time: Jul 24 00:42:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jul 23 06:00:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	201088	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	209502	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	90165	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	92227	17.957	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.840%		
7) Chloroethane-d5	2.873	69	72060	21.031	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	84.120%		
11) 1,1-Dichloroethene-d2	4.013	63	55770	13.335	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	53.360%		
21) 2-Butanone-d5	7.080	46	44328	55.644	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	111.280%		
24) Chloroform-d	7.647	84	140081	23.927	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	95.720%		
26) 1,2-Dichloroethane-d4	8.305	65	83820	23.409	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	93.640%		
32) Benzene-d6	8.269	84	240517	22.085	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.320%		
36) 1,2-Dichloropropane-d6	9.274	67	78602	23.961	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.840%		
41) Toluene-d8	10.323	98	216700	19.617	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	78.480%		
43) trans-1,3-Dichloroprop...	10.573	79	29577	19.235	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	76.920%		
47) 2-Hexanone-d5	10.920	63	34835	50.499	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.000%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	85905	23.696	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.800%		
66) 1,2-Dichlorobenzene-d4	13.853	152	83564	25.962	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	103.840%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	5528m	9.815	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072222\
Data File : VW024054.D
Acq On : 23 Jul 2022 14:22
Operator : SY/VA
Sample : N3790-19
Misc : 6.02g/10mL/MSVOA_W/SOIL
ALS Vial : 21 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBUL5

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/25/2022
Supervised By :Mahesh Dadoda 07/25/2022

Quant Time: Jul 24 00:42:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM071322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jul 23 06:00:17 2022
Response via : Initial Calibration

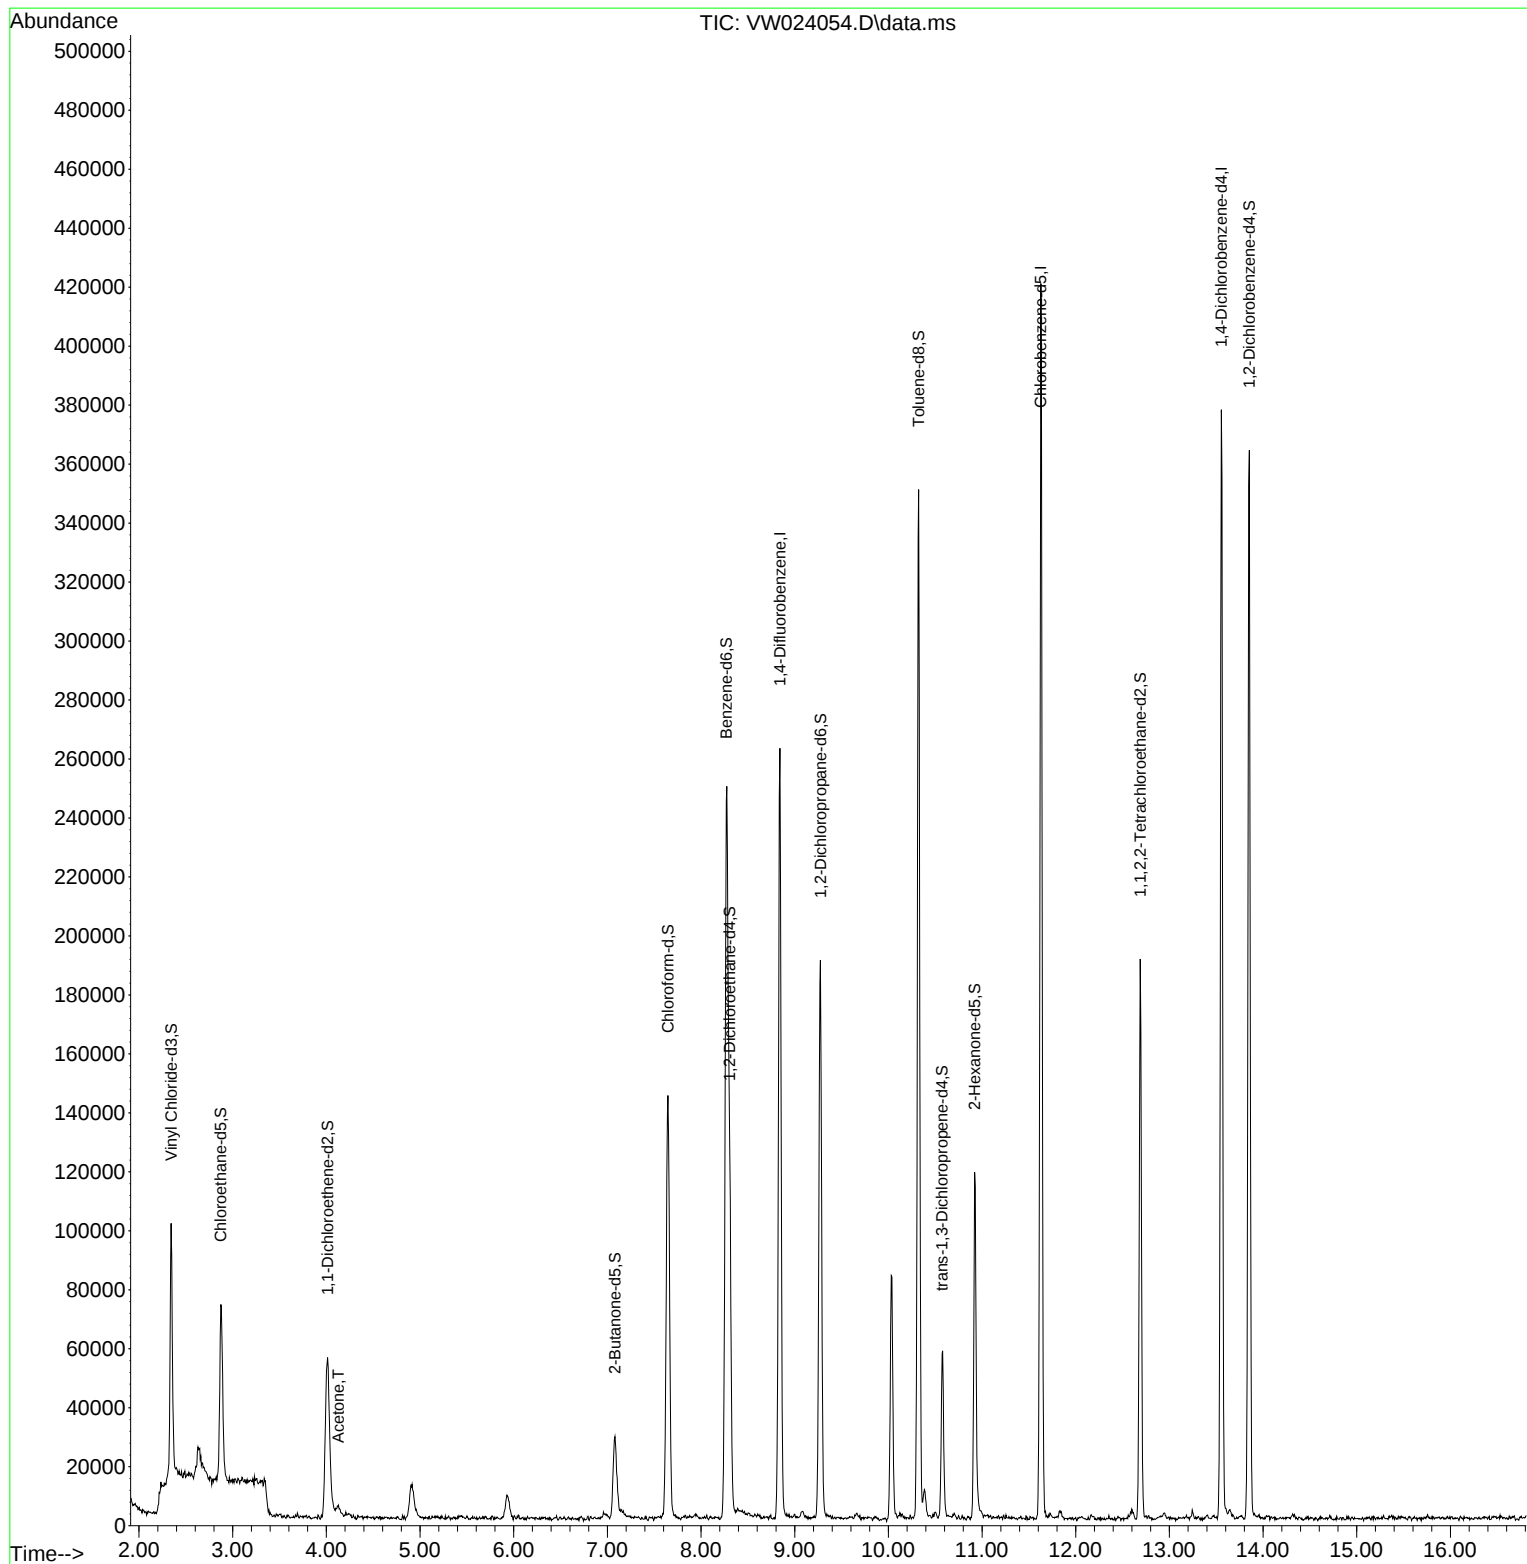

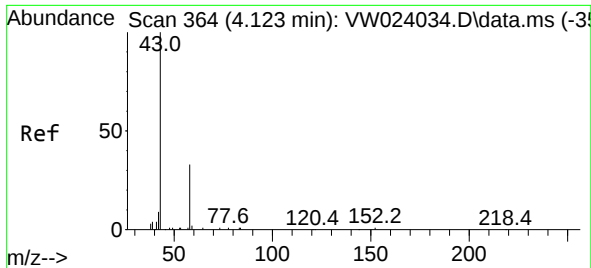

#13

Acetone

Concen: 9.815 ug/L m

RT: 4.129 min Scan# 30

Delta R.T. 0.006 min

Lab File: VW024054.D

Acq: 23 Jul 2022 14:22

Instrument :

MSVOA_W

ClientSampleId :

DBUL5

Tgt Ion: 43 Resp: 5528

Ion Ratio Lower Upper

43 100

58 22.2 0.0 64.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 07/25/2022

Supervised By :Mahesh Dadoda 07/25/2022

