

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072224\
 Data File : VW029678.D
 Acq On : 22 Jul 2024 13:02
 Operator : SY/MD
 Sample : P3298-15
 Misc : 6.87g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BHB45

Manual IntegrationsAPPROVED

Quant Time: Jul 22 14:35:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 19 23:16:32 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/23/2024
 Supervised By :Mahesh Dadoda 07/24/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	376566	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	356841	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	171636	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	70031	11.512	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	46.040%
7) Chloroethane-d5	2.899	69	59057	13.483	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.920%
11) 1,1-Dichloroethene-d2	4.027	65	35131	12.861	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.440%
21) 2-Butanone-d5	7.081	46	53517	29.307	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	58.620%
24) Chloroform-d	7.648	84	168148	15.446	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	61.800%
26) 1,2-Dichloroethane-d4	8.307	65	103568m	16.220	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	64.880%#
32) Benzene-d6	8.270	84	320037	14.971	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	59.880%
36) 1,2-Dichloropropane-d6	9.276	67	110055	16.102	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	64.400%#
41) Toluene-d8	10.319	98	275730	14.667	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	58.680%
43) trans-1,3-Dichloroprop...	10.575	79	39835	13.763	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	55.040%
47) 2-Hexanone-d5	10.922	63	37056	29.836	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.680%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	88095	15.875	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	63.480%
66) 1,2-Dichlorobenzene-d4	13.848	152	98187	16.427	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	65.720%#
Target Compounds						
16) Methylene chloride	4.923	84	27924	4.142	ug/L	95
20) cis-1,2-Dichloroethene	7.173	96	49669	8.762	ug/L	95
34) Trichloroethene	9.099	95	5591	0.948	ug/L	83
46) Tetrachloroethene	10.861	164	8709	2.079	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072224\
 Data File : VW029678.D
 Acq On : 22 Jul 2024 13:02
 Operator : SY/MD
 Sample : P3298-15
 Misc : 6.87g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BHB45

Manual IntegrationsAPPROVED

Quant Time: Jul 22 14:35:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 19 23:16:32 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 07/23/2024
 Supervised By :Mahesh Dadoda 07/24/2024

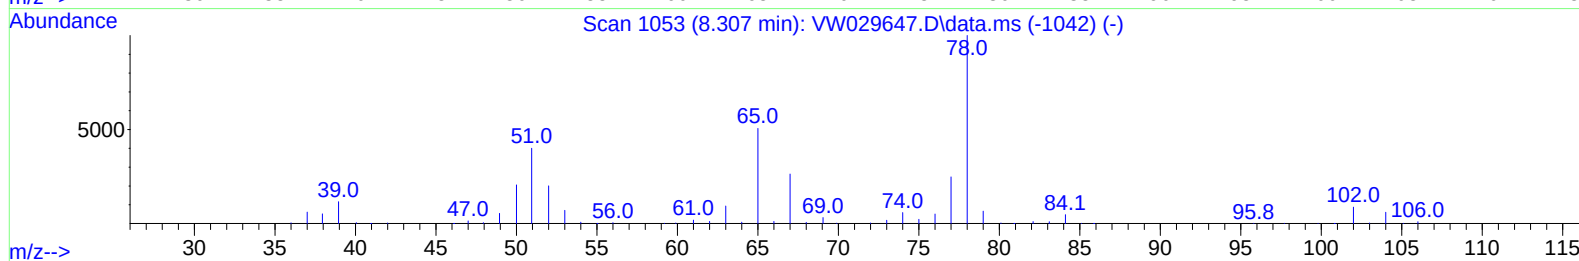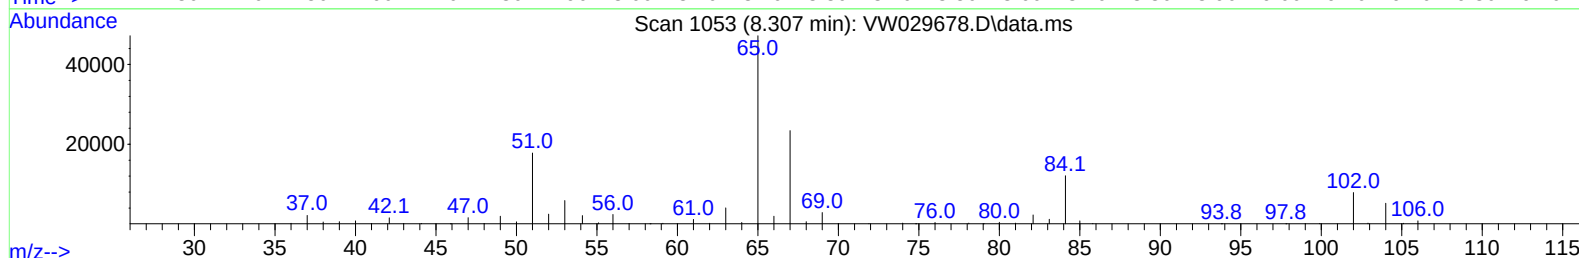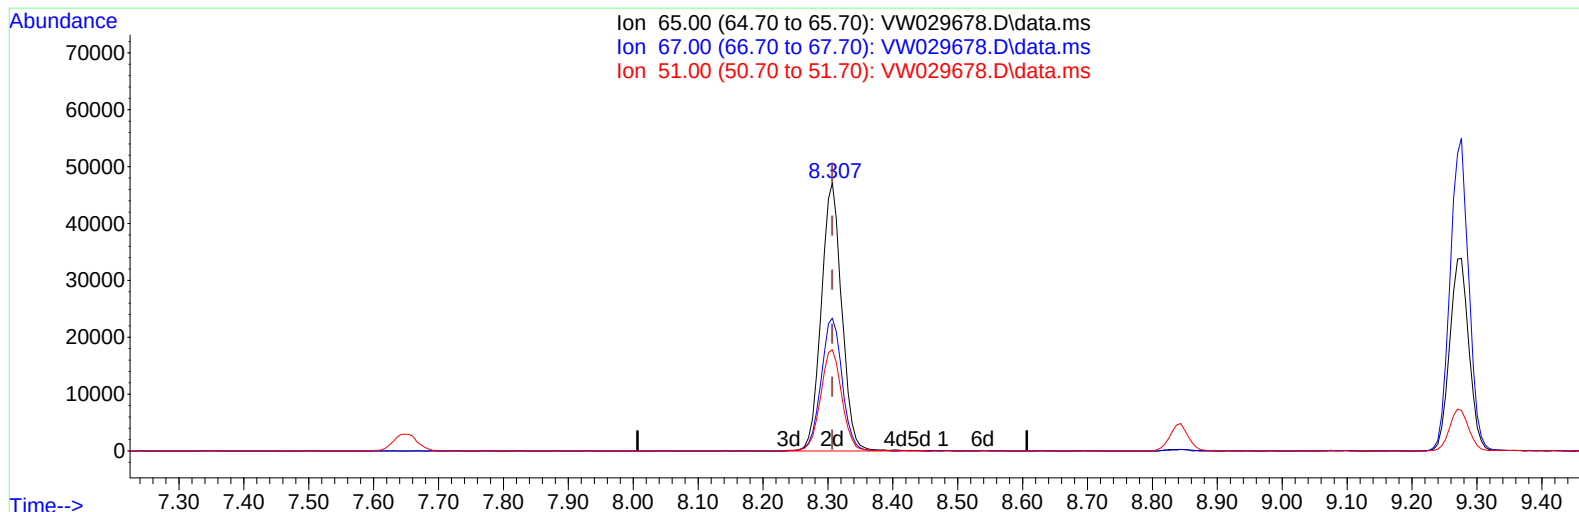

TIC: VW029678.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 16.22 ug/L m

response 103568

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.60	0.04#
51.00	101.40	0.08#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072224\
Data File : VW029678.D
Acq On : 22 Jul 2024 13:02
Operator : SY/MD
Sample : P3298-15
Misc : 6.87g/10mL/MSVOA_W/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BHB45

Manual IntegrationsAPPROVED

Quant Time: Jul 22 14:35:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 19 23:16:32 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/23/2024
Supervised By :Mahesh Dadoda 07/24/2024

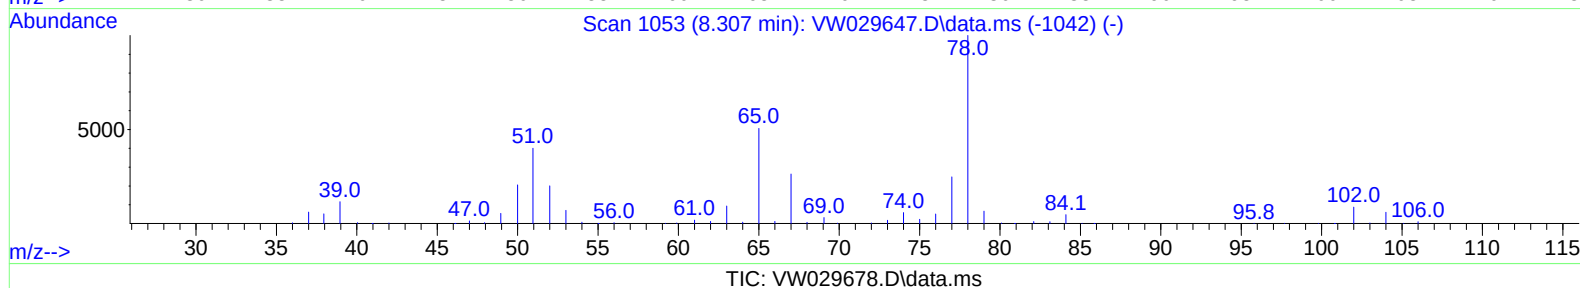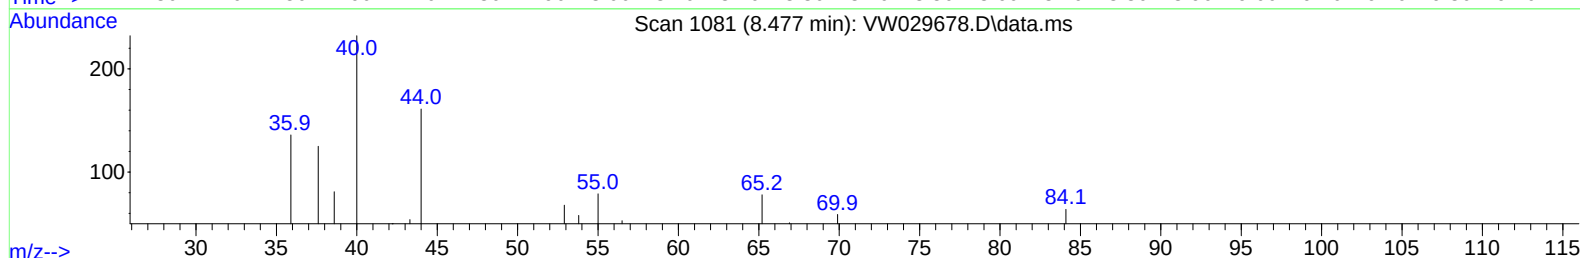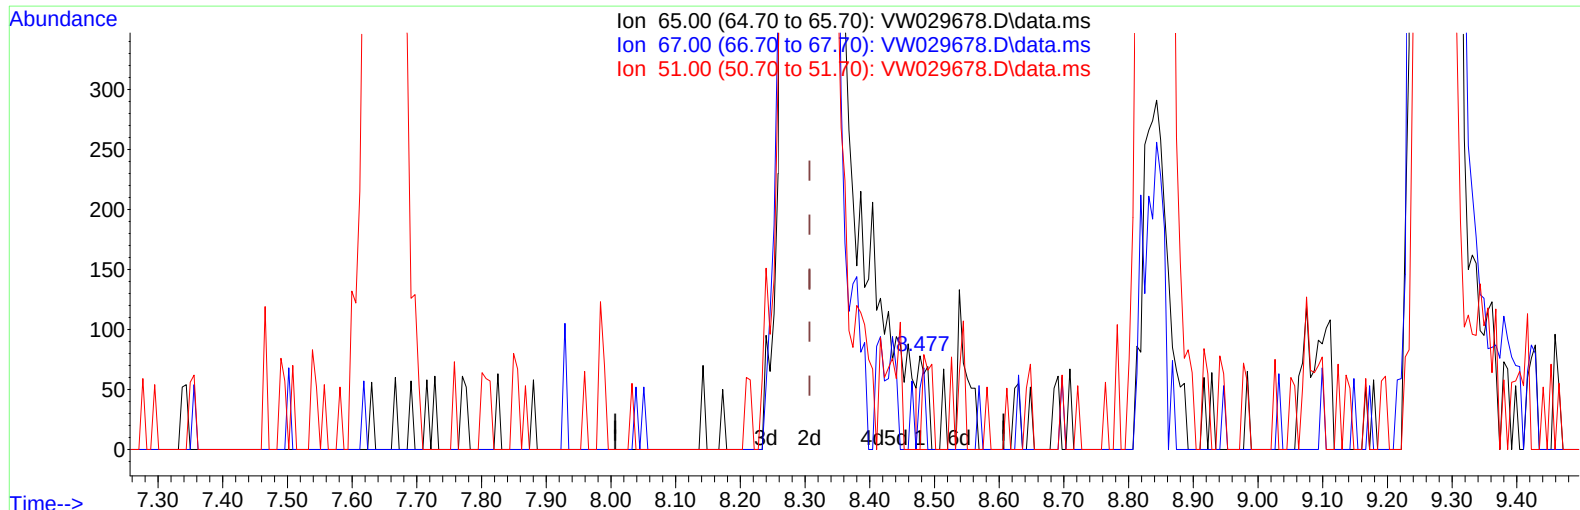

TIC: VW029678.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.477min (+ 0.171) 0.01 ug/L

response 77

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.60	57.14
51.00	101.40	102.60
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072224\
Data File : VW029678.D
Acq On : 22 Jul 2024 13:02
Operator : SY/MD
Sample : P3298-15
Misc : 6.87g/10mL/MSVOA_W/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BHB45

Manual IntegrationsAPPROVED

Quant Time: Jul 22 14:35:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 19 23:16:32 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 07/23/2024
Supervised By :Mahesh Dadoda 07/24/2024

