

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072324\
 Data File : VW029699.D
 Acq On : 23 Jul 2024 12:33
 Operator : SY/MD
 Sample : P3313-01
 Misc : 6.80g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jul 24 01:14:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 24 01:12:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	385640	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	360477	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	163626	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	71672	11.505	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	46.000%
7) Chloroethane-d5	2.899	69	62235	13.874	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.480%
11) 1,1-Dichloroethene-d2	4.015	65	35477	12.682	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.720%
21) 2-Butanone-d5	7.075	46	72291	38.656	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.320%
24) Chloroform-d	7.642	84	199207	17.868	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.480%
26) 1,2-Dichloroethane-d4	8.301	65	124943	19.107	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	76.440%
32) Benzene-d6	8.270	84	355455	16.460	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	65.840%
36) 1,2-Dichloropropane-d6	9.270	67	126795	18.364	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	73.440%
41) Toluene-d8	10.319	98	302843	15.946	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	63.800%
43) trans-1,3-Dichloroprop...	10.575	79	47846	16.364	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.440%
47) 2-Hexanone-d5	10.922	63	53730	42.825	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.640%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	115460	20.596	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.400%
66) 1,2-Dichlorobenzene-d4	13.849	152	115416	20.254	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.000%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3774	0.403	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072324\
Data File : VW029699.D
Acq On : 23 Jul 2024 12:33
Operator : SY/MD
Sample : P3313-01
Misc : 6.80g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jul 24 01:14:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 24 01:12:32 2024
Response via : Initial Calibration

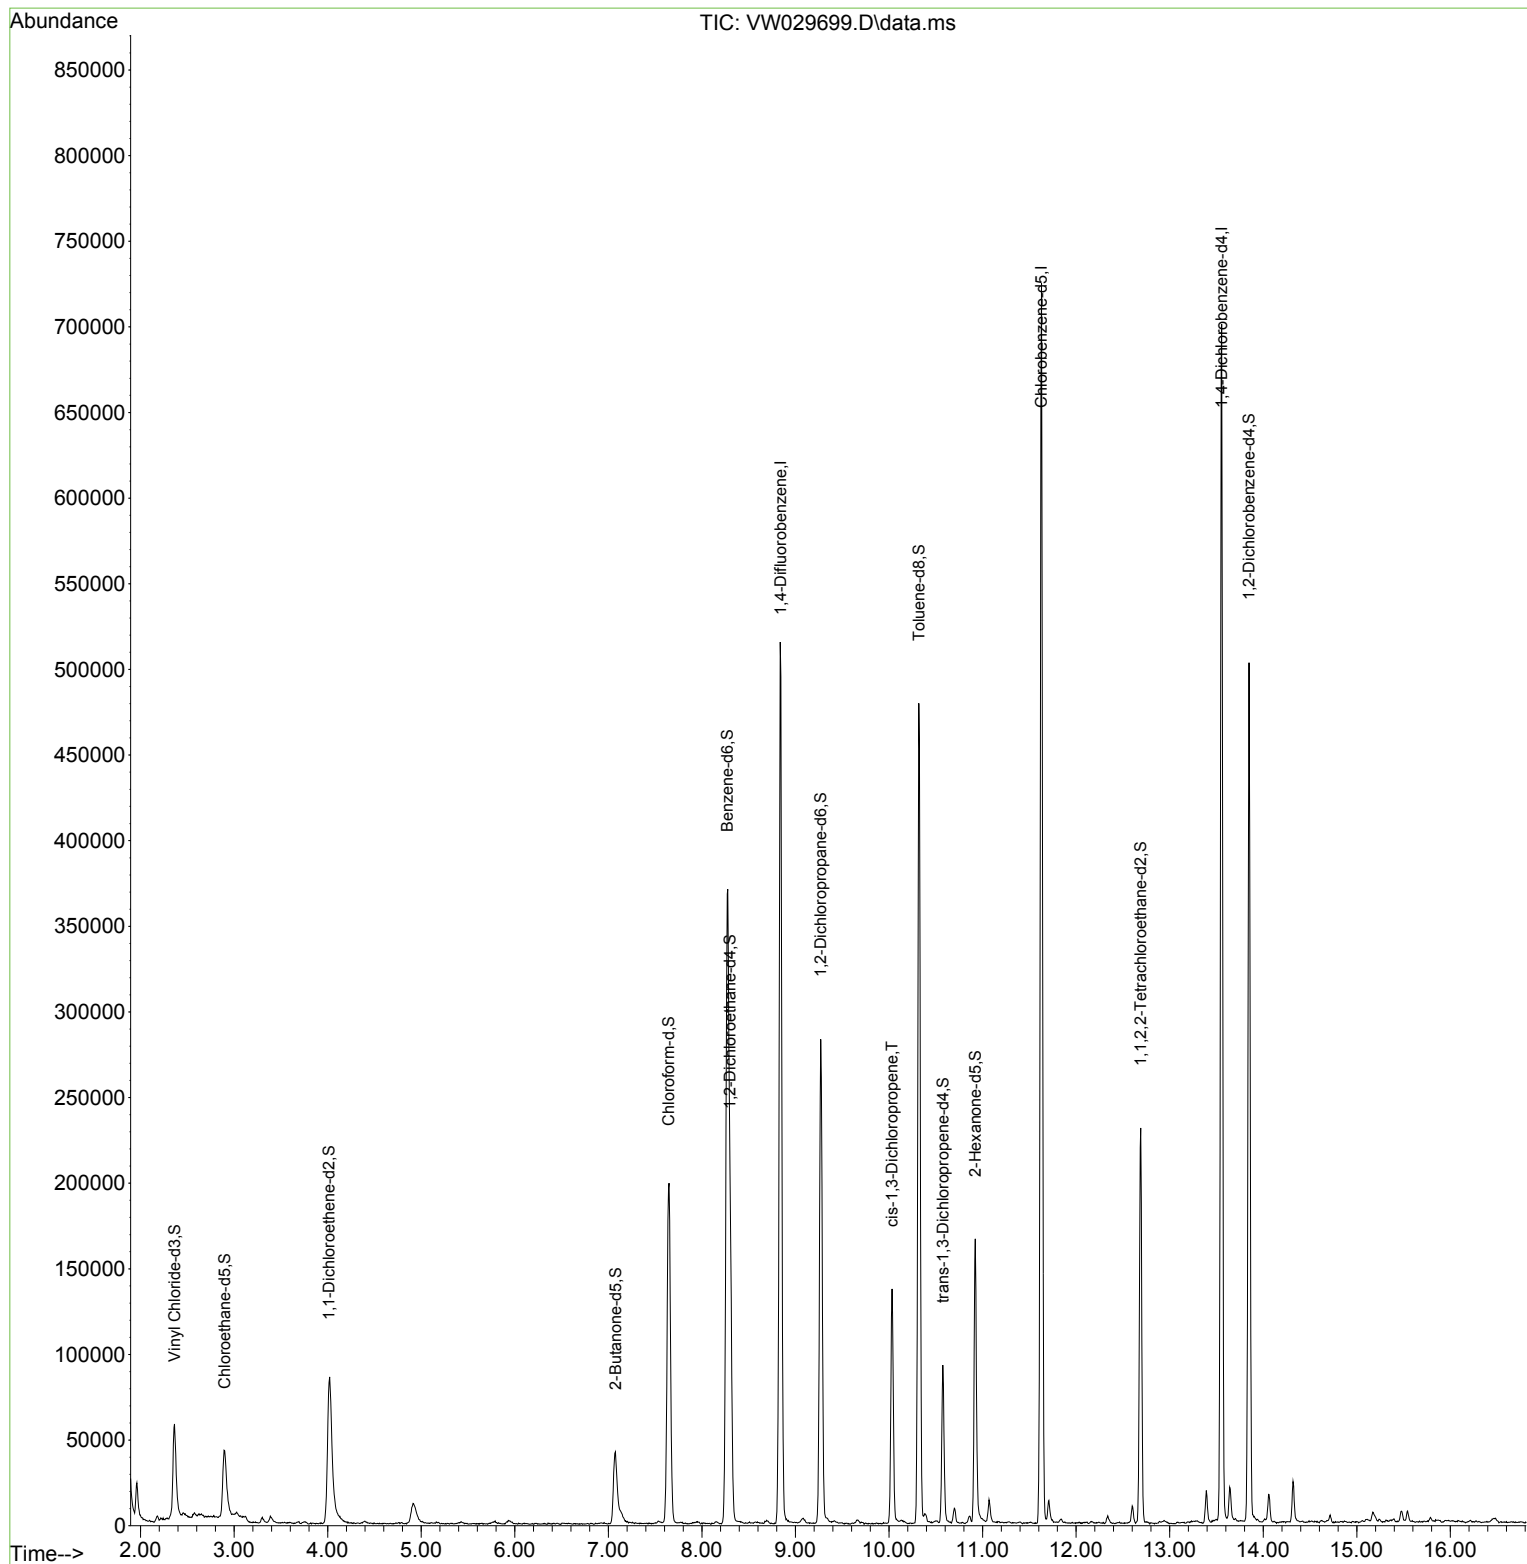

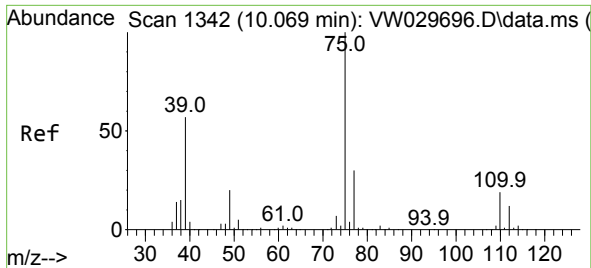

#39
cis-1,3-Dichloropropene
Concen: 0.403 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.037 min
Lab File: VW029699.D
Acq: 23 Jul 2024 12:33

Instrument :
MSVOA_W
ClientSampleId :

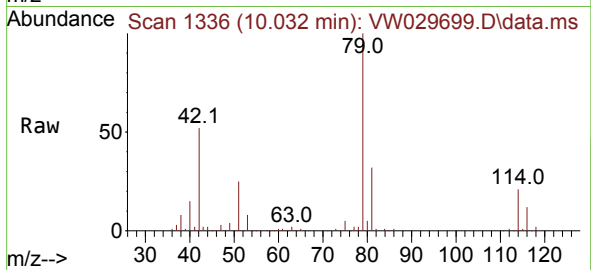

Tgt Ion: 75 Resp: 3774
Ion Ratio Lower Upper
75 100
77 40.3 22.2 41.2

