

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072324\
 Data File : VW029705.D
 Acq On : 23 Jul 2024 15:06
 Operator : SY/MD
 Sample : P3278-22
 Misc : 8.81g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E1ZS2

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

Quant Time: Jul 24 01:16:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 24 01:12:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	140676	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	62438	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	9512	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	44542	19.600	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	78.400%		
7) Chloroethane-d5	2.893	69	37171	22.716	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.880%		
11) 1,1-Dichloroethene-d2	4.021	65	18037	17.675	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	70.720%		
21) 2-Butanone-d5	7.075	46	58175	85.278	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	170.560%#		
24) Chloroform-d	7.648	84	85666	21.064	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.240%		
26) 1,2-Dichloroethane-d4	8.307	65	57608	24.150	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	96.600%		
32) Benzene-d6	8.276	84	136503	36.494	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	145.960%#		
36) 1,2-Dichloropropane-d6	9.270	67	50181	41.960	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	167.840%#		
41) Toluene-d8	10.325	98	65845	20.017	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.080%		
43) trans-1,3-Dichloroprop...	10.575	79	10623	20.976	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.920%		
47) 2-Hexanone-d5	10.922	63	21509	98.976	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	197.960%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	38596	39.749	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	159.000%#		
66) 1,2-Dichlorobenzene-d4	13.848	152	7382	22.285	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.120%		
Target Compounds						
5) Vinyl chloride	2.375	62	6082	2.892	ug/L	96
12) 1,1-Dichloroethene	4.039	96	18092m	10.342	ug/L	
13) Acetone	4.124	43	10053	14.601	ug/L	97
14) Carbon disulfide	4.399	76	6933	1.220	ug/L	97
17) trans-1,2-Dichloroethene	5.429	96	16098	8.312	ug/L	99
19) 1,1-Dichloroethane	6.216	63	236390	59.436	ug/L	98
20) cis-1,2-Dichloroethene	7.167	96	2170280	1024.808	ug/L	94
27) 1,2-Dichloroethane	8.404	62	3455	1.197	ug/L	97
34) Trichloroethene	9.093	95	106185	102.930	ug/L	98
46) Tetrachloroethene	10.855	164	470	0.641	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072324\
Data File : VW029705.D
Acq On : 23 Jul 2024 15:06
Operator : SY/MD
Sample : P3278-22
Misc : 8.81g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
E1ZS2

Quant Time: Jul 24 01:16:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 24 01:12:32 2024
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

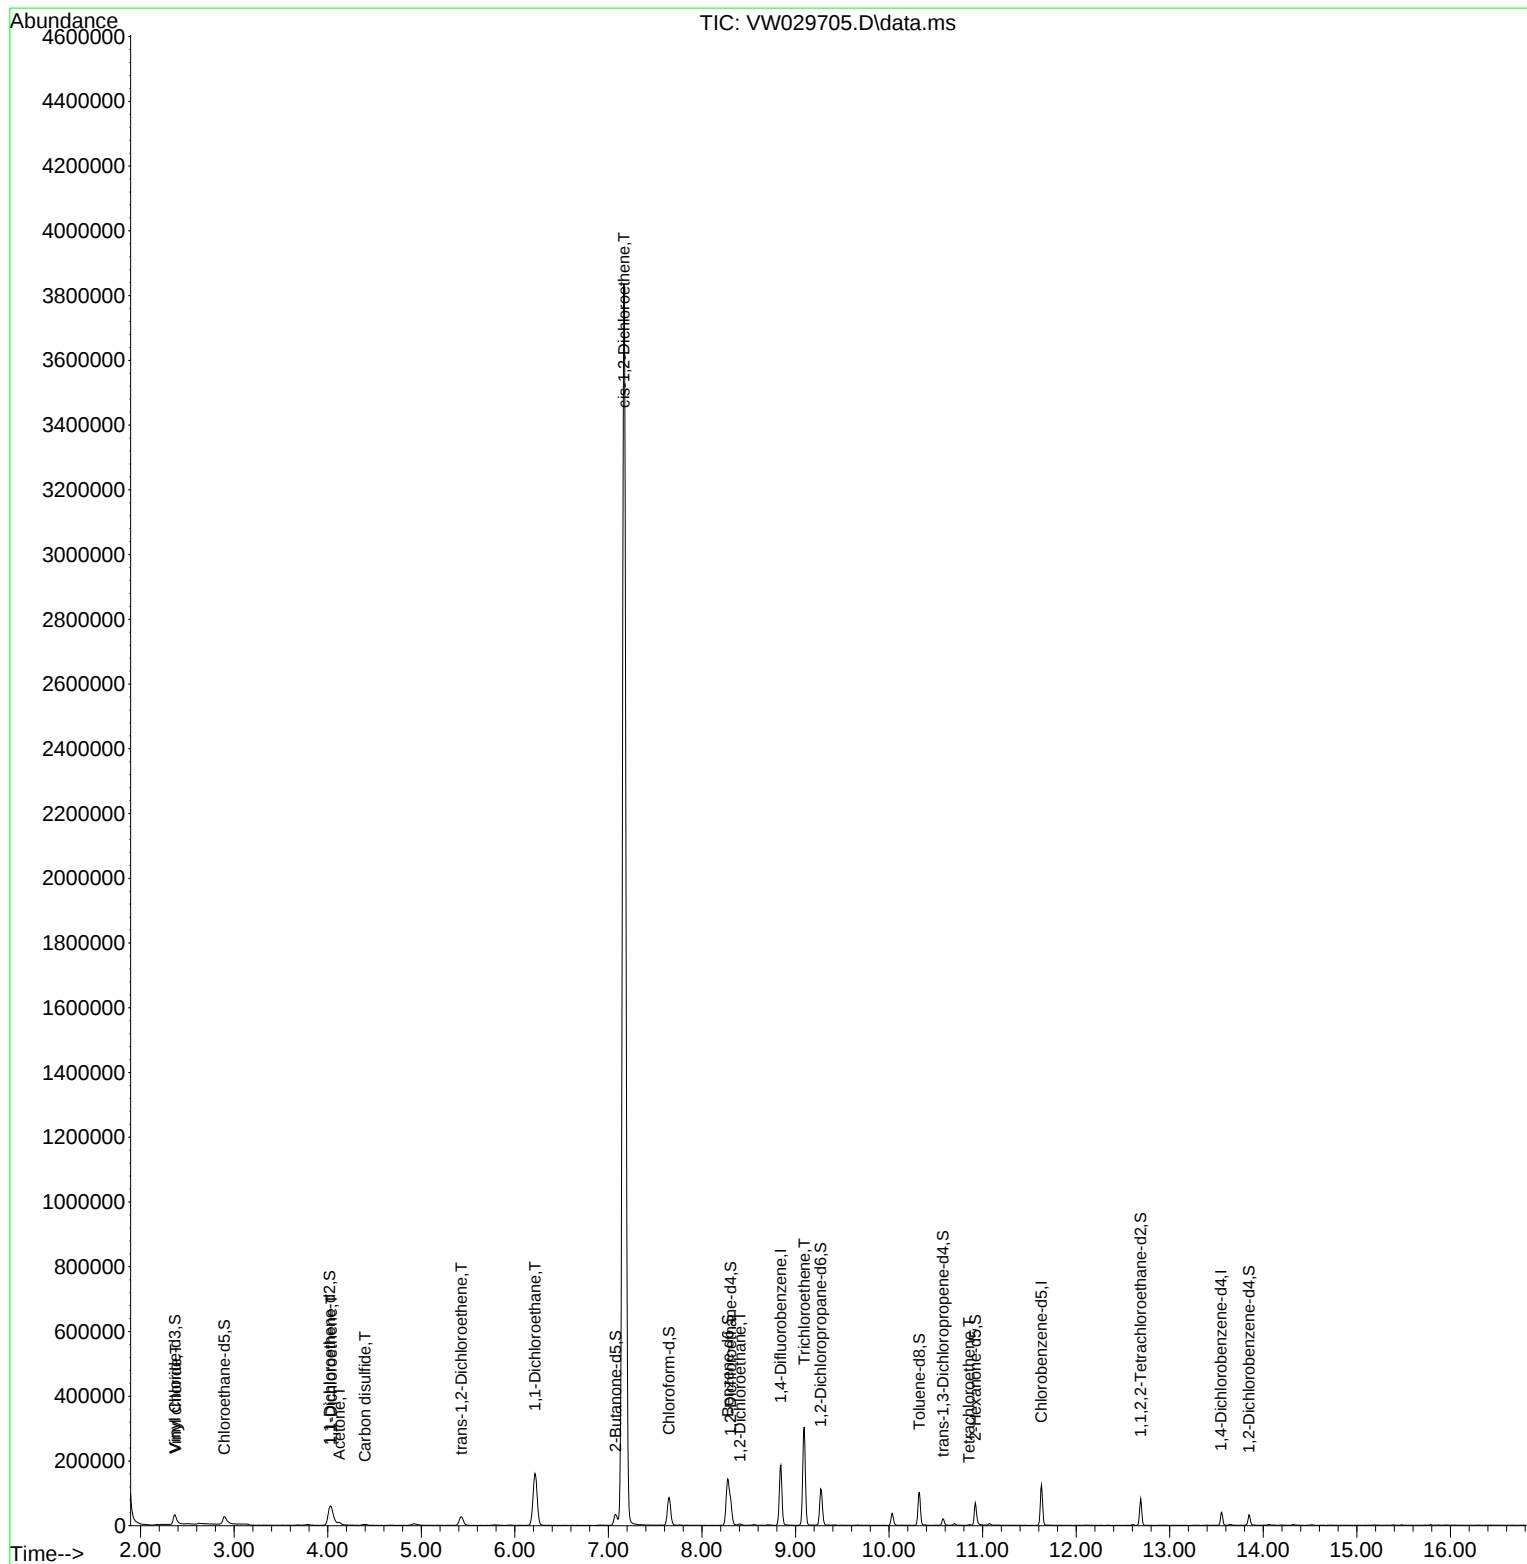

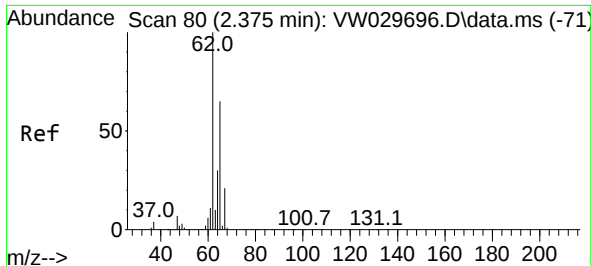





#5
 Vinyl chloride
 Concen: 2.892 ug/L
 RT: 2.375 min Scan# 80
 Delta R.T. -0.000 min
 Lab File: VW029705.D
 Acq: 23 Jul 2024 15:06

Instrument :
 MSVOA_W
 ClientSampleId :
 E1ZS2

Tgt Ion: 62 Resp: 608
 Ion Ratio Lower Upper
 62 100
 64 38.1 25.1 46.5




Manual Integrations
 APPROVED


Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

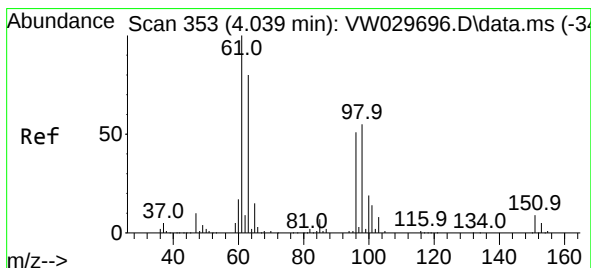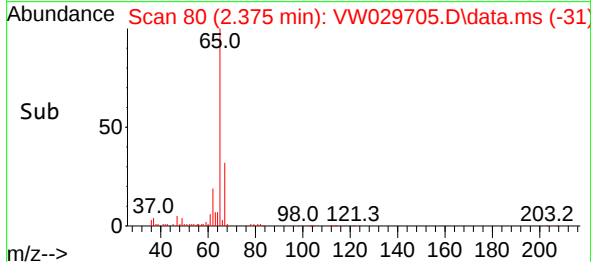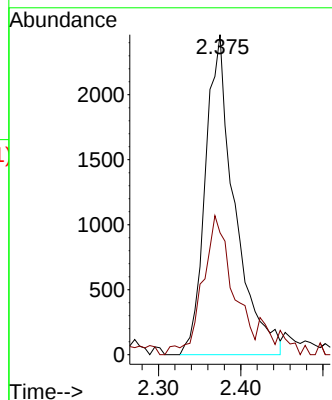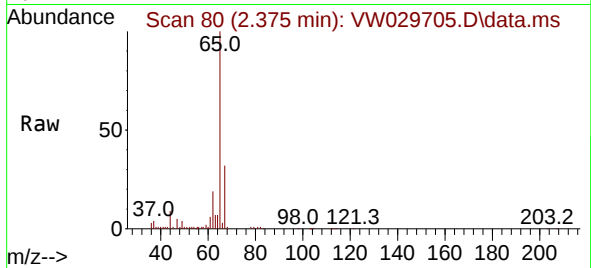

#12
 1,1-Dichloroethene
 Concen: 10.342 ug/L m
 RT: 4.039 min Scan# 353
 Delta R.T. -0.000 min
 Lab File: VW029705.D
 Acq: 23 Jul 2024 15:06


Tgt Ion: 96 Resp: 18092
 Ion Ratio Lower Upper
 96 100
 61 205.3 132.4 245.8
 63 268.5 108.4 201.2#

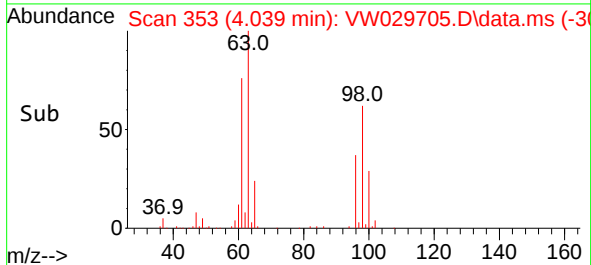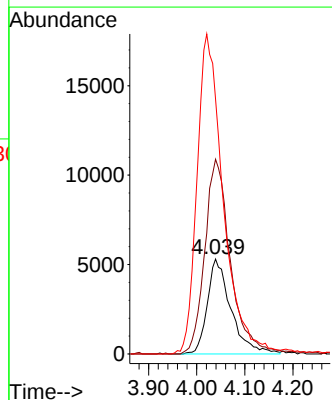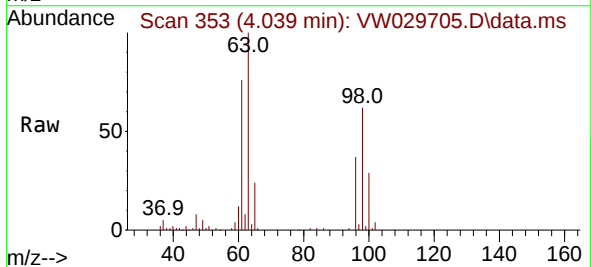

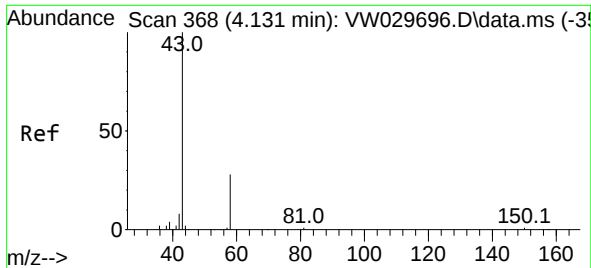

#13
Acetone
Concen: 14.601 ug/L
RT: 4.124 min Scan# 367
Delta R.T. -0.006 min
Lab File: VW029705.D
Acq: 23 Jul 2024 15:06




Instrument :
MSVOA_W
ClientSampleId :
E1ZS2

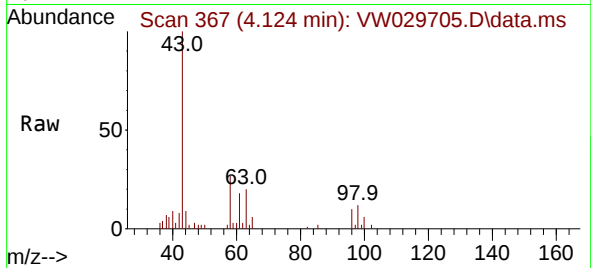

Tgt Ion: 43 Resp: 1005
Ion Ratio Lower Upper
43 100
58 29.6 0.0 55.6




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

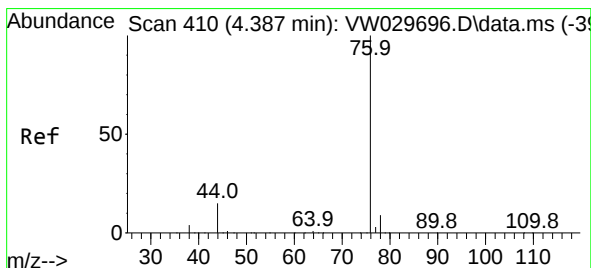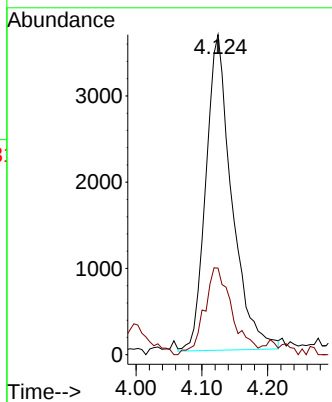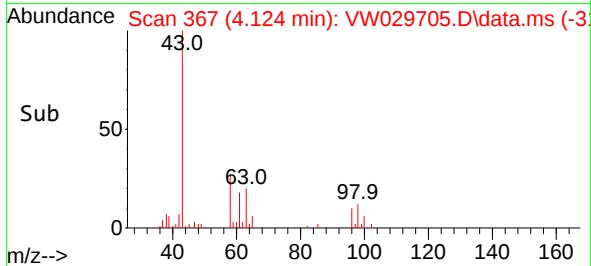

#14
Carbon disulfide
Concen: 1.220 ug/L
RT: 4.399 min Scan# 412
Delta R.T. 0.012 min
Lab File: VW029705.D
Acq: 23 Jul 2024 15:06


Tgt Ion: 76 Resp: 6933
Ion Ratio Lower Upper
76 100
78 9.7 7.0 10.4

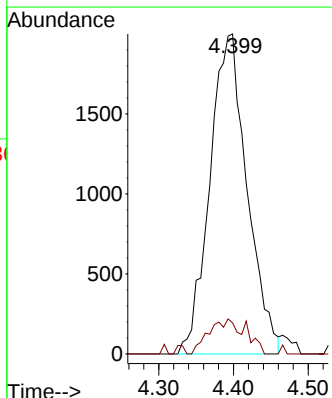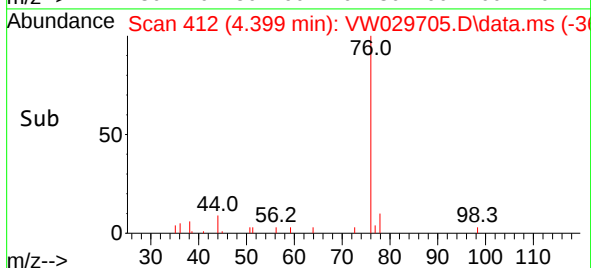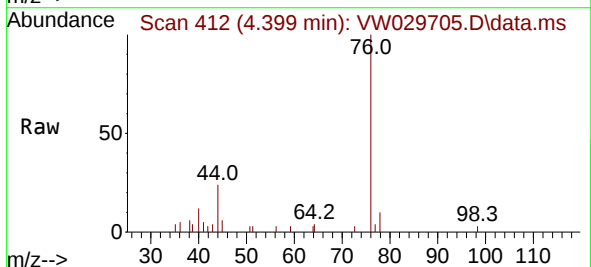

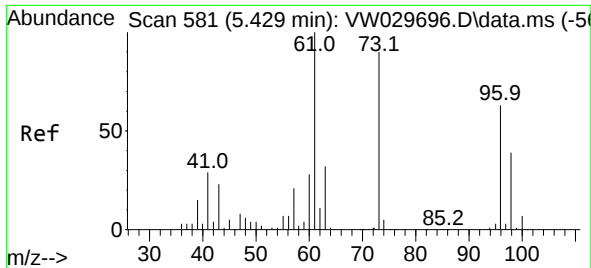

#17
trans-1,2-Dichloroethene
Concen: 8.312 ug/L
RT: 5.429 min Scan# 581
Delta R.T. -0.000 min
Lab File: VW029705.D
Acq: 23 Jul 2024 15:06




Instrument :
MSVOA_W
ClientSampleId :
E1ZS2

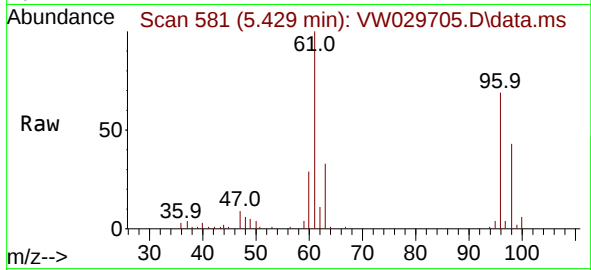


Tgt Ion: 96 Resp: 16098
Ion Ratio Lower Upper
96 100
61 144.5 102.9 191.1
98 62.8 43.9 81.5

Manual Integrations
APPROVED



Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

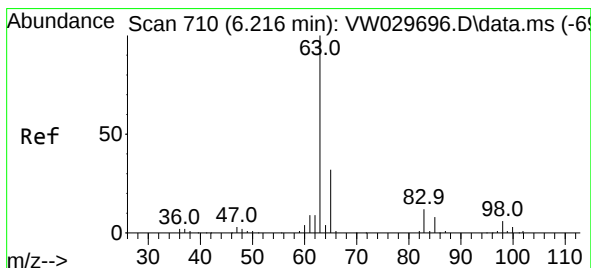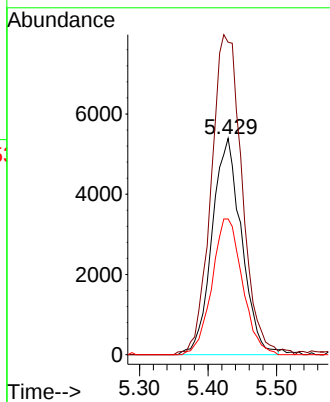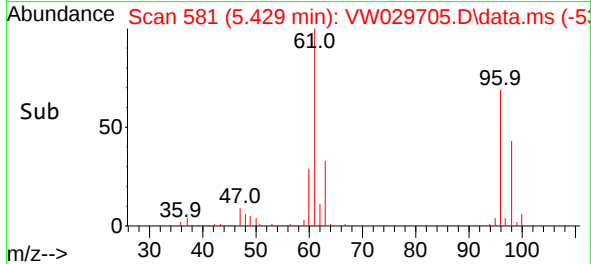


#19
1,1-Dichloroethane
Concen: 59.436 ug/L
RT: 6.216 min Scan# 710
Delta R.T. -0.000 min
Lab File: VW029705.D
Acq: 23 Jul 2024 15:06

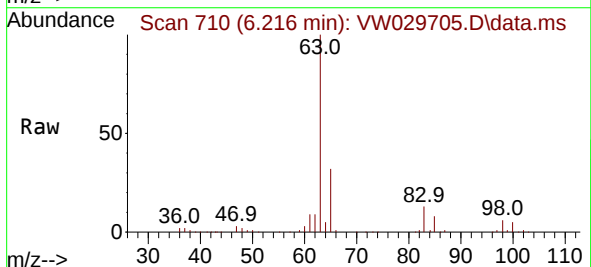


Tgt Ion: 63 Resp: 236390
Ion Ratio Lower Upper
63 100
65 32.2 21.5 39.9
83 12.9 8.7 16.1

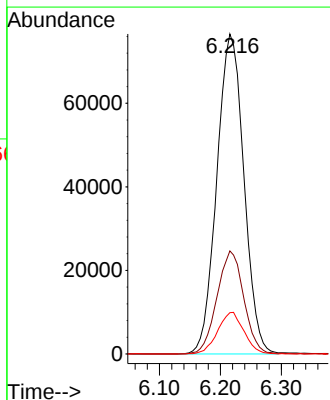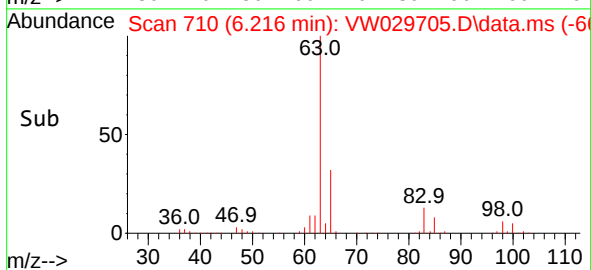

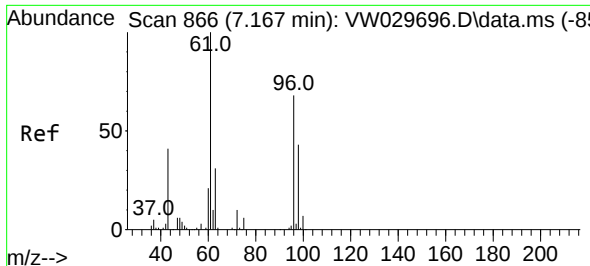

#20
 cis-1,2-Dichloroethene
 Concen: 1024.808 ug/L
 RT: 7.167 min Scan# 866
 Delta R.T. -0.000 min
 Lab File: VW029705.D
 Acq: 23 Jul 2024 15:06




Instrument :
 MSVOA_W
 ClientSampleId :
 E1ZS2

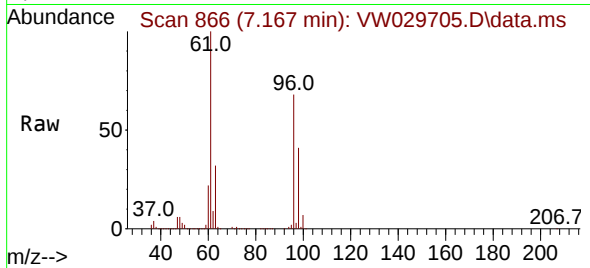


Tgt Ion: 96 Resp: 2170280
 Ion Ratio Lower Upper
 96 100
 61 147.8 97.4 180.8
 98 60.8 41.6 77.2

Manual Integrations
 APPROVED



Reviewed By :Mahesh Dadoda 07/24/2024
 Supervised By :Semsettin Yesilyurt 07/24/2024

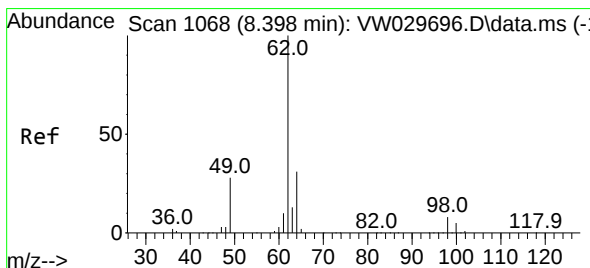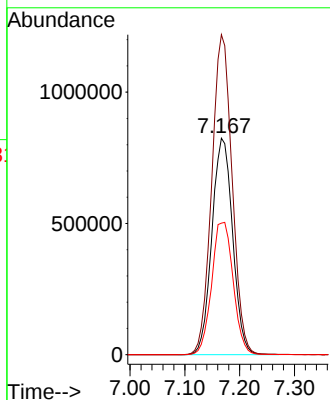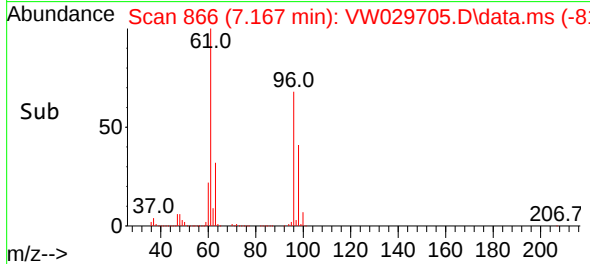


#27
 1,2-Dichloroethane
 Concen: 1.197 ug/L
 RT: 8.404 min Scan# 1069
 Delta R.T. 0.006 min
 Lab File: VW029705.D
 Acq: 23 Jul 2024 15:06

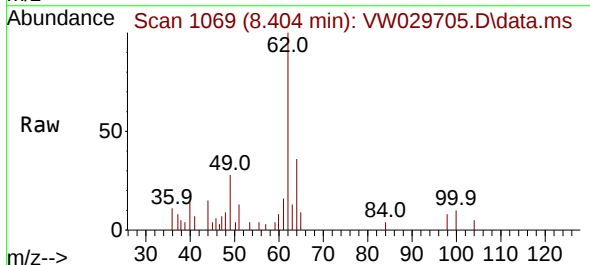


Tgt Ion: 62 Resp: 3455
 Ion Ratio Lower Upper
 62 100
 98 8.4 6.0 9.0

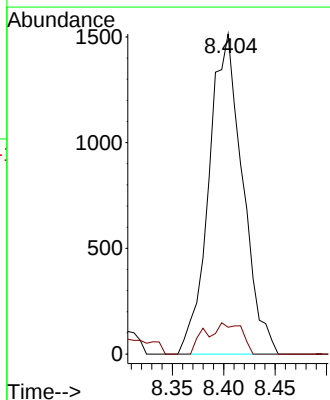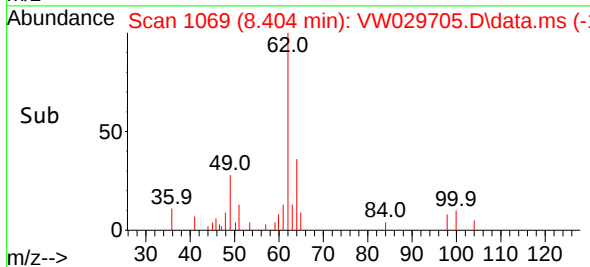

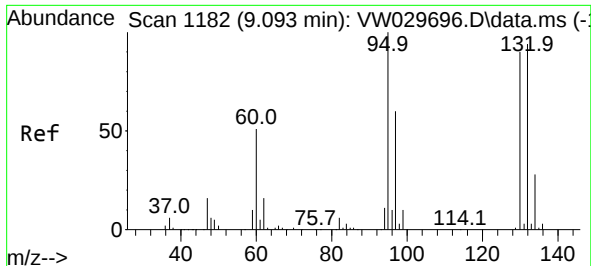

#34
Trichloroethene
Concen: 102.930 ug/L
RT: 9.093 min Scan# 1182
Delta R.T. -0.000 min
Lab File: VW029705.D
Acq: 23 Jul 2024 15:06




Instrument :
MSVOA_W
ClientSampleId :
E1ZS2

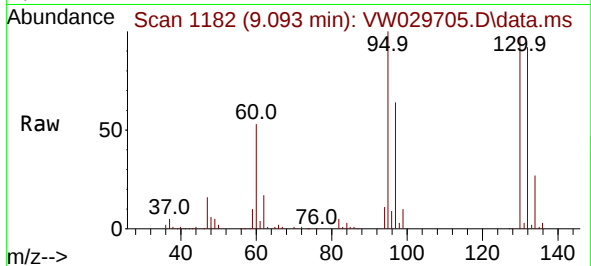


Tgt Ion: 95 Resp: 10618
Ion Ratio Lower Upper
95 100
97 64.3 47.3 87.9
132 91.9 65.8 122.2
130 97.1 67.8 125.8

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/24/2024
Supervised By :Semsettin Yesilyurt 07/24/2024

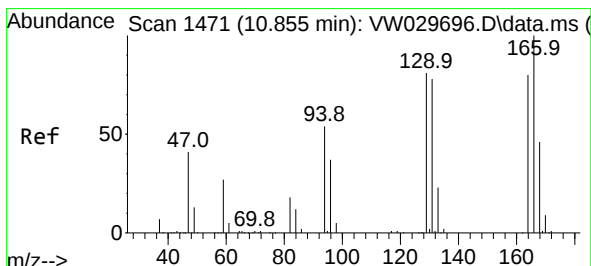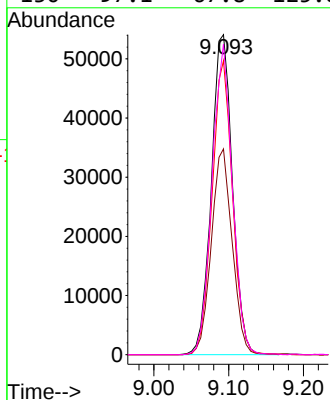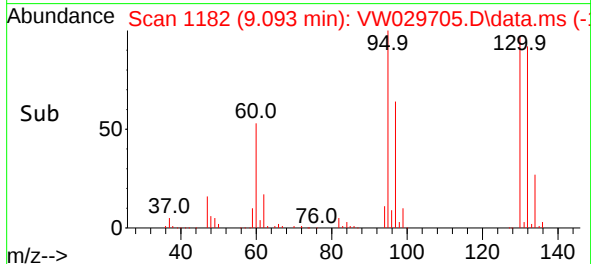

#46
Tetrachloroethene
Concen: 0.641 ug/L
RT: 10.855 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VW029705.D
Acq: 23 Jul 2024 15:06

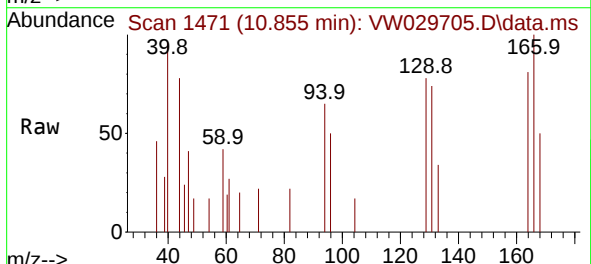

Tgt Ion:164 Resp: 470
Ion Ratio Lower Upper
164 100
129 96.4 60.0 111.4
131 92.0 64.6 120.0
166 124.1 80.4 149.2

