

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072324\
 Data File : VW029707.D
 Acq On : 23 Jul 2024 15:54
 Operator : SY/MD
 Sample : P3278-15
 Misc : 8.77g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E1ZR7

Quant Time: Jul 24 01:16:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jul 24 01:12:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	230098	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	214713	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	95341	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	64451	17.339	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.360%
7) Chloroethane-d5	2.899	69	54693	20.435	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.720%
11) 1,1-Dichloroethene-d2	4.027	65	32327	19.367	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	77.480%
21) 2-Butanone-d5	7.075	46	40209	36.035	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.080%
24) Chloroform-d	7.648	84	152832	22.975	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.920%
26) 1,2-Dichloroethane-d4	8.307	65	88744	22.745	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.000%
32) Benzene-d6	8.276	84	283051	22.006	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.040%
36) 1,2-Dichloropropane-d6	9.276	67	95558	23.235	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.960%
41) Toluene-d8	10.325	98	242530	21.440	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.760%
43) trans-1,3-Dichloroprop...	10.575	79	32402	18.605	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.440%
47) 2-Hexanone-d5	10.922	63	25076	33.555	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	67.120%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	68499	20.514	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.040%
66) 1,2-Dichlorobenzene-d4	13.848	152	80746	24.319	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.280%
Target Compounds						
16) Methylene chloride	4.923	84	12925	3.138	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072324\
Data File : VW029707.D
Acq On : 23 Jul 2024 15:54
Operator : SY/MD
Sample : P3278-15
Misc : 8.77g/10mL/MSVOA_W/SOIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1ZR7


Quant Time: Jul 24 01:16:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jul 24 01:12:32 2024
Response via : Initial Calibration

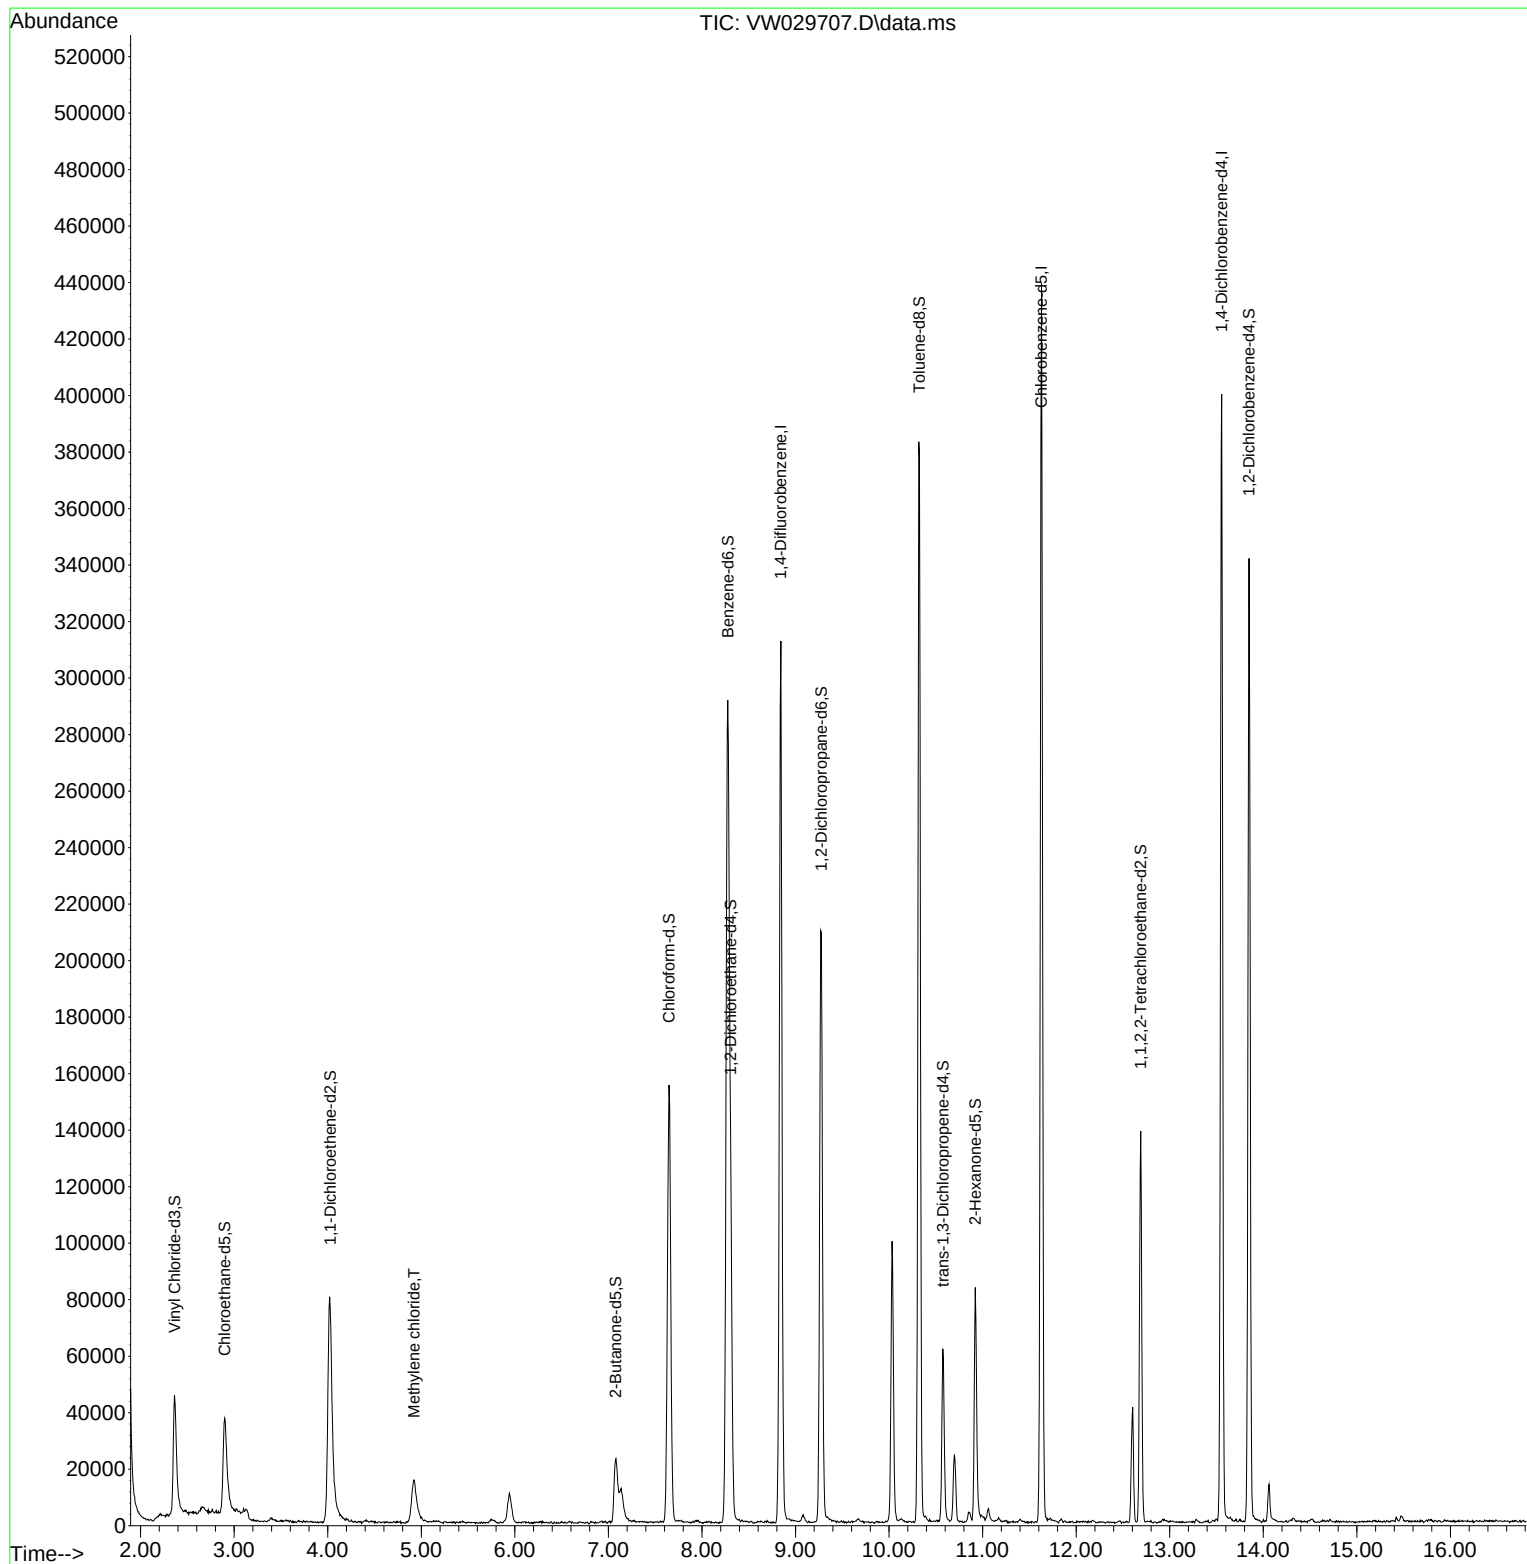

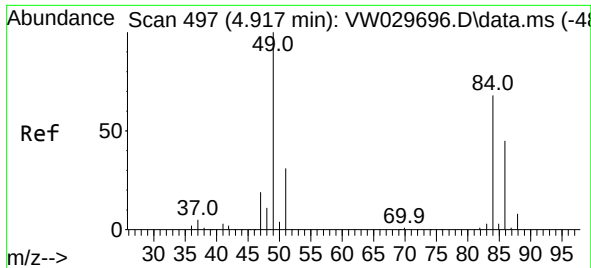

#16
Methylene chloride
Concen: 3.138 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW029707.D
Acq: 23 Jul 2024 15:54

Instrument :
MSVOA_W
ClientSampleId :
E1ZR7

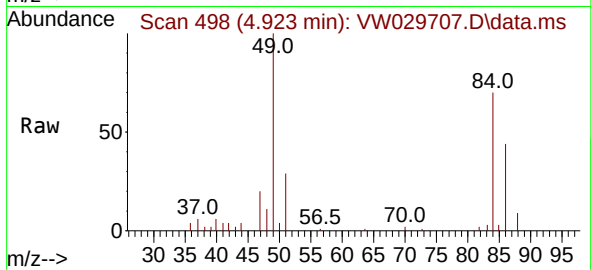

Tgt Ion: 84 Resp: 12925

Ion	Ratio	Lower	Upper
84	100		
86	63.6	46.2	85.8
49	143.2	96.7	179.7

