
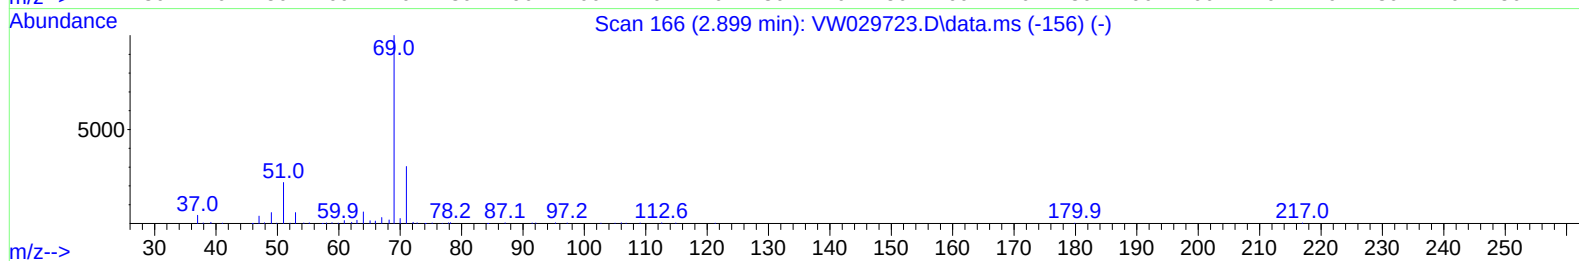
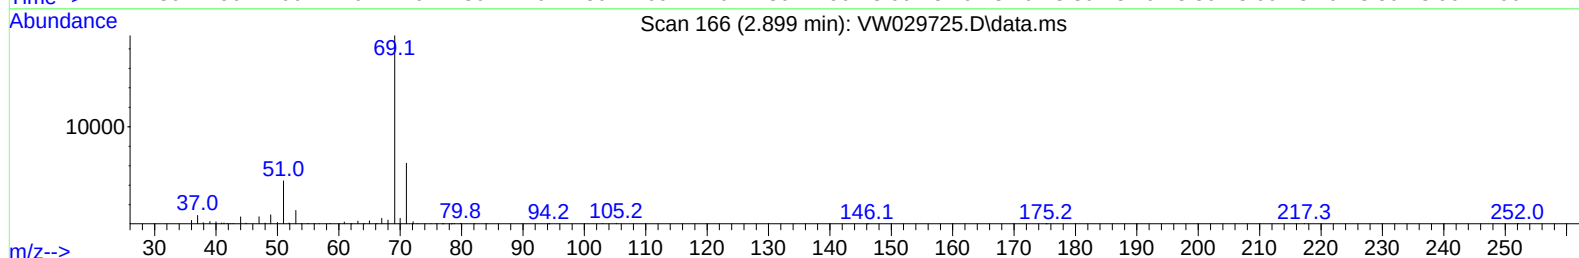


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029725.D
Acq On : 25 Jul 2024 10:37
Operator : SY/MD
Sample : P3313-03
Misc : 5.07g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Jul 26 01:27:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

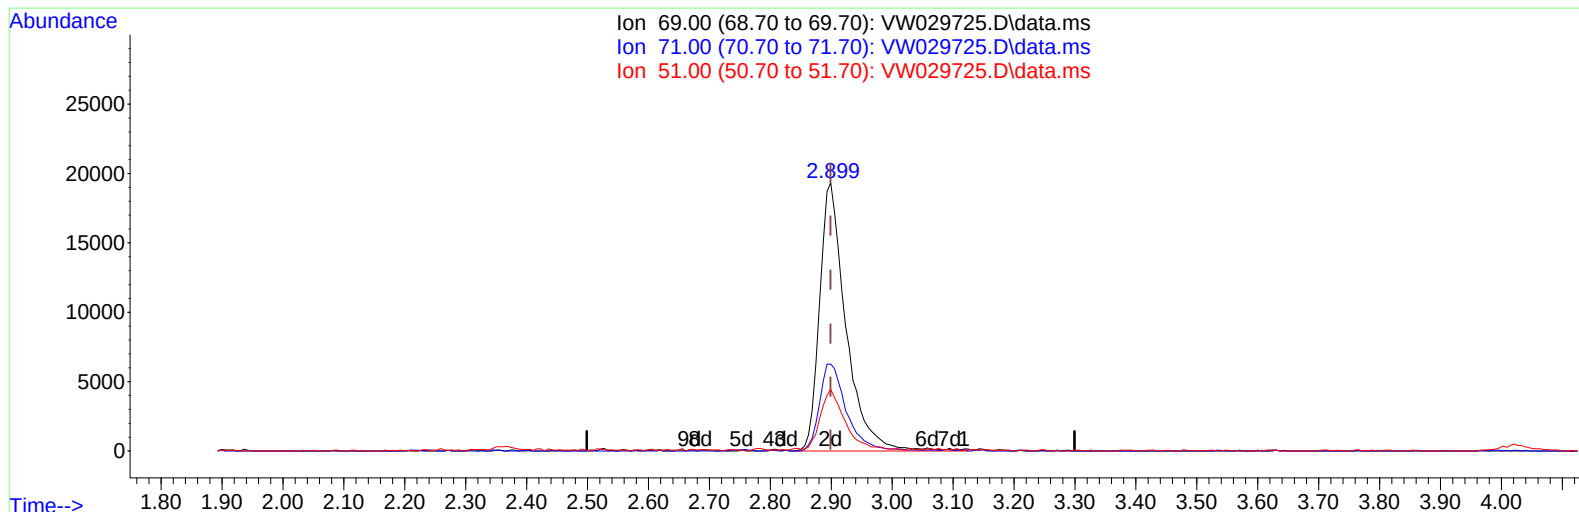

TIC: VW029725.D\data.ms

(7) Chloroethane-d5 (S)




2.899min (+ 0.000) 21.98 ug/L m

response 58269

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.70	0.09#
51.00	31.60	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029725.D
Acq On : 25 Jul 2024 10:37
Operator : SY/MD
Sample : P3313-03
Misc : 5.07g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Jul 26 01:27:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

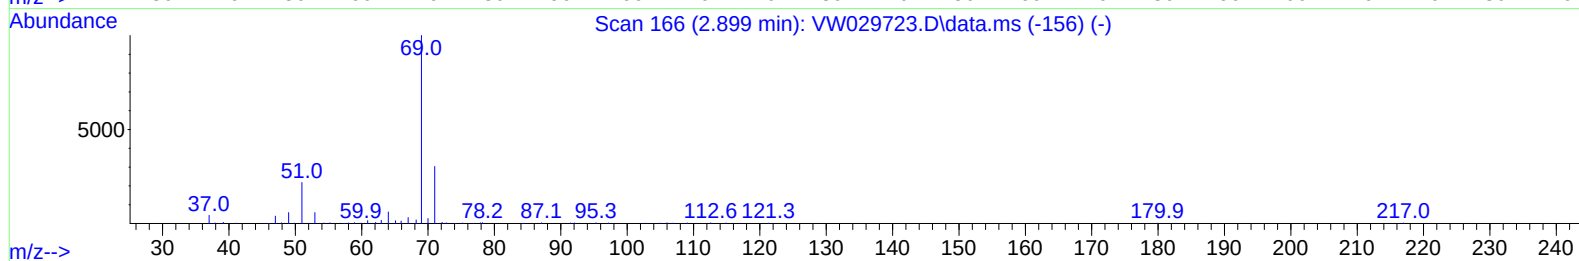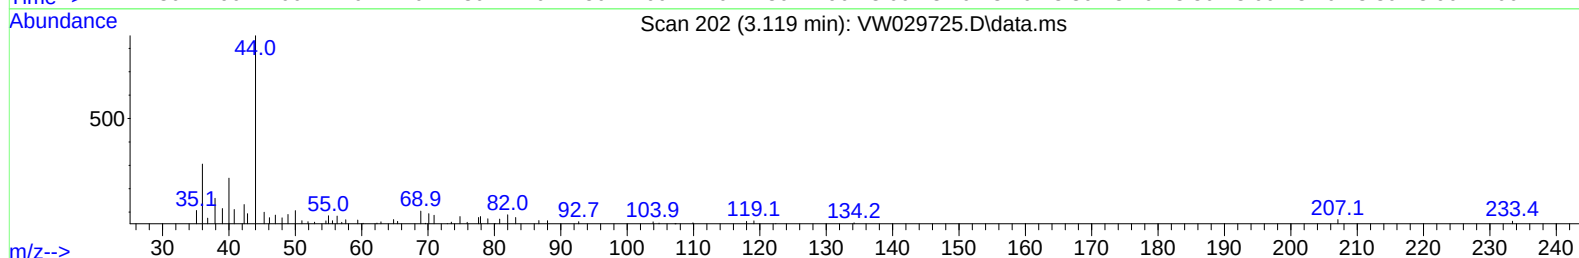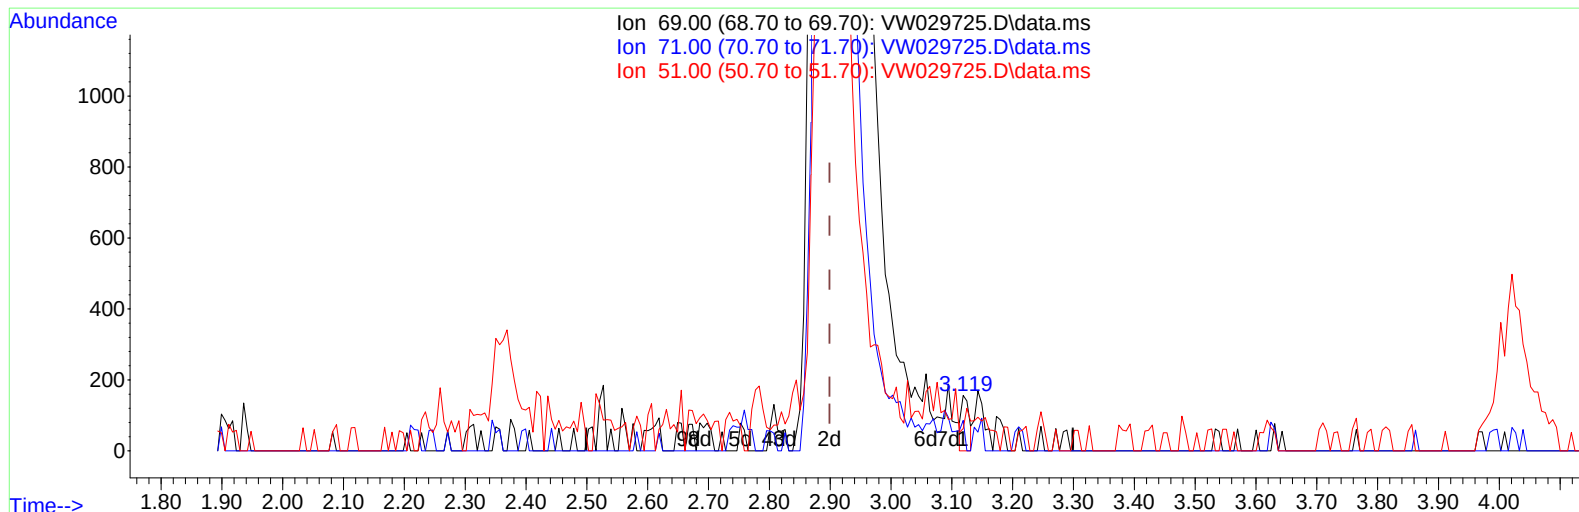

TIC: VW029725.D\data.ms

(7) Chloroethane-d5 (S)

3.119min (+ 0.220) 0.05 ug/L

response	134	
Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.70	38.81
51.00	31.60	30.60
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
 Data File : VW029725.D
 Acq On : 25 Jul 2024 10:37
 Operator : SY/MD
 Sample : P3313-03
 Misc : 5.07g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Jul 26 01:27:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 25 01:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	261614	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	237860	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	103877	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	78019	21.006	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.040%
7) Chloroethane-d5	2.899	69	58269m	21.975	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.920%
11) 1,1-Dichloroethene-d2	4.015	65	37163	21.920	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	87.680%
21) 2-Butanone-d5	7.081	46	37928	37.259	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.520%
24) Chloroform-d	7.648	84	155166	22.912	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.640%
26) 1,2-Dichloroethane-d4	8.307	65	89906	23.308	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.240%
32) Benzene-d6	8.270	84	307080	23.894	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.560%
36) 1,2-Dichloropropane-d6	9.270	67	97592	23.781	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.120%
41) Toluene-d8	10.318	98	274265	24.000	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.000%
43) trans-1,3-Dichloroprop...	10.575	79	36957	22.256	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.040%
47) 2-Hexanone-d5	10.922	63	25148	37.164	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.320%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	65460	21.483	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.920%
66) 1,2-Dichlorobenzene-d4	13.854	152	79837	24.752	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.000%
Target Compounds						
16) Methylene chloride	4.917	84	18731	3.425	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029725.D
Acq On : 25 Jul 2024 10:37
Operator : SY/MD
Sample : P3313-03
Misc : 5.07g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Jul 26 01:27:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

