
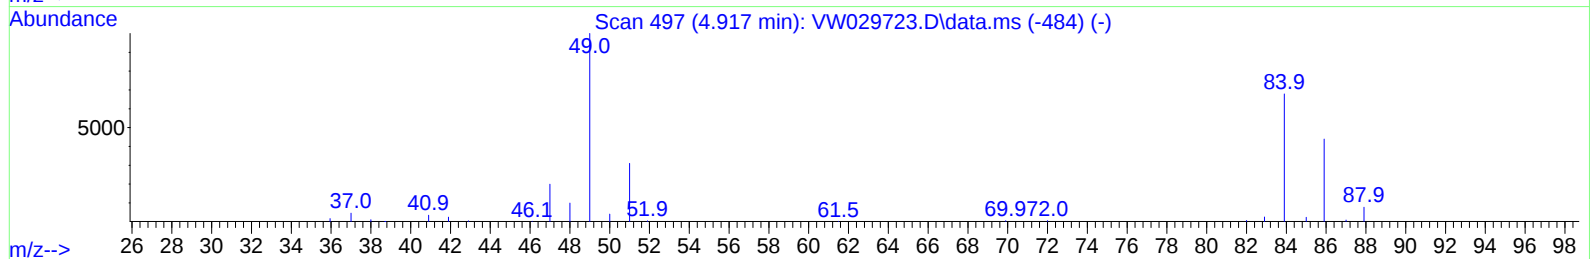
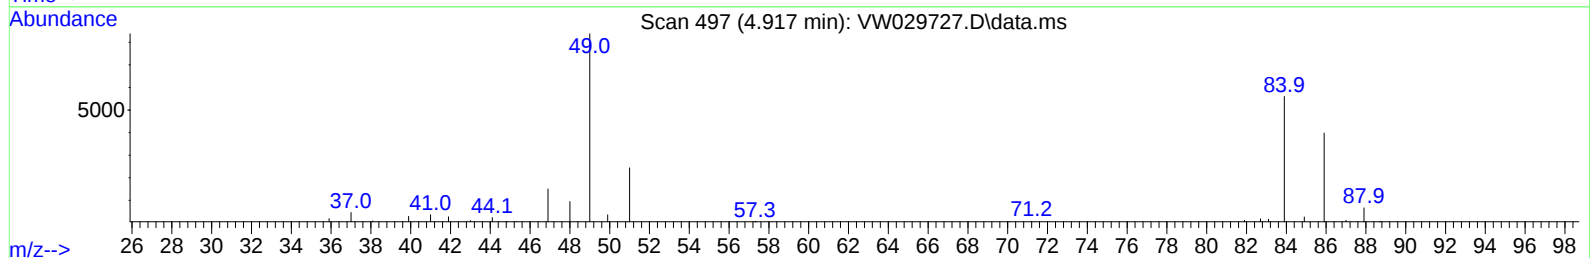


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029727.D
Acq On : 25 Jul 2024 11:25
Operator : SY/MD
Sample : P3278-03
Misc : 9.17g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jul 26 01:28:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

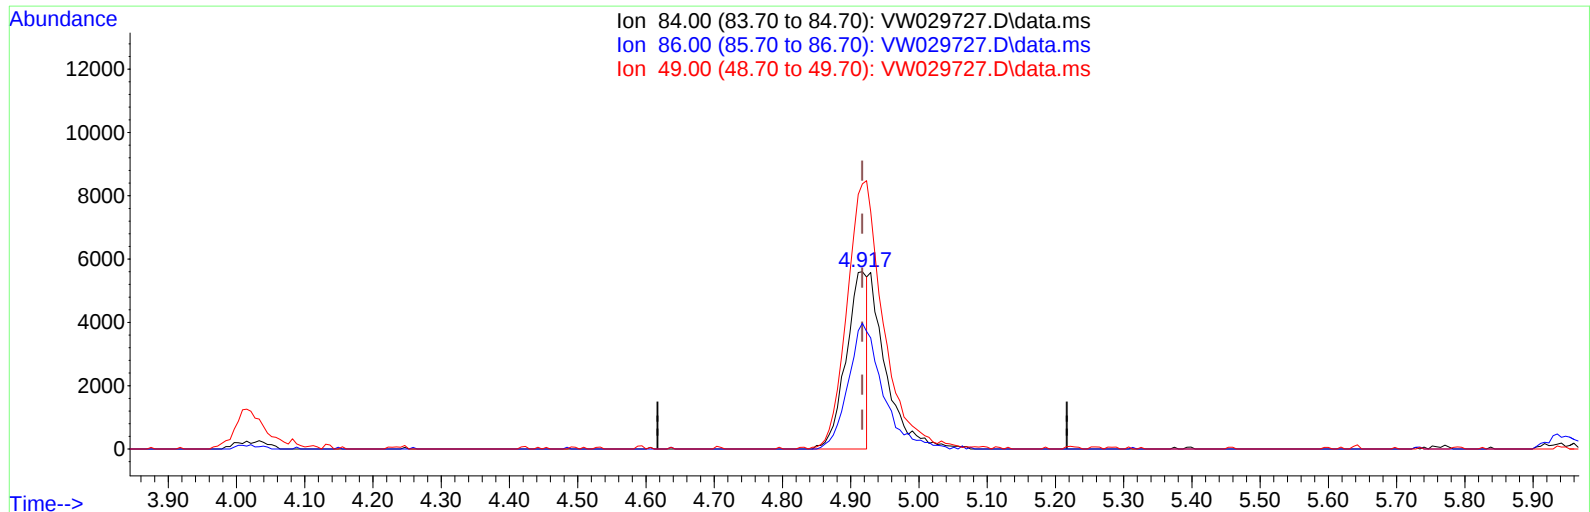

TIC: VW029727.D\data.ms

(16) Methylene chloride (T)




4.917min (+ 0.000) 2.17 ug/L

response 12091

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.80	70.94
49.00	141.50	149.55
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029727.D
Acq On : 25 Jul 2024 11:25
Operator : SY/MD
Sample : P3278-03
Misc : 9.17g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jul 26 01:28:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

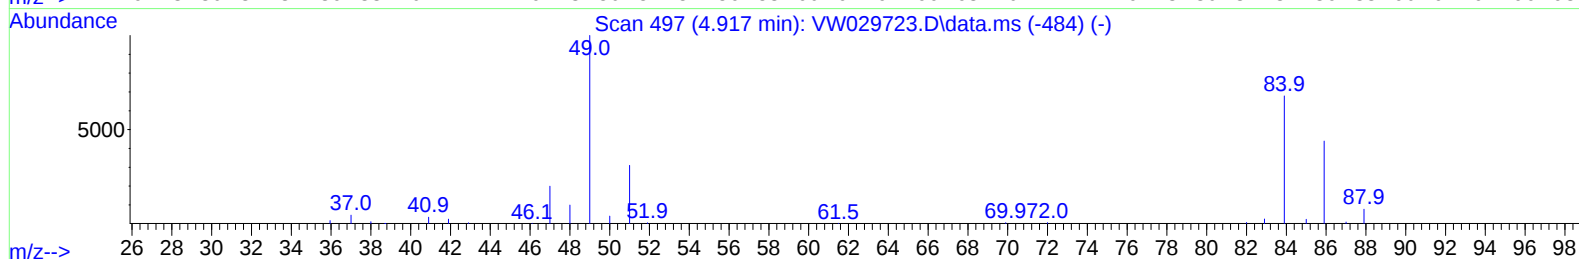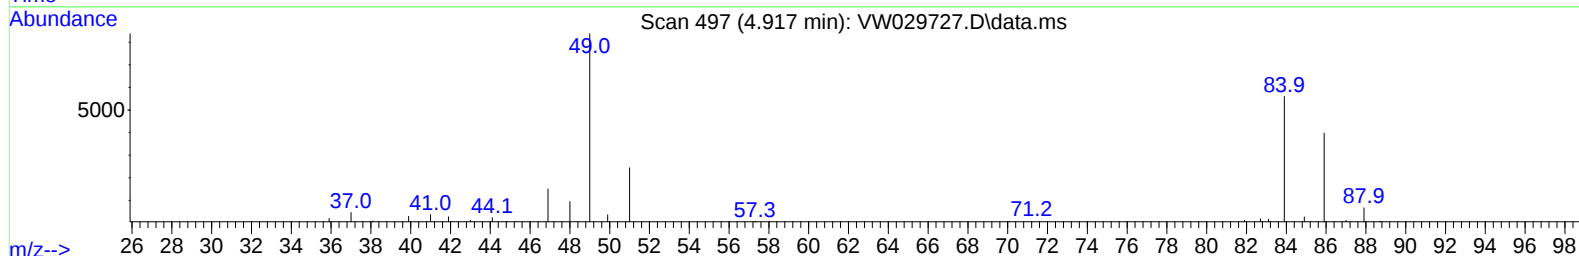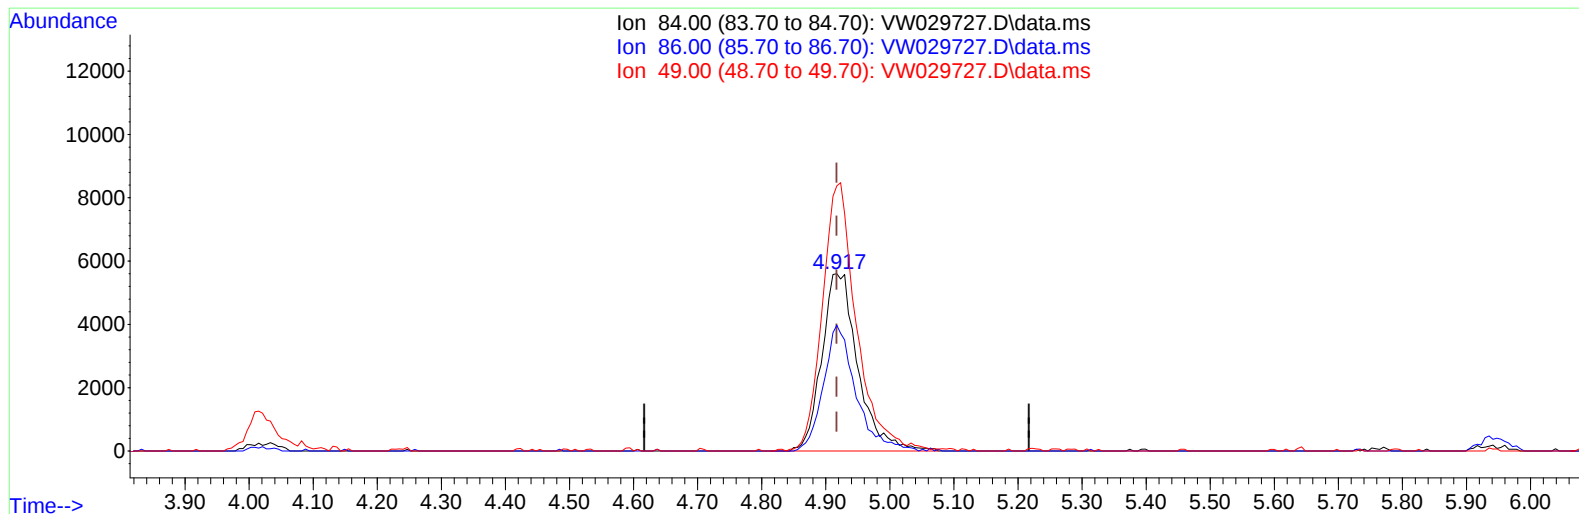

TIC: VW029727.D\data.ms

(16) Methylene chloride (T)

4.917min (+ 0.000) 3.95 ug/L m

response 21967

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.80	70.94
49.00	141.50	149.55
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
 Data File : VW029727.D
 Acq On : 25 Jul 2024 11:25
 Operator : SY/MD
 Sample : P3278-03
 Misc : 9.17g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jul 26 01:28:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 25 01:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	265962	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	242856	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	109264	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	81671	21.630	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.520%
7) Chloroethane-d5	2.893	69	62665	23.247	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.000%
11) 1,1-Dichloroethene-d2	4.021	65	39814	23.100	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	92.400%
21) 2-Butanone-d5	7.081	46	51350	49.619	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.240%
24) Chloroform-d	7.648	84	176235	25.598	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.400%
26) 1,2-Dichloroethane-d4	8.307	65	107645	27.450	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.800%
32) Benzene-d6	8.276	84	347698	26.497	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	106.000%
36) 1,2-Dichloropropane-d6	9.270	67	111667	26.651	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.600%
41) Toluene-d8	10.325	98	312383	26.774	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	107.080%
43) trans-1,3-Dichloroprop...	10.575	79	44286	26.121	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	104.480%
47) 2-Hexanone-d5	10.922	63	34043	49.275	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.540%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	82324	26.461	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.840%
66) 1,2-Dichlorobenzene-d4	13.848	152	91965	27.107	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.440%
Target Compounds						
16) Methylene chloride	4.917	84	21967m	3.951	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029727.D
Acq On : 25 Jul 2024 11:25
Operator : SY/MD
Sample : P3278-03
Misc : 9.17g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jul 26 01:28:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

