
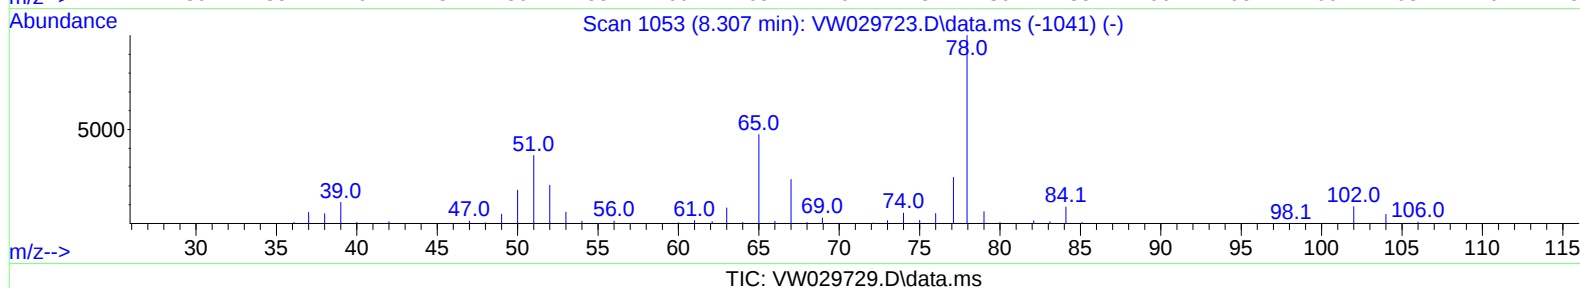
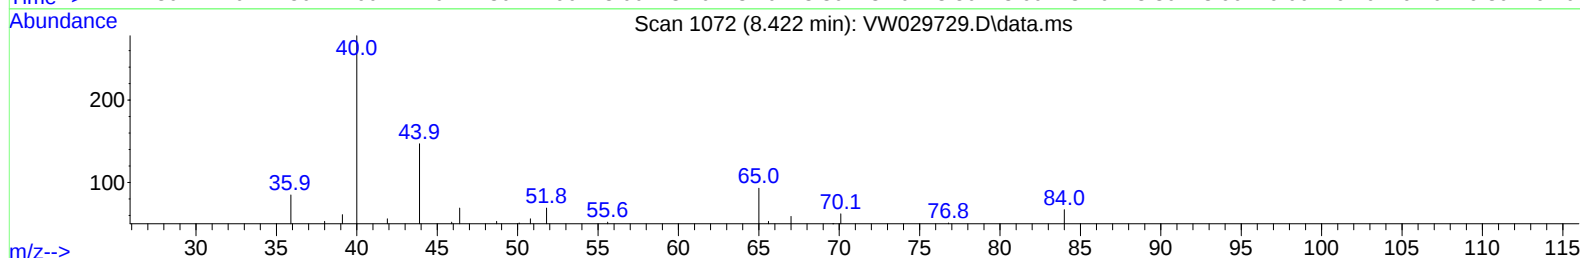


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029729.D
Acq On : 25 Jul 2024 12:13
Operator : SY/MD
Sample : P3278-07
Misc : 9.03g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jul 26 01:28:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

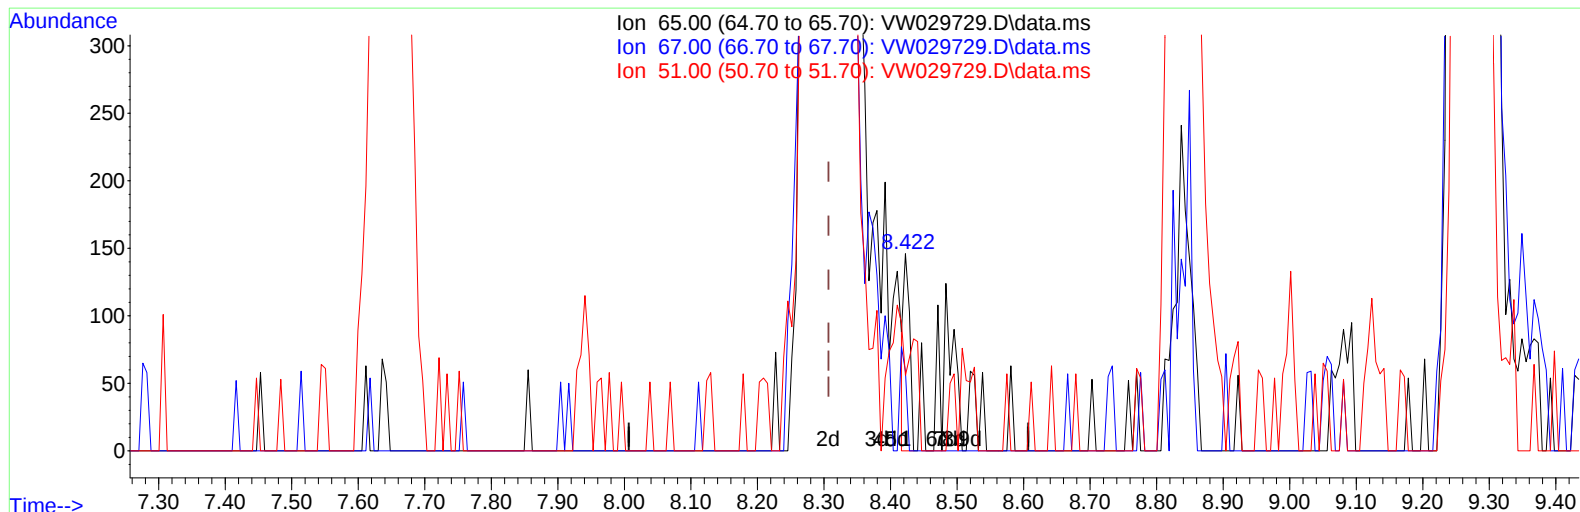

TIC: VW029729.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.422min (+ 0.115) 0.04 ug/L

response 91

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	54.95
51.00	120.50	93.41
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029729.D
Acq On : 25 Jul 2024 12:13
Operator : SY/MD
Sample : P3278-07
Misc : 9.03g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jul 26 01:28:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

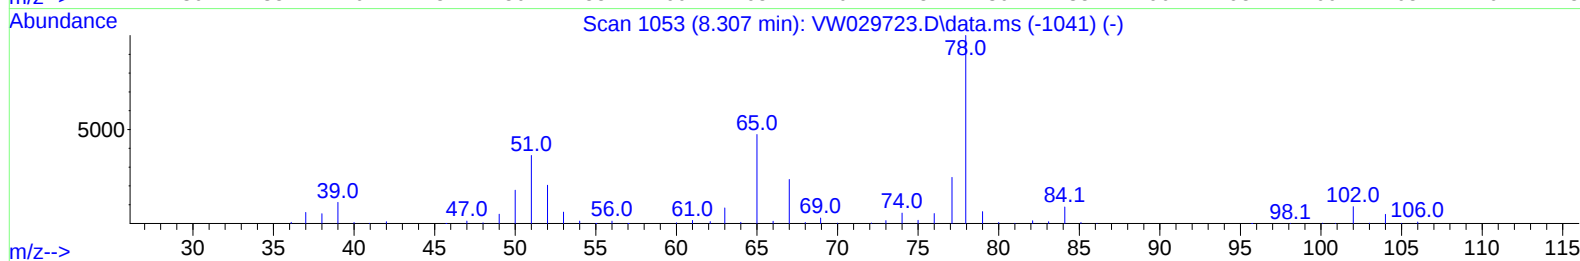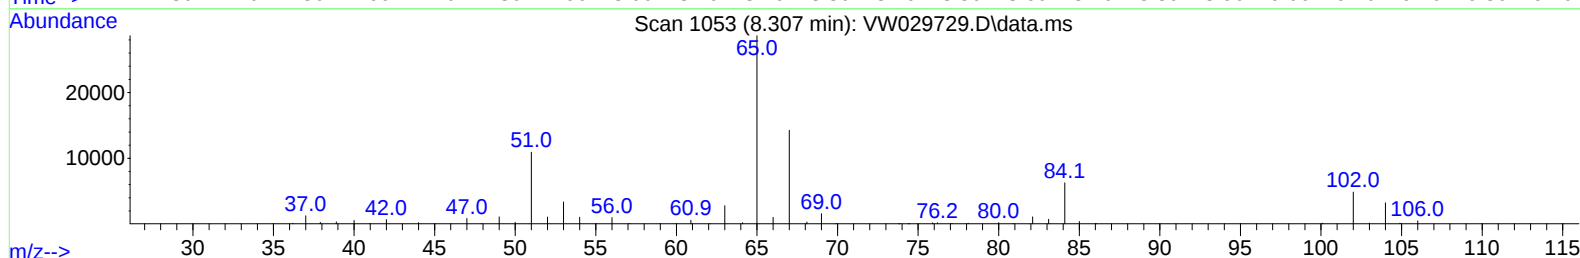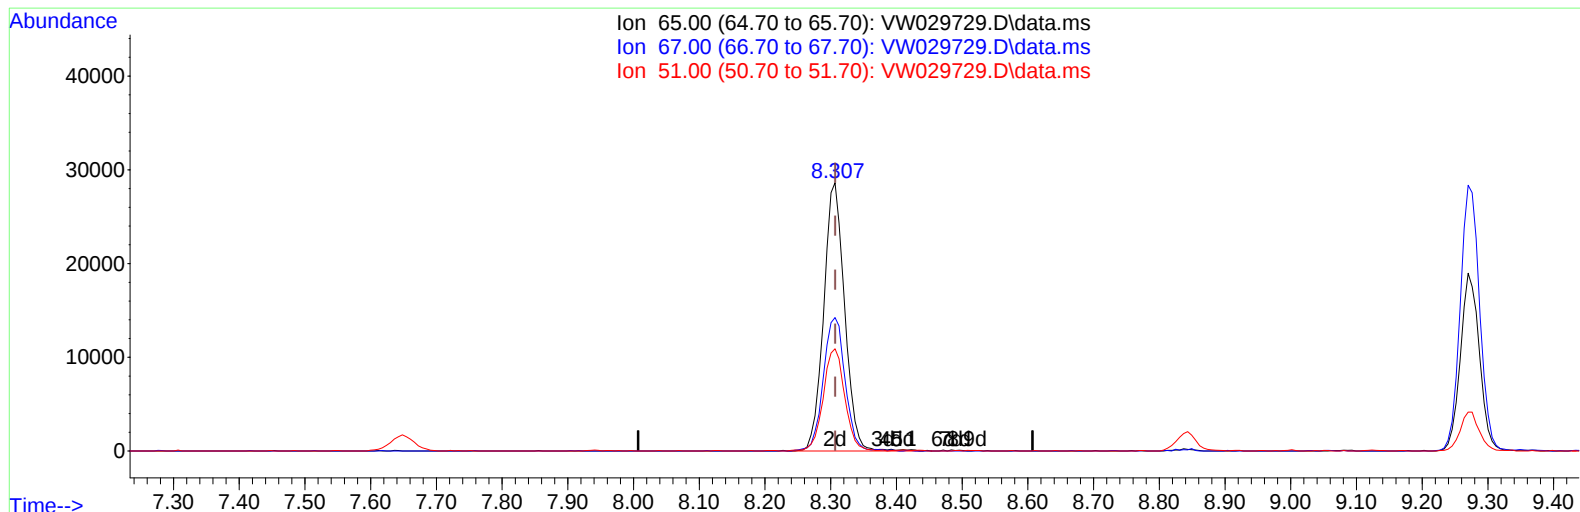

TIC: VW029729.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 26.08 ug/L m

response 63333

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.08#
51.00	120.50	0.13#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
 Data File : VW029729.D
 Acq On : 25 Jul 2024 12:13
 Operator : SY/MD
 Sample : P3278-07
 Misc : 9.03g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jul 26 01:28:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 25 01:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	164702	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	74935	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	12754	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	46310	19.806	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.240%
7) Chloroethane-d5	2.893	69	40110	24.027	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.120%
11) 1,1-Dichloroethene-d2	4.021	65	18717	17.536	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.160%
21) 2-Butanone-d5	7.081	46	57485	89.698	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	179.400%#
24) Chloroform-d	7.648	84	97793	22.937	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.760%
26) 1,2-Dichloroethane-d4	8.307	65	63333m	26.080	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.320%
32) Benzene-d6	8.276	84	151840	37.502	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	150.000%#
36) 1,2-Dichloropropane-d6	9.270	67	58115	44.952	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	179.800%#
41) Toluene-d8	10.318	98	76948	21.374	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.480%
43) trans-1,3-Dichloroprop...	10.581	79	11510	22.002	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.000%
47) 2-Hexanone-d5	10.922	63	24515	114.999	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	230.000%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	46384	48.319	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	193.280%#
66) 1,2-Dichlorobenzene-d4	13.848	152	8954	22.610	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.440%
Target Compounds						Qvalue
13) Acetone	4.143	43	8930	11.212	ug/L	98
14) Carbon disulfide	4.387	76	5705	0.762	ug/L #	91
16) Methylene chloride	4.917	84	16770	4.871	ug/L	95
34) Trichloroethene	9.093	95	1506	1.119	ug/L	94
46) Tetrachloroethene	10.867	164	574	0.587	ug/L #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029729.D
Acq On : 25 Jul 2024 12:13
Operator : SY/MD
Sample : P3278-07
Misc : 9.03g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jul 26 01:28:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

