
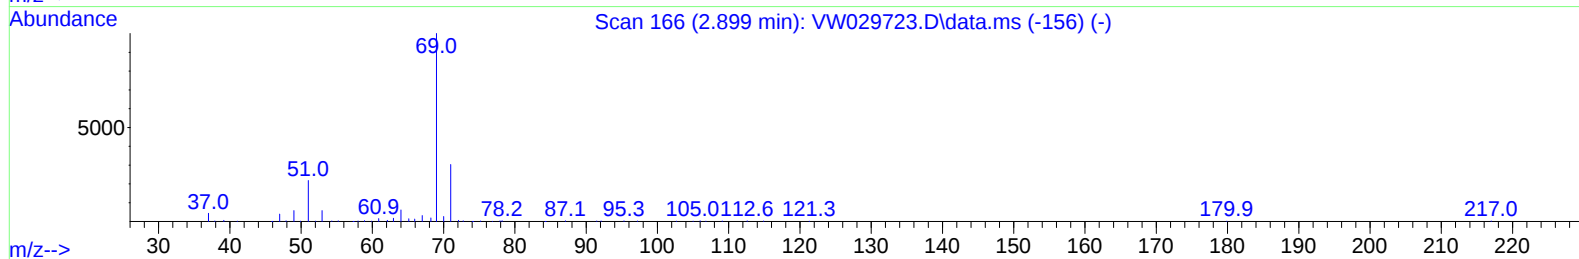
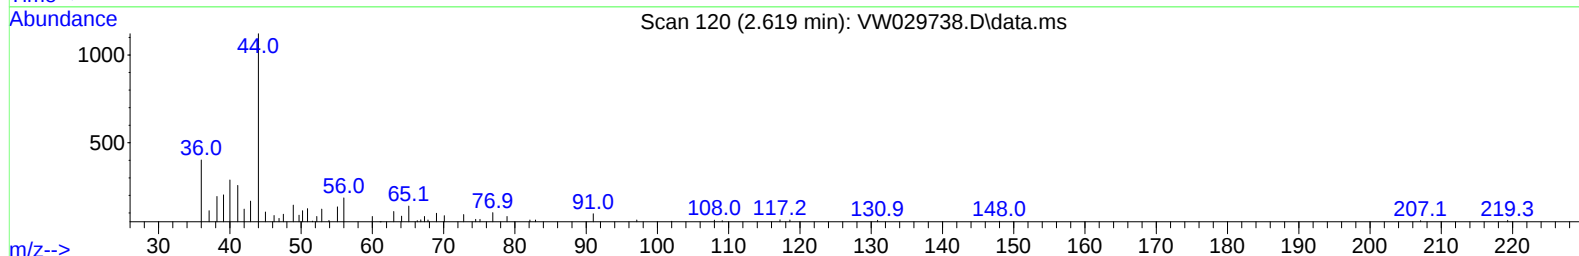


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029738.D
Acq On : 25 Jul 2024 16:23
Operator : SY/MD
Sample : P3344-10
Misc : 6.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jul 26 01:29:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

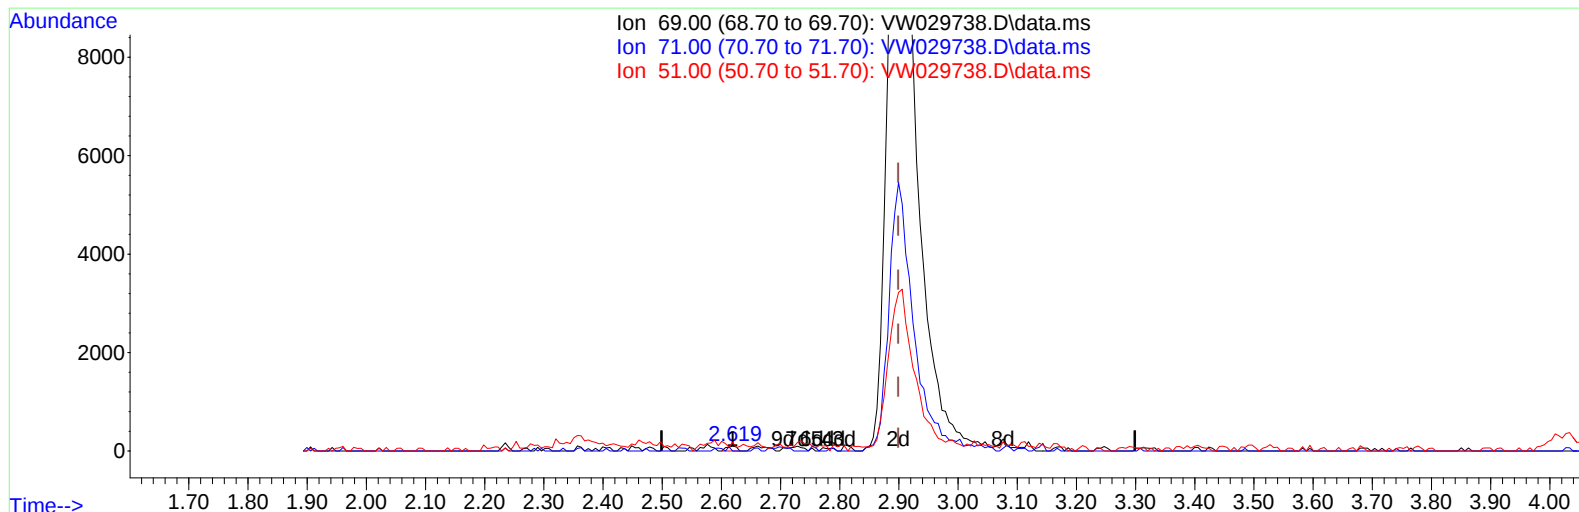

TIC: VW029738.D\data.ms




(7) Chloroethane-d5 (S)

2.619min (-0.280) 0.04 ug/L

response	121	
Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.70	26.45
51.00	31.60	38.84
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029738.D
Acq On : 25 Jul 2024 16:23
Operator : SY/MD
Sample : P3344-10
Misc : 6.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jul 26 01:29:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

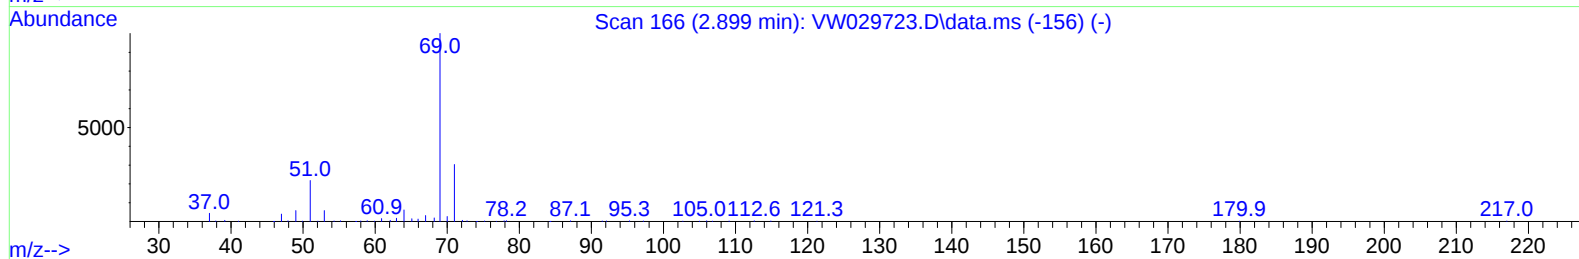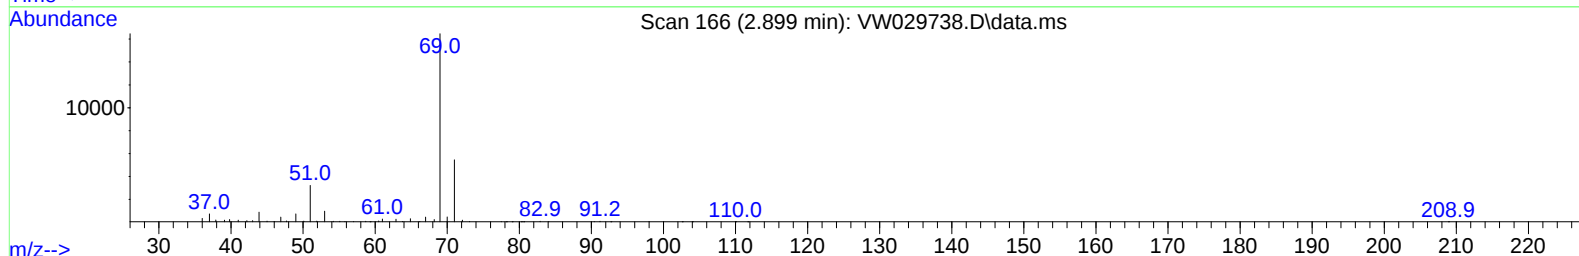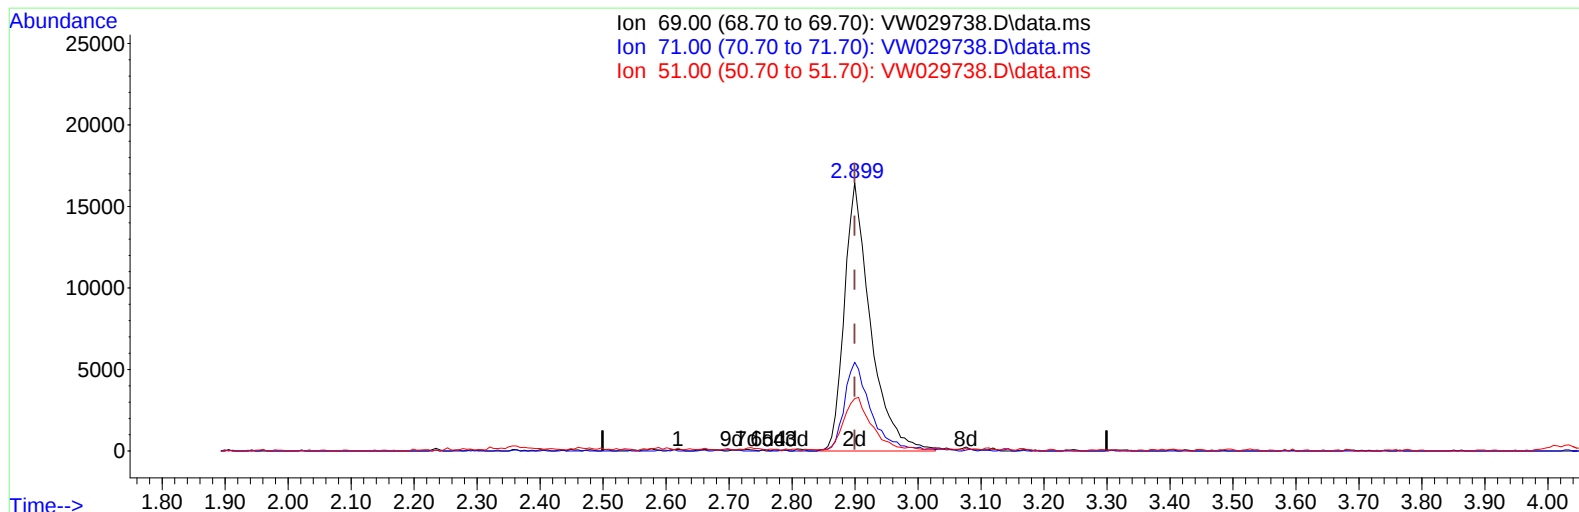

TIC: VW029738.D\data.ms

(7) Chloroethane-d5 (S)**2.899min (+ 0.000) 14.19 ug/L m****response 47557**

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.70	0.07#
51.00	31.60	0.10#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
 Data File : VW029738.D
 Acq On : 25 Jul 2024 16:23
 Operator : SY/MD
 Sample : P3344-10
 Misc : 6.01g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jul 26 01:29:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 25 01:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	330746	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	321659	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	151523	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	51616	10.993	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	43.960%
7) Chloroethane-d5	2.899	69	47557m	14.186	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.760%
11) 1,1-Dichloroethene-d2	4.027	65	26618	12.419	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.680%
21) 2-Butanone-d5	7.075	46	64246	49.921	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.840%
24) Chloroform-d	7.648	84	152802	17.847	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.400%
26) 1,2-Dichloroethane-d4	8.307	65	96932	19.877	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.520%
32) Benzene-d6	8.276	84	266759	15.349	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	61.400%
36) 1,2-Dichloropropane-d6	9.270	67	98444	17.739	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	70.960%
41) Toluene-d8	10.325	98	220889	14.294	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	57.160%
43) trans-1,3-Dichloroprop...	10.575	79	36106	16.079	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	64.320%
47) 2-Hexanone-d5	10.922	63	45135	49.325	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.640%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	96294	23.369	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.480%
66) 1,2-Dichlorobenzene-d4	13.849	152	90080	19.146	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	76.600%
Target Compounds						Qvalue
16) Methylene chloride	4.929	84	16992	2.457	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029738.D
Acq On : 25 Jul 2024 16:23
Operator : SY/MD
Sample : P3344-10
Misc : 6.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jul 26 01:29:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

