

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
 Data File : VW029724.D
 Acq On : 25 Jul 2024 10:06
 Operator : SY/MD
 Sample : VW0725SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK521

Quant Time: Jul 26 01:27:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 25 01:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	256480	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	244316	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	112980	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	75063	20.615	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.480%
7) Chloroethane-d5	2.899	69	57666	22.183	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.720%
11) 1,1-Dichloroethene-d2	4.015	65	36901	22.201	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	88.800%
21) 2-Butanone-d5	7.075	46	47752	47.848	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.700%
24) Chloroform-d	7.648	84	158387	23.856	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.440%
26) 1,2-Dichloroethane-d4	8.307	65	96074	25.405	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.640%
32) Benzene-d6	8.276	84	314985	23.861	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.440%
36) 1,2-Dichloropropane-d6	9.270	67	102946	24.423	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.680%
41) Toluene-d8	10.325	98	284024	24.198	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.800%
43) trans-1,3-Dichloroprop...	10.575	79	39610	23.223	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.880%
47) 2-Hexanone-d5	10.922	63	31672	45.569	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.140%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	75592	24.152	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	87804	25.029	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.120%
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	12573	2.345	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072524\
Data File : VW029724.D
Acq On : 25 Jul 2024 10:06
Operator : SY/MD
Sample : VW0725SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK521

Quant Time: Jul 26 01:27:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072424SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 25 01:35:38 2024
Response via : Initial Calibration

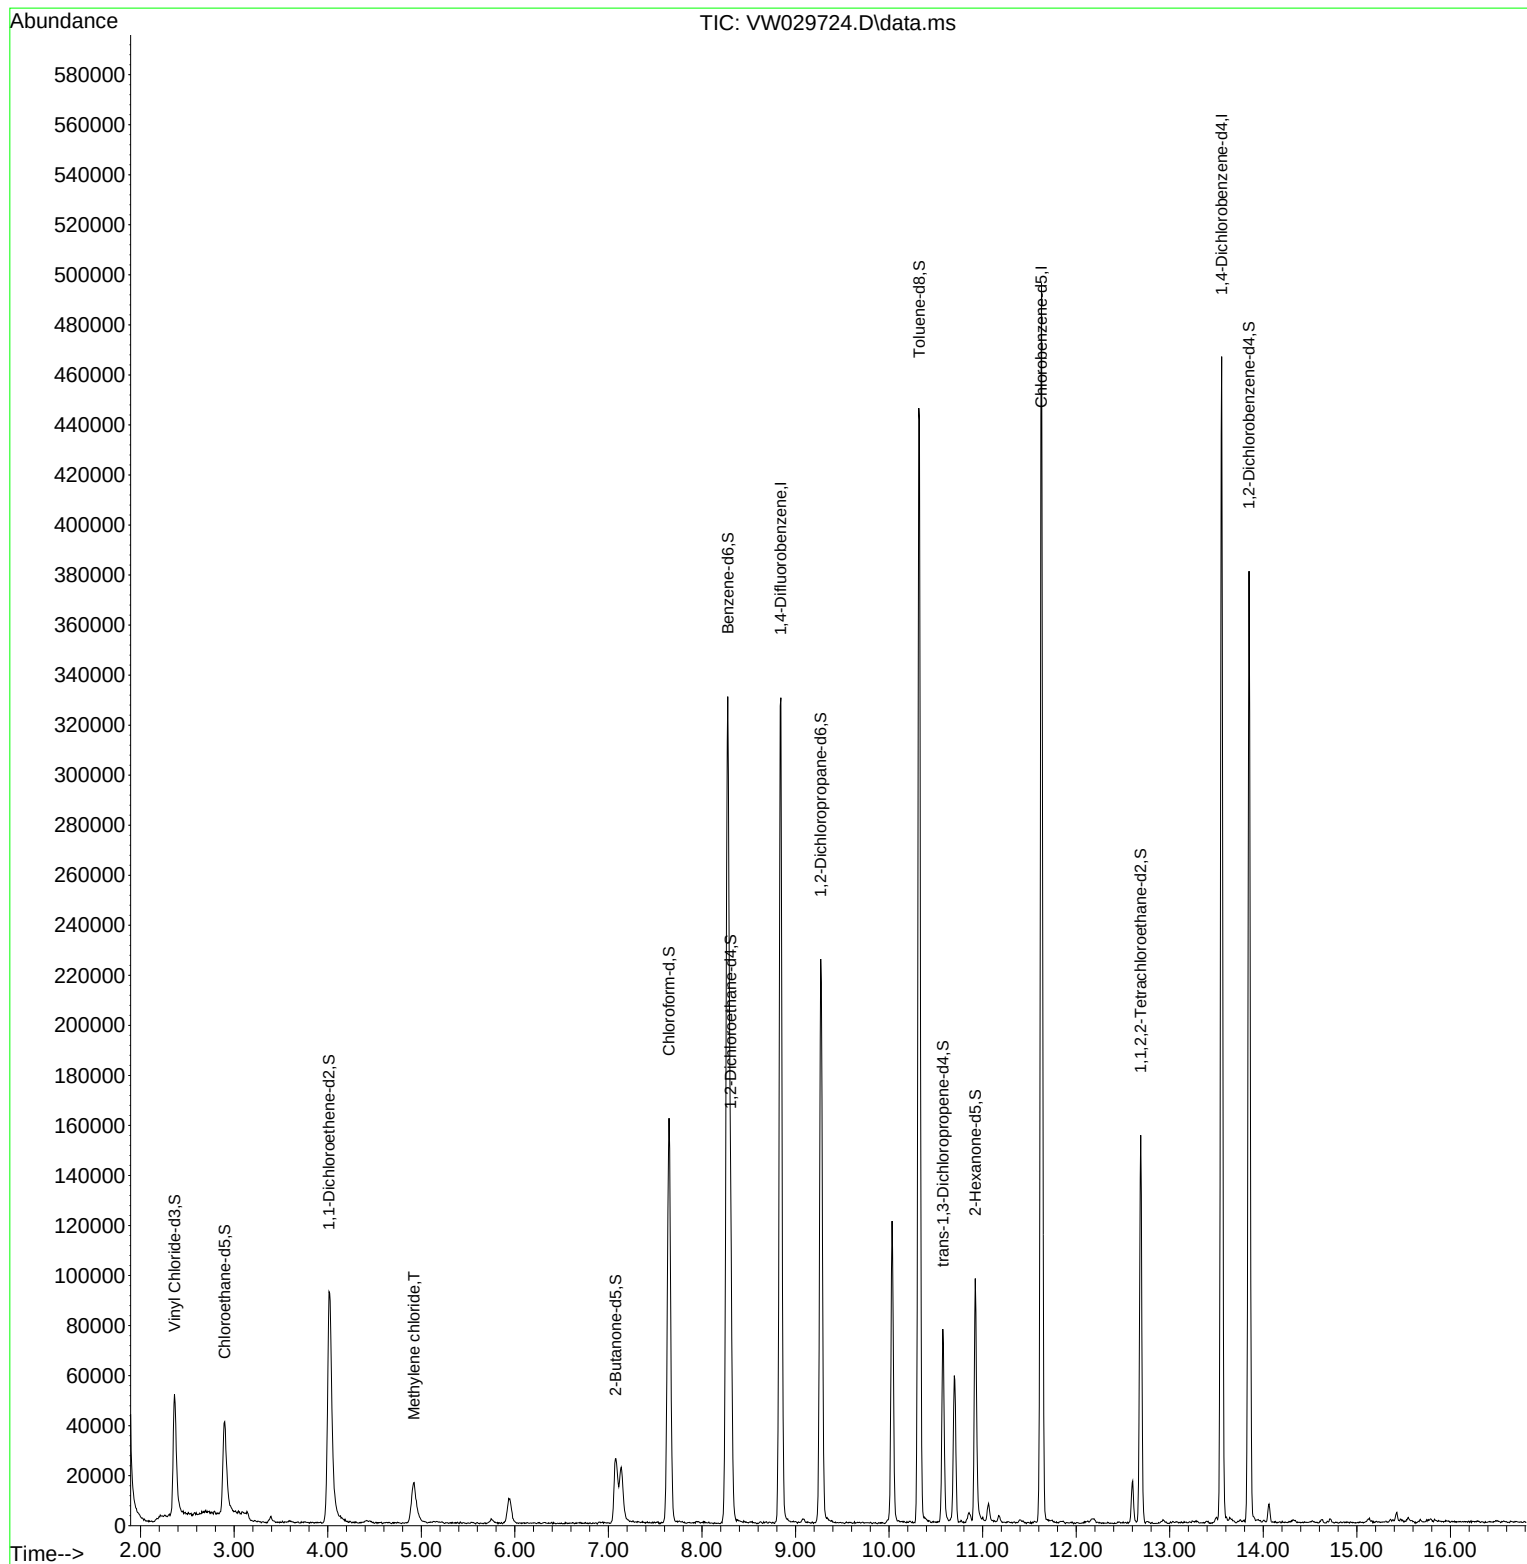

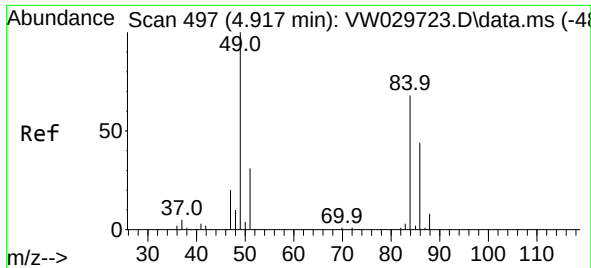

#16
Methylene chloride
Concen: 2.345 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW029724.D
Acq: 25 Jul 2024 10:06

Instrument :
MSVOA_W
ClientSampleId :
VBLK521

Tgt Ion: 84 Resp: 12573
Ion Ratio Lower Upper
84 100
86 61.6 44.7 82.9
49 134.9 99.0 184.0

