

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
 Data File : VW024089.D
 Acq On : 26 Jul 2022 10:06
 Operator : SY/VA
 Sample : N3795-06
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Jul 26 23:40:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jul 26 23:39:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	232973	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	234247	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	102283	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	131030	26.239	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.960%
7) Chloroethane-d5	2.873	69	73473	21.775	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.120%
11) 1,1-Dichloroethene-d2	4.007	63	77764	17.685	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.760%
21) 2-Butanone-d5	7.074	46	33767	38.047	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.100%
24) Chloroform-d	7.641	84	143429	22.394	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.560%
26) 1,2-Dichloroethane-d4	8.299	65	83747	22.759	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.040%
32) Benzene-d6	8.269	84	277505	25.503	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.000%
36) 1,2-Dichloropropane-d6	9.275	67	81209	23.661	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.640%
41) Toluene-d8	10.323	98	259819	23.875	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.520%
43) trans-1,3-Dichloroprop...	10.573	79	33887	22.268	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.080%
47) 2-Hexanone-d5	10.921	63	28614	39.878	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.760%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	73597	18.584	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	74.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	85783	25.897	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.600%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	3526	0.707	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072622\
Data File : VW024089.D
Acq On : 26 Jul 2022 10:06
Operator : SY/VA
Sample : N3795-06
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Jul 26 23:40:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM072522SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jul 26 23:39:35 2022
Response via : Initial Calibration

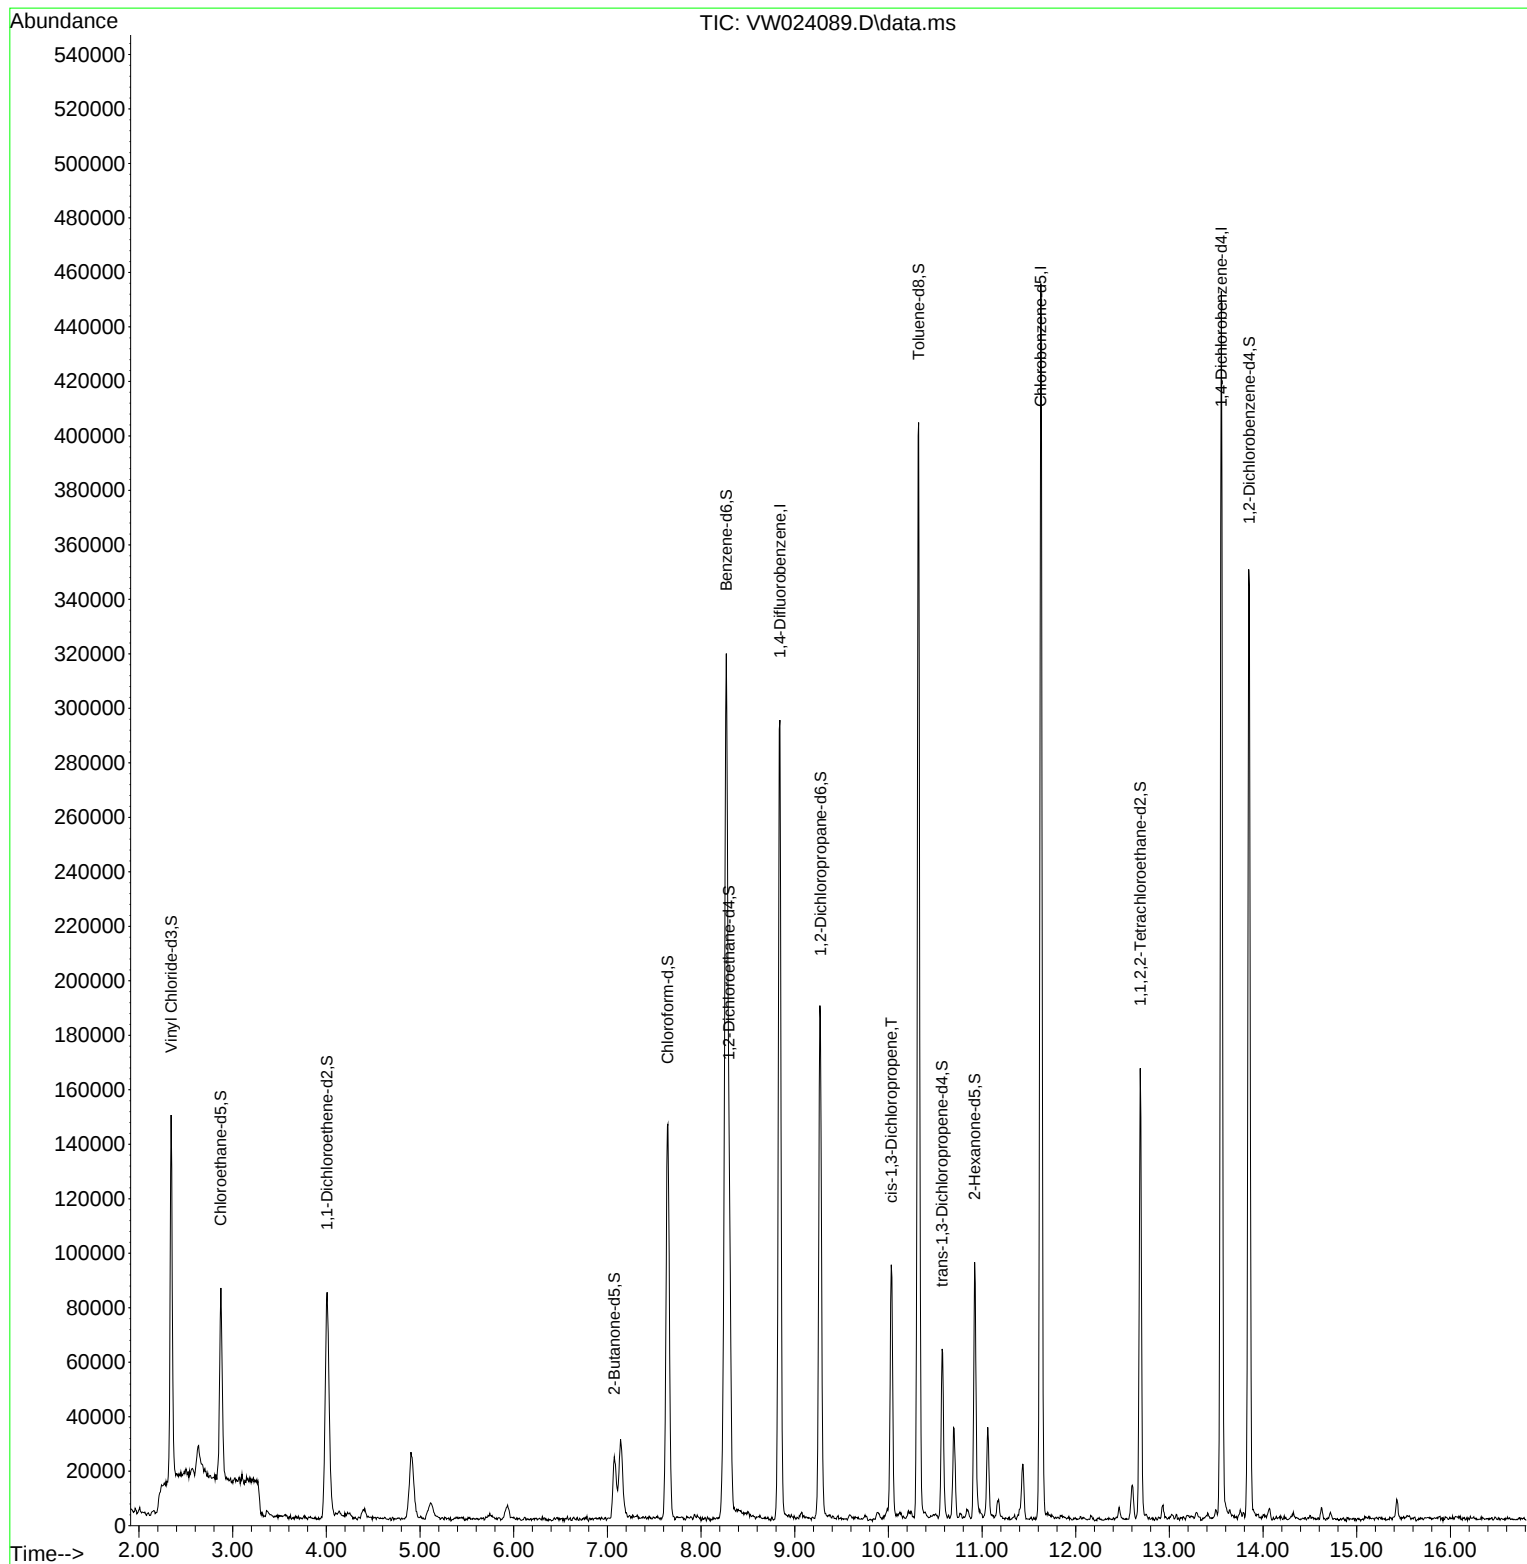

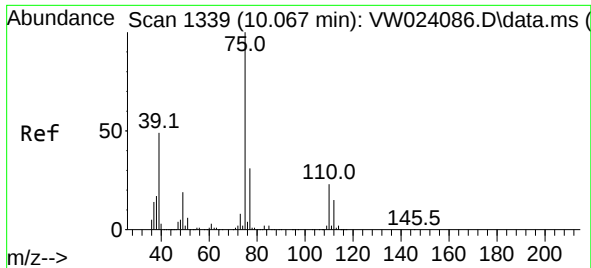

#39
 cis-1,3-Dichloropropene
 Concen: 0.707 ug/L
 RT: 10.030 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW024089.D
 Acq: 26 Jul 2022 10:06

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 3526
 Ion Ratio Lower Upper
 75 100
 77 36.0 21.8 40.6

